

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030620\
Data File : FB023804.D
Signal(s) : FID2B.CH
Acq On : 6 Mar 2020 12:51
Operator : DD/AJ
Sample : L1753-02
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 06 22:14:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	420675	19.984 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.667	4014	0.130 ng/ml
3) t n-Heptane	7.751	3428	0.103 ng/ml
6) t Toluene	10.639	16382	0.402 ng/ml
7) t Ethylbenzene	13.067	2342	0.061 ng/ml
8) t m-Xylene	13.208	9269	0.252 ng/ml
9) t O-Xylene	13.941	1624	0.046 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030620\
Data File : FB023804.D
Signal(s) : FID2B.CH
Acq On : 6 Mar 2020 12:51
Operator : DD/AJ
Sample : L1753-02
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 06 22:14:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

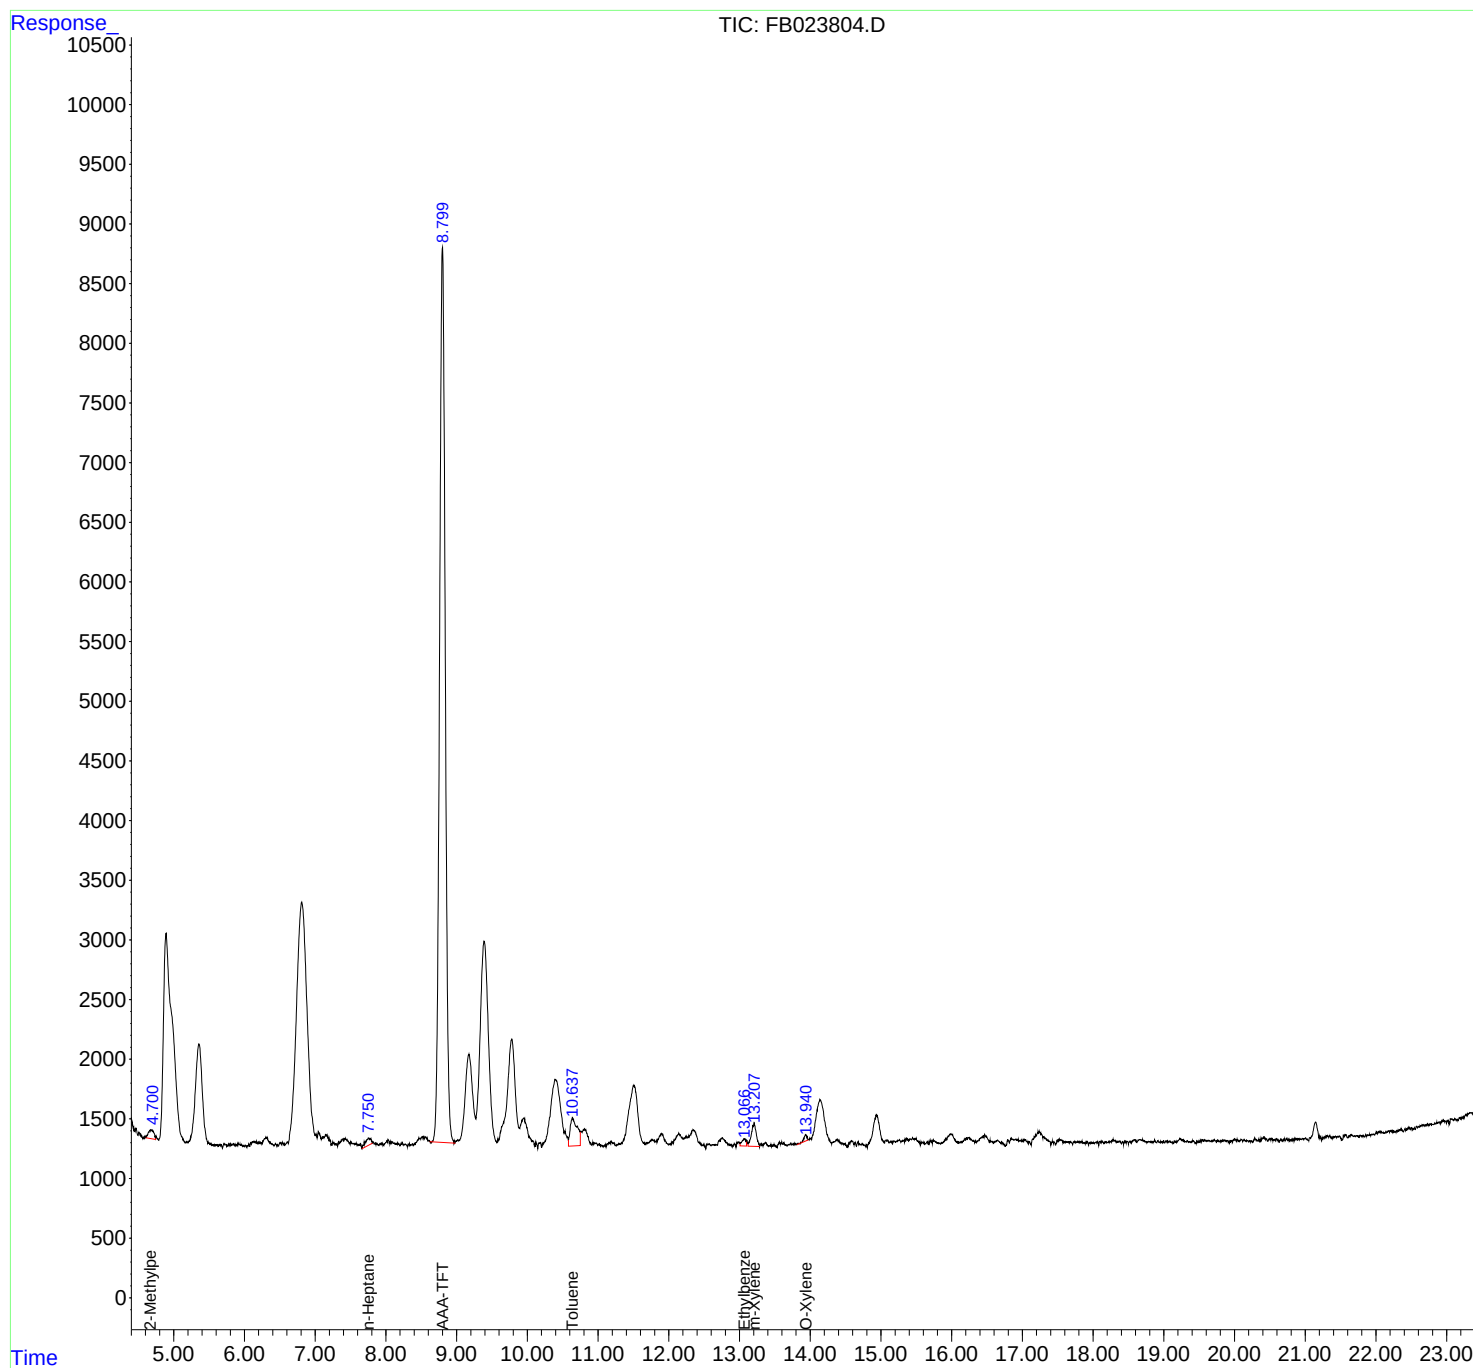

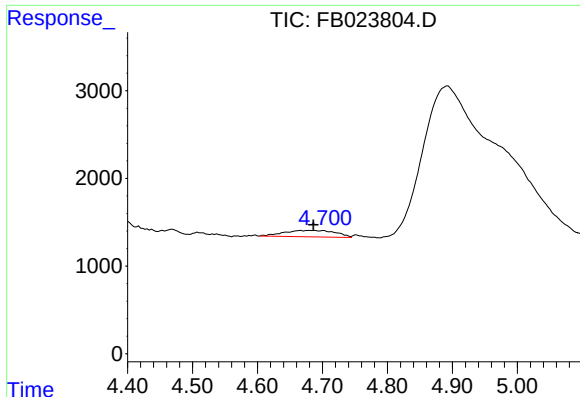


#1 2-Methylpentane

R.T.: 4.667 min
Delta R.T.: -0.019 min
Response: 4014
Conc: 0.13 ng/ml

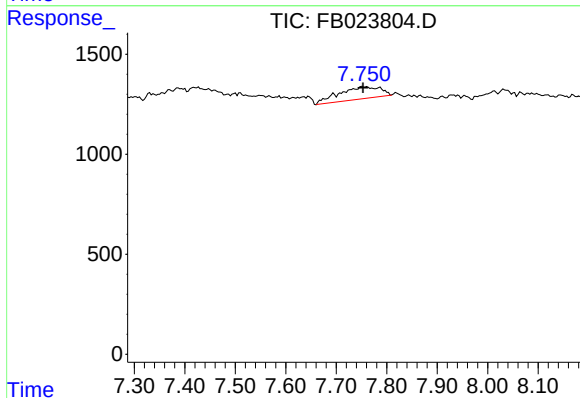


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.002 min
Response: 3428
Conc: 0.10 ng/ml

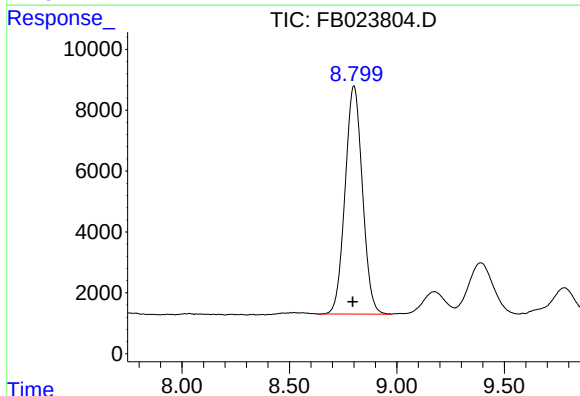


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.006 min
Response: 420675
Conc: 19.98 ng/ml

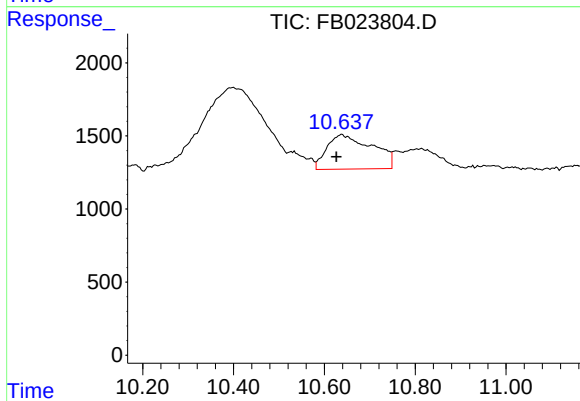


#6 Toluene

R.T.: 10.639 min
Delta R.T.: 0.012 min
Response: 16382
Conc: 0.40 ng/ml

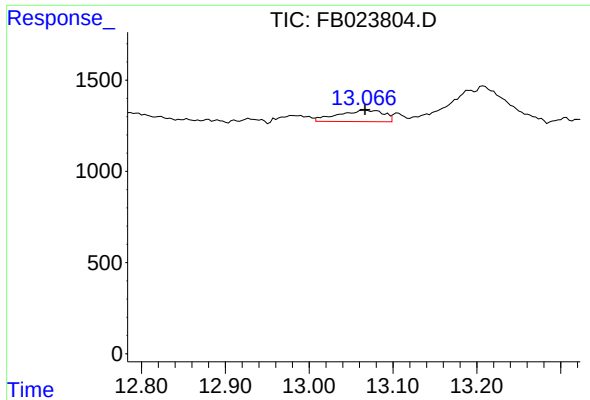


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.000 min
Response: 2342
Conc: 0.06 ng/ml

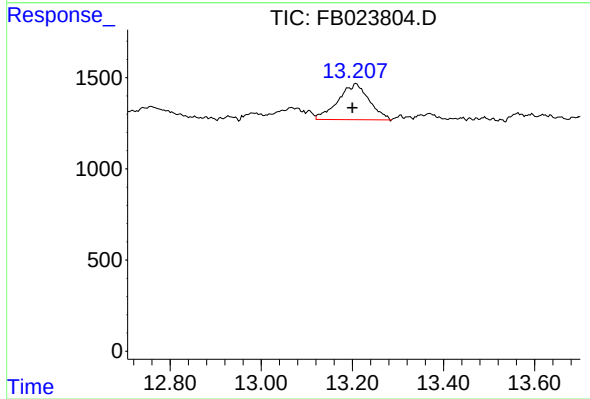

#8 m-Xylene

R.T.: 13.208 min
Delta R.T.: 0.009 min
Response: 9269
Conc: 0.25 ng/ml

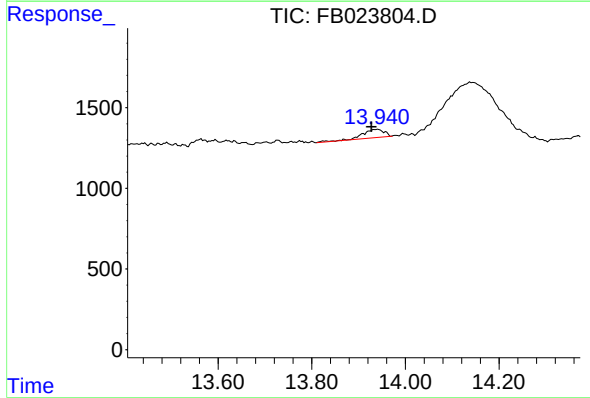

#9 O-Xylene

R.T.: 13.941 min
Delta R.T.: 0.013 min
Response: 1624
Conc: 0.05 ng/ml