

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030623\
 Data File : FB029409.D
 Signal(s) : FID2B.CH
 Acq On : 6 Mar 2023 11:07
 Operator : YP/AJ
 Sample : BSF0306S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0306S1

Integration File: Calibration.e
 Quant Time: Mar 07 02:24:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	234401	19.347 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	506740	33.025 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	533855	31.693 ng/ml
3) t n-Heptane	7.746	189478	10.955 ng/ml
4) t Benzene	7.882	219345	10.806 ng/ml
6) t Toluene	10.614	653827	33.124 ng/ml
7) t Ethylbenzene	13.050	206672	11.101 ng/ml
8) t m-Xylene	13.184	408302	21.948 ng/ml
9) t O-Xylene	13.910	396834	21.552 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	397596	21.347 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030623\
Data File : FB029409.D
Signal(s) : FID2B.CH
Acq On : 6 Mar 2023 11:07
Operator : YP/AJ
Sample : BSF0306S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0306S1

Integration File: Calibration.e
Quant Time: Mar 07 02:24:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

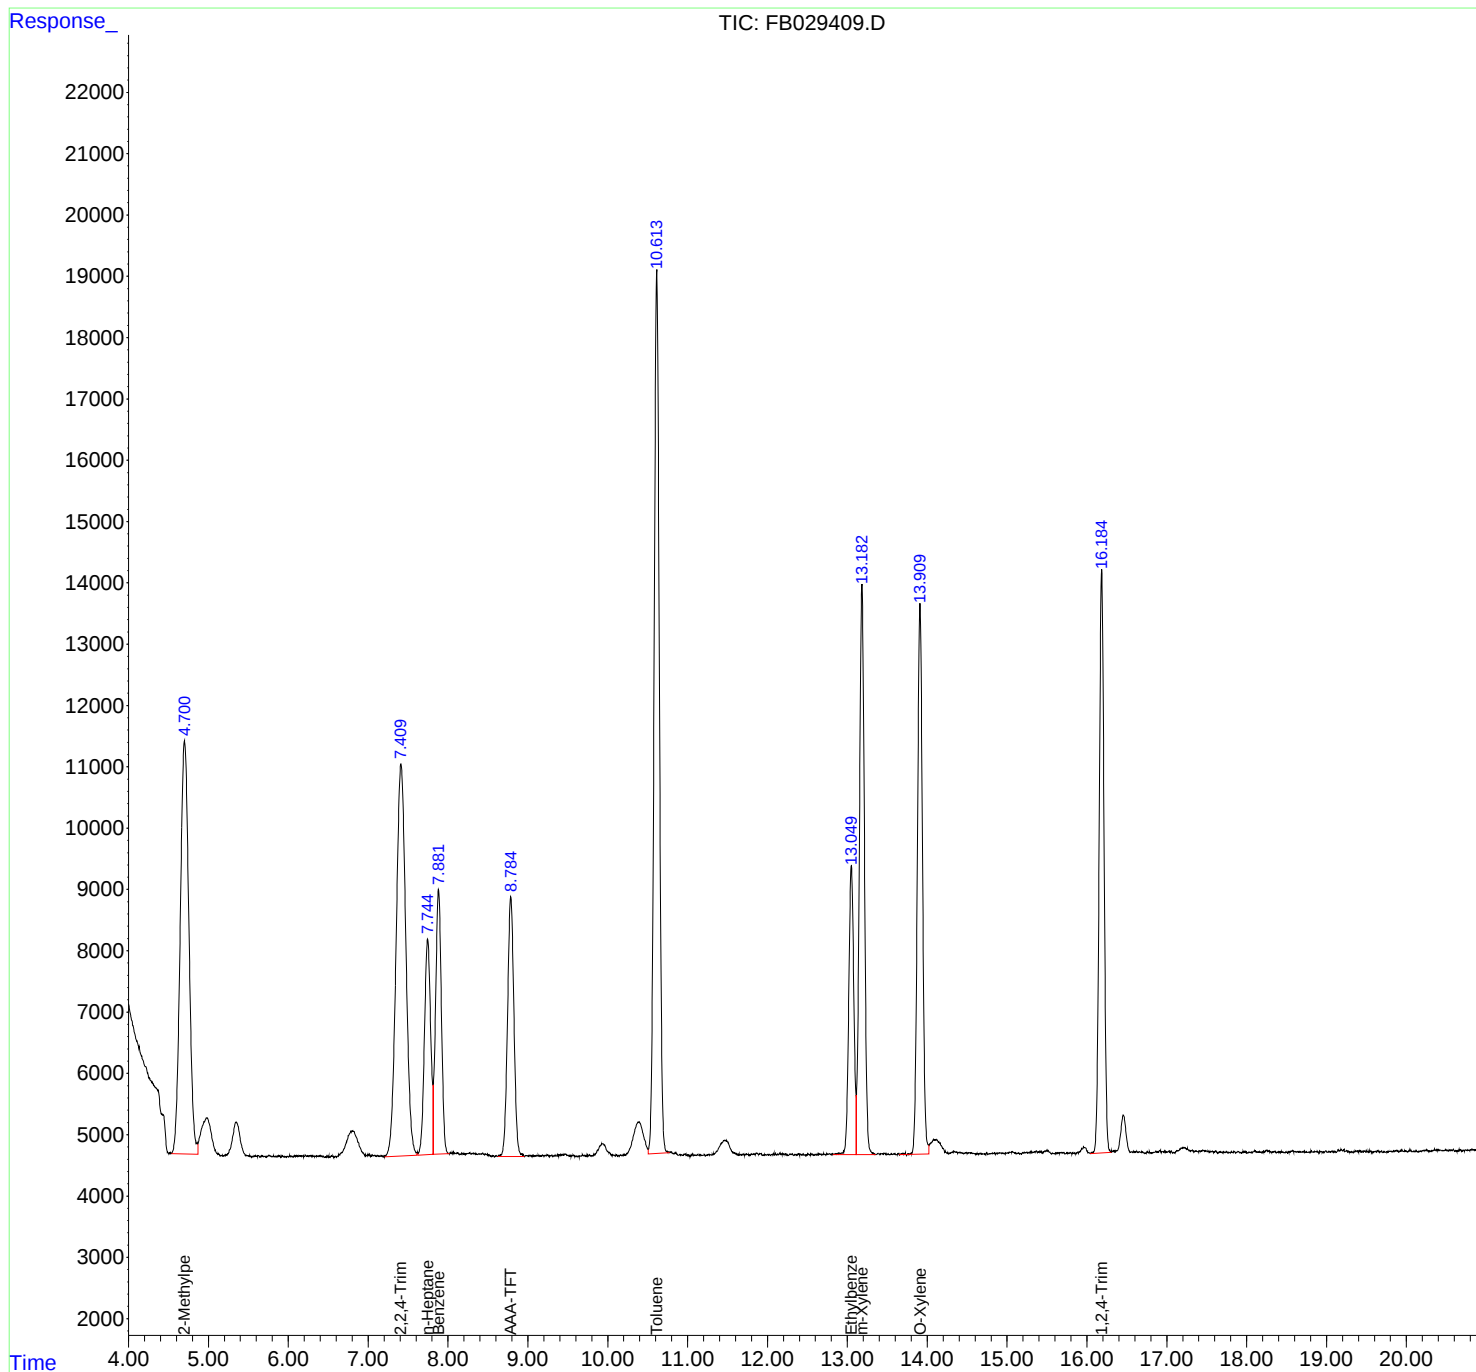


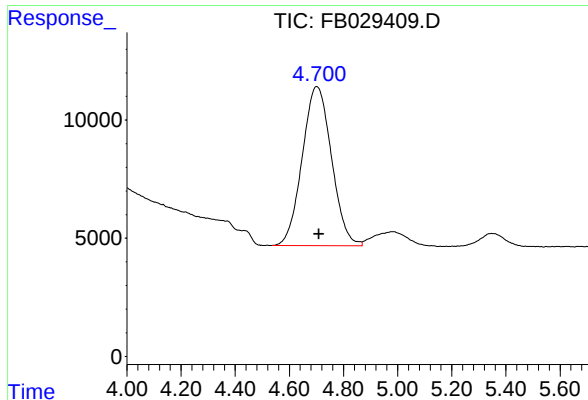

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.009 min
Response: 506740
Conc: 33.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0306S1

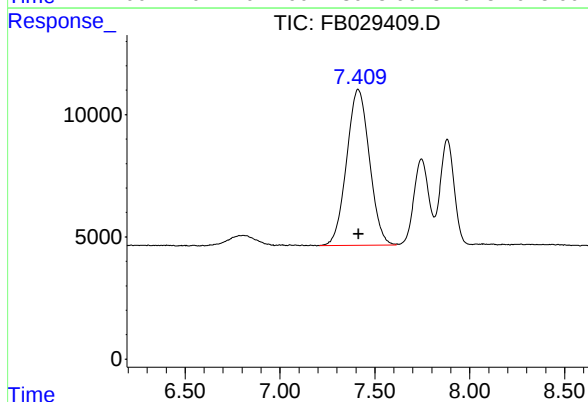


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.005 min
Response: 533855
Conc: 31.69 ng/ml

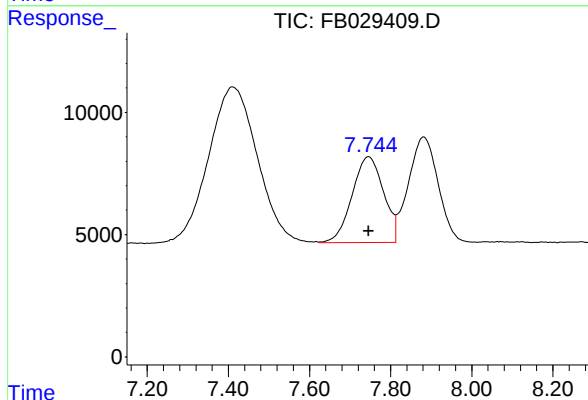


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 189478
Conc: 10.96 ng/ml

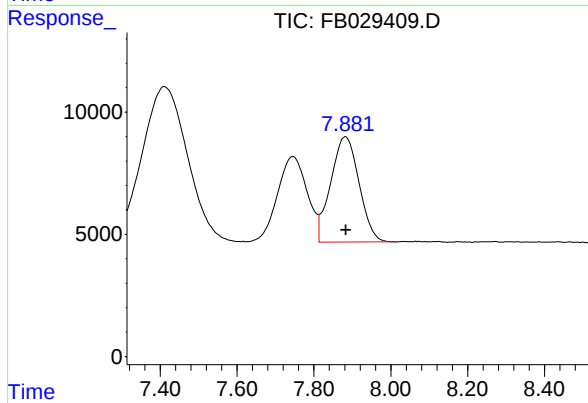

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.001 min
Response: 219345
Conc: 10.81 ng/ml

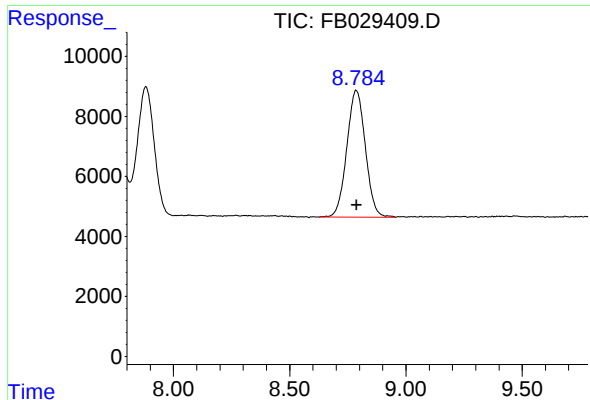

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.002 min
Response: 234401
Conc: 19.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0306S1

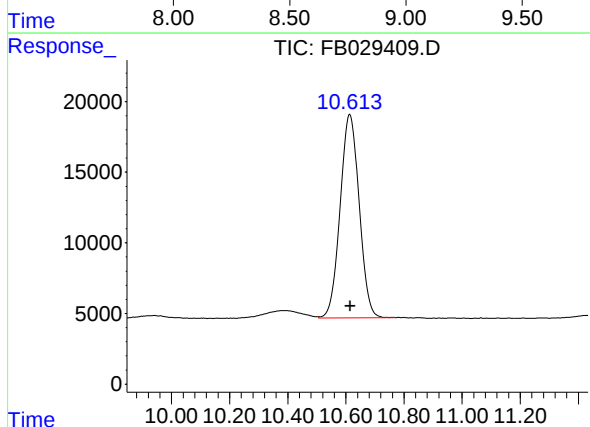


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.002 min
Response: 653827
Conc: 33.12 ng/ml

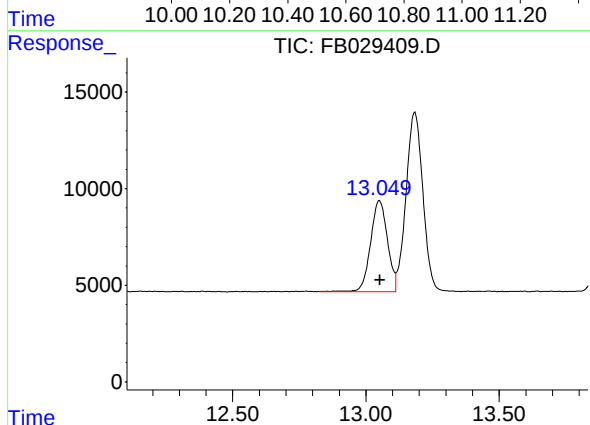


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.002 min
Response: 206672
Conc: 11.10 ng/ml

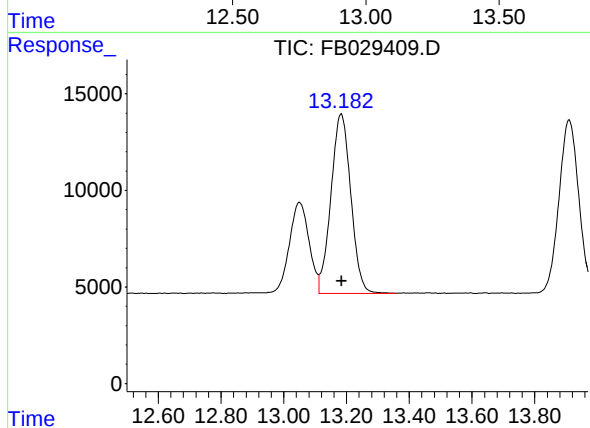

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: -0.001 min
Response: 408302
Conc: 21.95 ng/ml

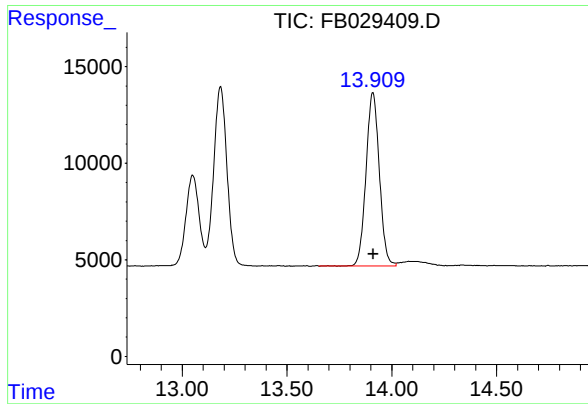

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.002 min
Response: 396834
Conc: 21.55 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0306S1

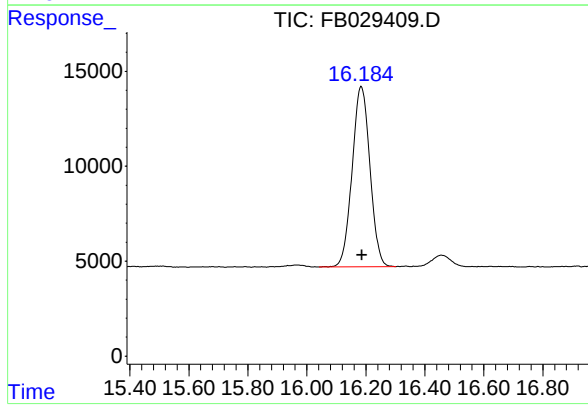

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.002 min
Response: 397596
Conc: 21.35 ng/ml