

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030623\
 Data File : FB029411.D
 Signal(s) : FID2B.CH
 Acq On : 6 Mar 2023 12:51
 Operator : YP/AJ
 Sample : BSF0306S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0306S2

Integration File: Calibration.e
 Quant Time: Mar 07 02:24:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	224854	18.559 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	431152	28.099 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	448468	26.624 ng/ml
3) t n-Heptane	7.746	164501	9.511 ng/ml
4) t Benzene	7.882	186534	9.190 ng/ml
6) t Toluene	10.616	548893	27.808 ng/ml
7) t Ethylbenzene	13.051	171815	9.229 ng/ml
8) t m-Xylene	13.185	340672	18.312 ng/ml
9) t O-Xylene	13.911	329834	17.913 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	327697	17.594 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030623\
Data File : FB029411.D
Signal(s) : FID2B.CH
Acq On : 6 Mar 2023 12:51
Operator : YP/AJ
Sample : BSF0306S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0306S2

Integration File: Calibration.e
Quant Time: Mar 07 02:24:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

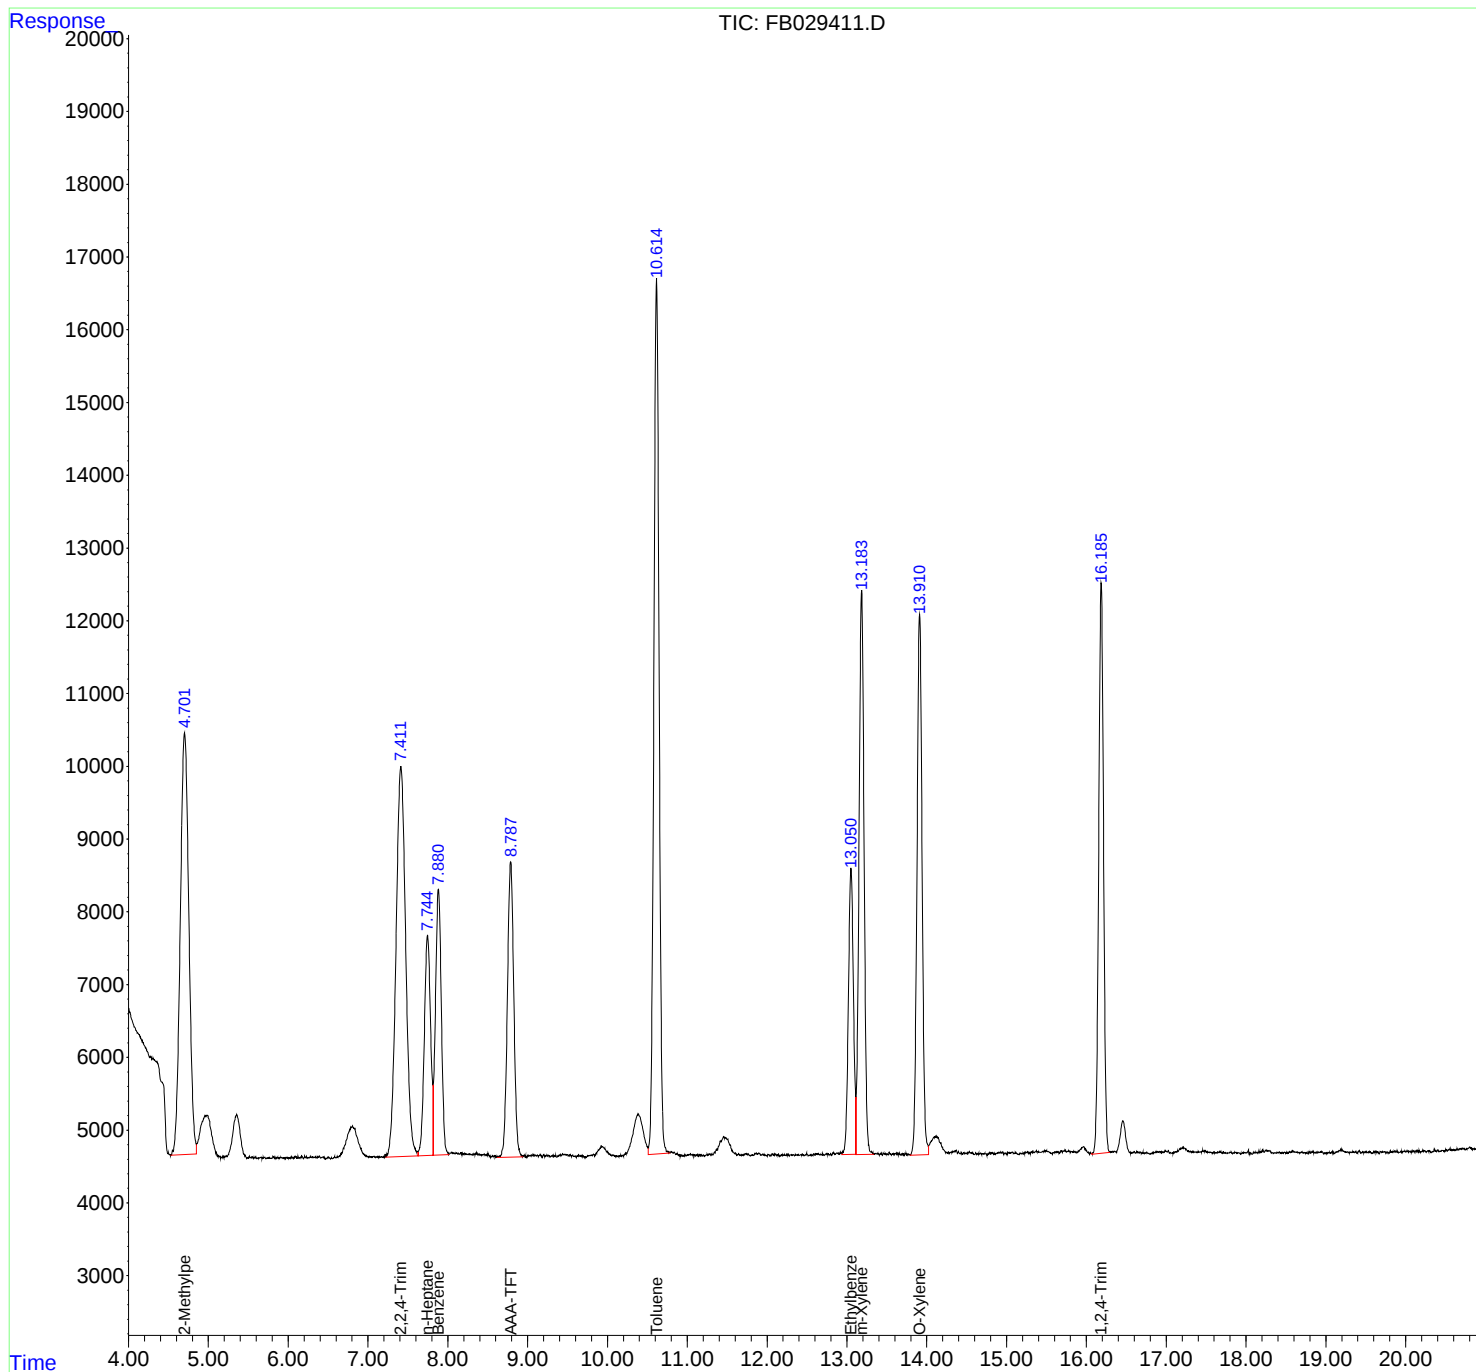


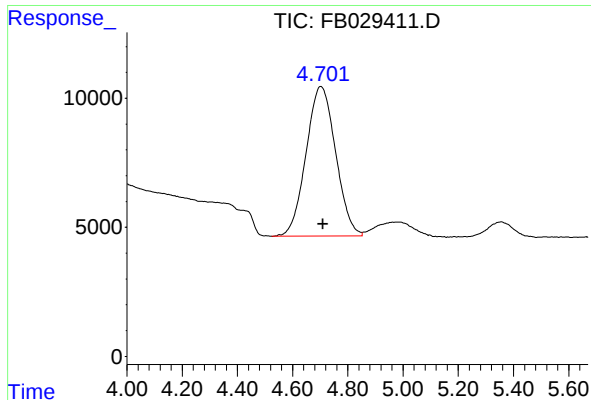

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.008 min
Response: 431152
Conc: 28.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0306S2

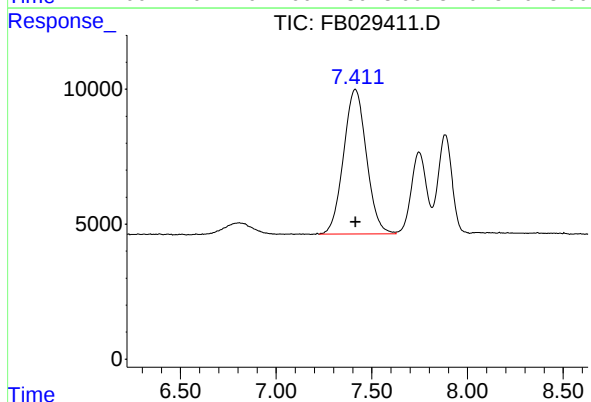


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.003 min
Response: 448468
Conc: 26.62 ng/ml

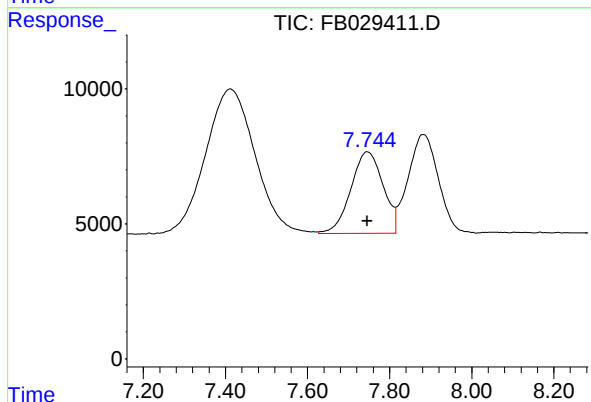


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: 0.000 min
Response: 164501
Conc: 9.51 ng/ml

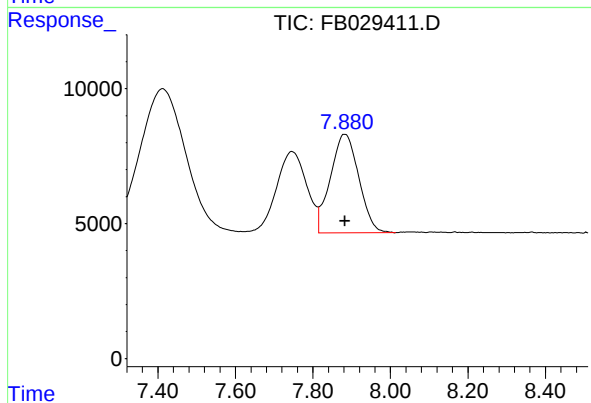

#4 Benzene


R.T.: 7.882 min
Delta R.T.: 0.000 min
Response: 186534
Conc: 9.19 ng/ml

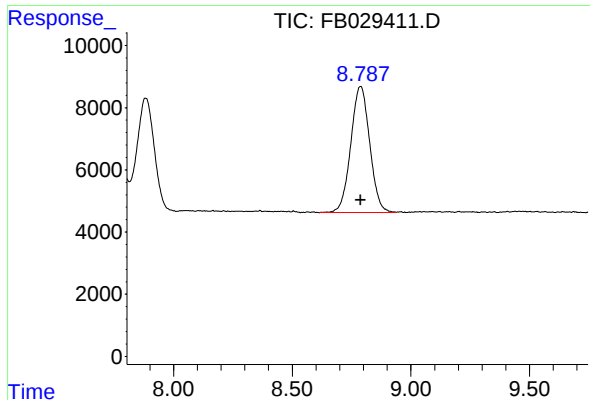

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 224854
Conc: 18.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0306S2

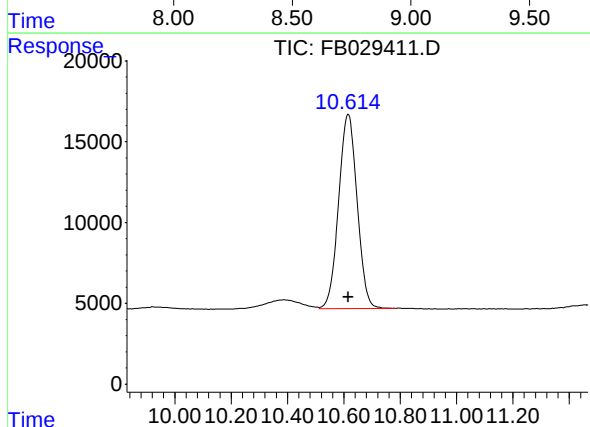


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.000 min
Response: 548893
Conc: 27.81 ng/ml

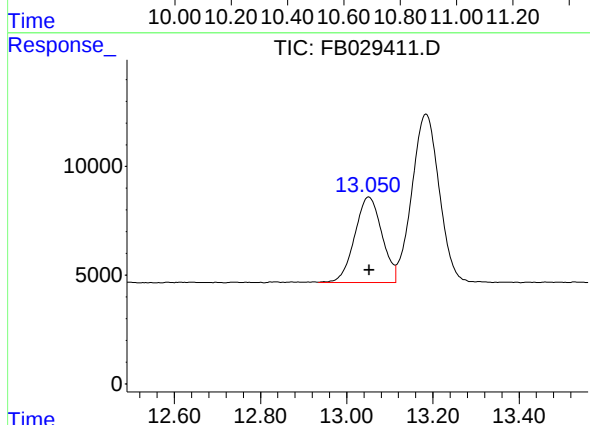


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.001 min
Response: 171815
Conc: 9.23 ng/ml

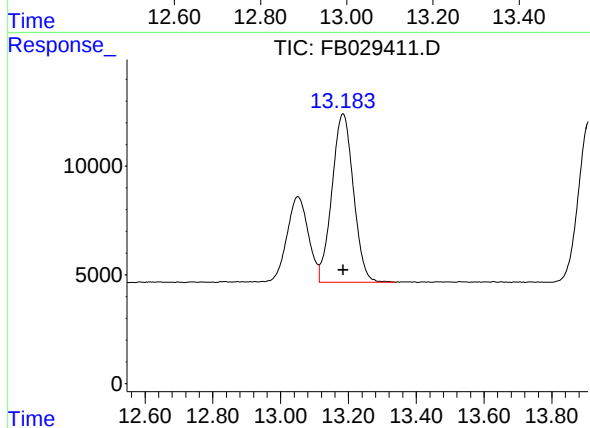

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 340672
Conc: 18.31 ng/ml

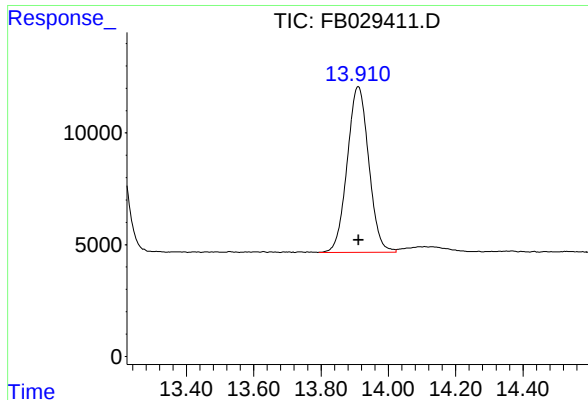

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.001 min
Response: 329834
Conc: 17.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0306S2

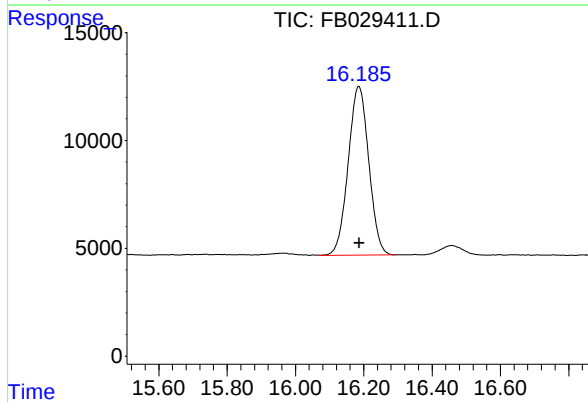

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: 0.000 min
Response: 327697
Conc: 17.59 ng/ml