

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030719\
 Data File : FB020084.D
 Signal(s) : FID2B.CH
 Acq On : 7 Mar 2019 9:35
 Operator : MJ/SJ
 Sample : BSF0307S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Mar 08 02:32:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.036	238557	21.288 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.900	498529	23.961 ng/ml
2) t	2,2,4-Trimethylpentane	7.661	539875	26.816 ng/ml
3) t	n-Heptane	7.992	171955	9.219 ng/ml
4) t	Benzene	8.131	191667	9.143 ng/ml
6) t	Toluene	10.883	598736	31.592 ng/ml
7) t	Ethylbenzene	13.334	231964	10.213 ng/ml
8) t	m-Xylene	13.467	467739	19.948 ng/ml
9) t	O-Xylene	14.199	462168	19.849 ng/ml
10) t	1,2,4-Trimethylbenzene	16.485	429339	18.647 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030719\
Data File : FB020084.D
Signal(s) : FID2B.CH
Acq On : 7 Mar 2019 9:35
Operator : MJ/SJ
Sample : BSF0307S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Mar 08 02:32:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

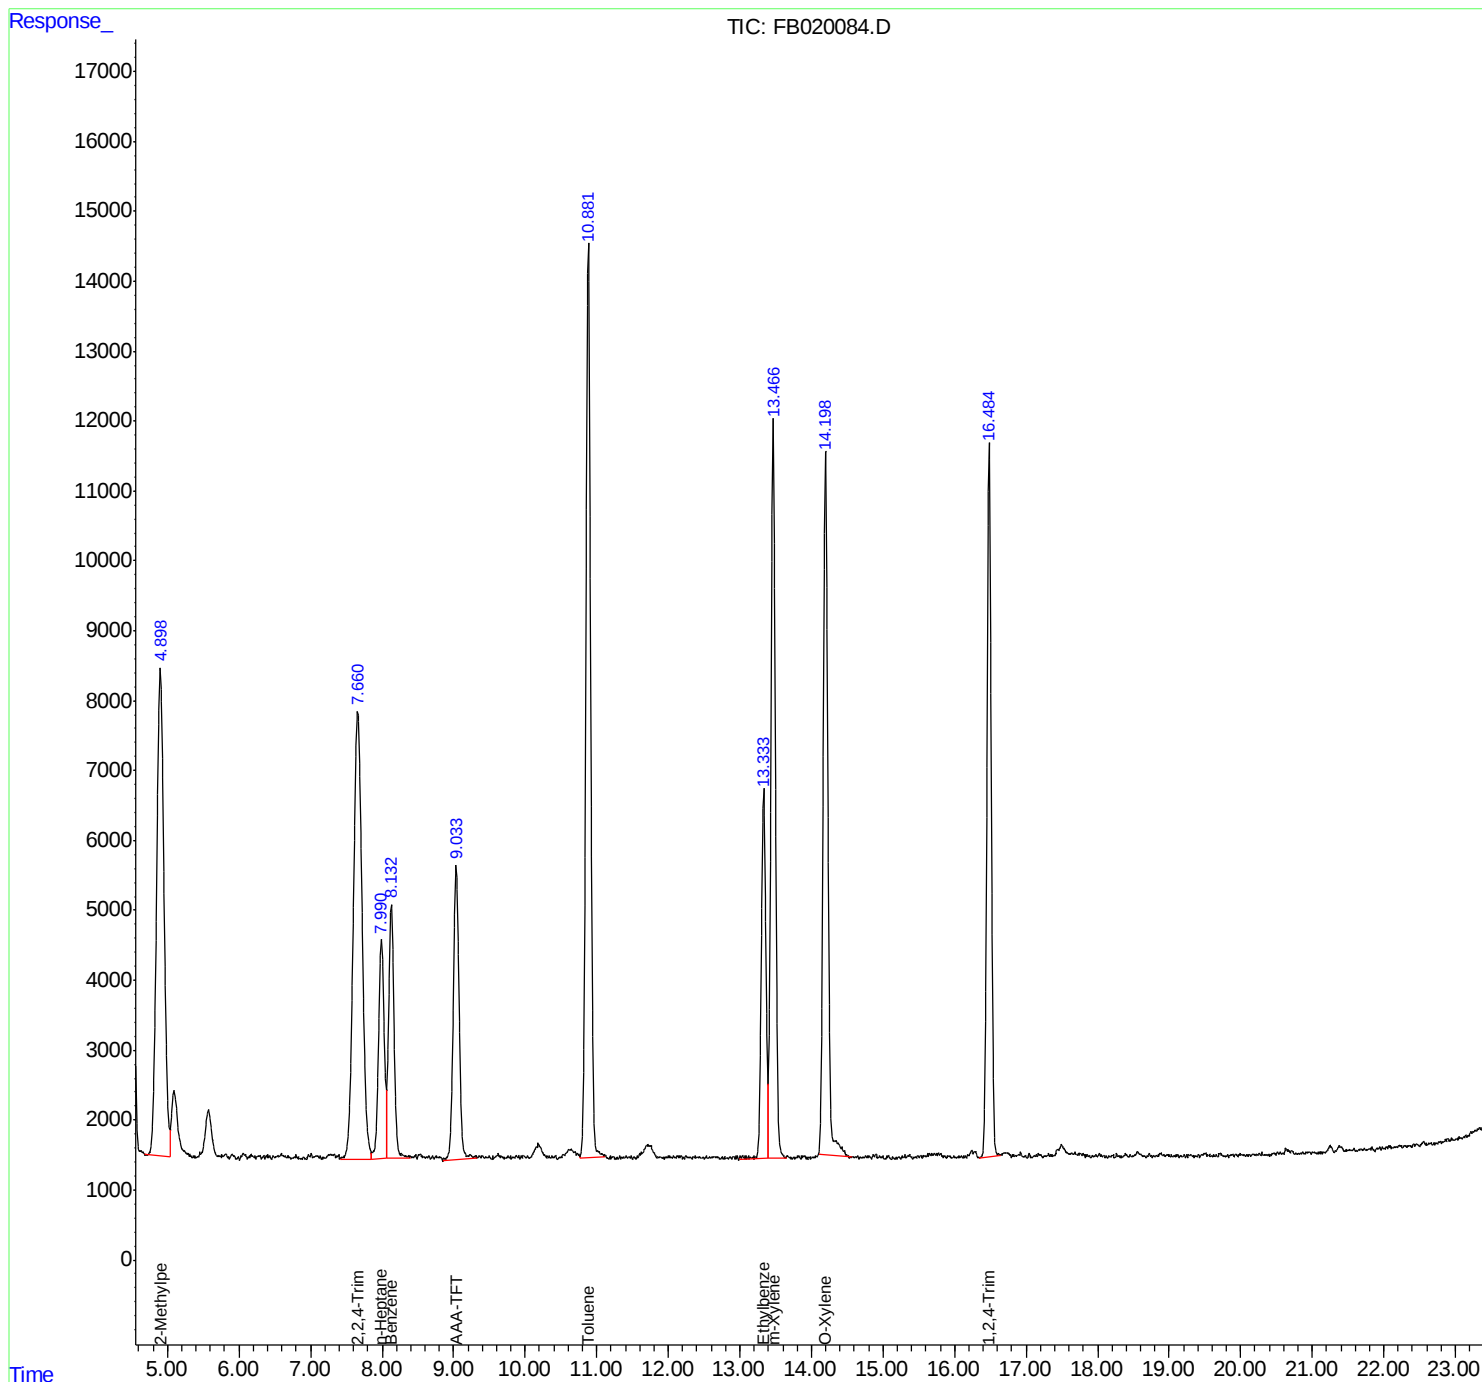

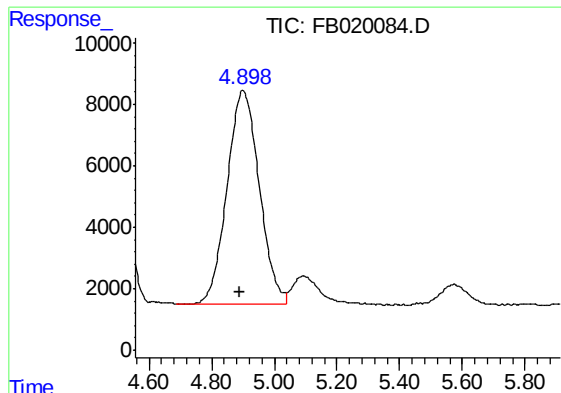


#1 2-Methylpentane

R.T.: 4.900 min
Delta R.T.: 0.009 min
Response: 498529
Conc: 23.96 ng/ml

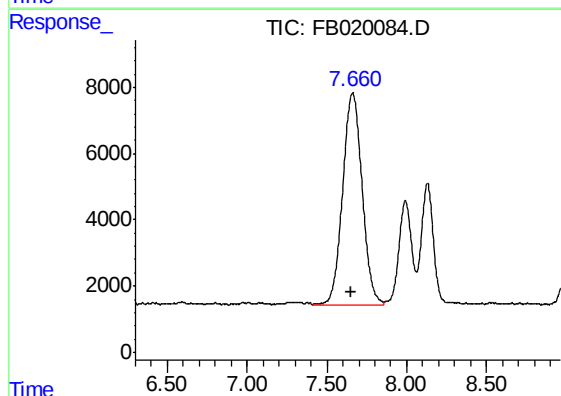


#2 2,2,4-Trimethylpentane

R.T.: 7.661 min
Delta R.T.: 0.009 min
Response: 539875
Conc: 26.82 ng/ml

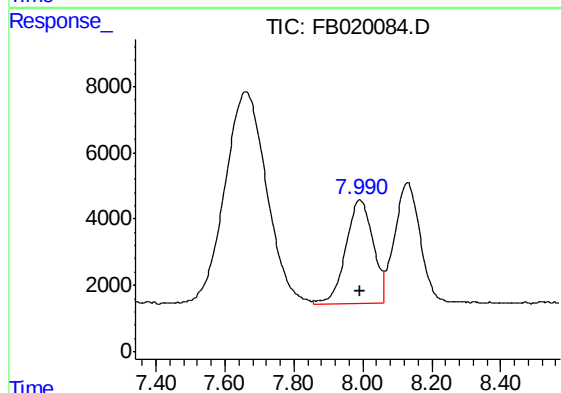


#3 n-Heptane

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 171955
Conc: 9.22 ng/ml

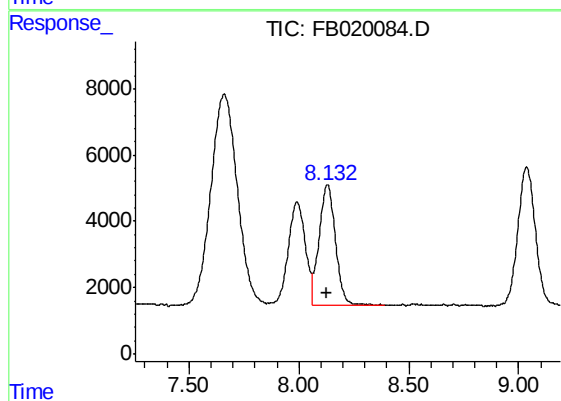


#4 Benzene

R.T.: 8.131 min
Delta R.T.: 0.002 min
Response: 191667
Conc: 9.14 ng/ml

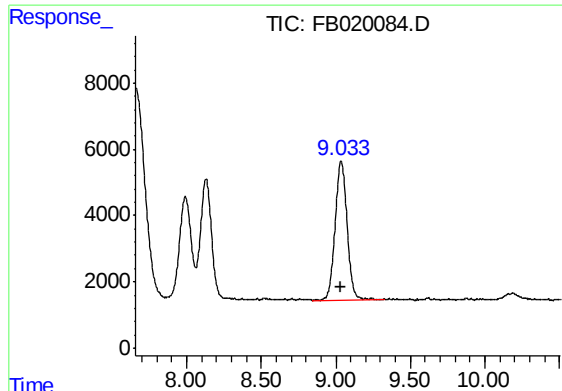


#5 AAA-TFT

R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 238557
Conc: 21.29 ng/ml

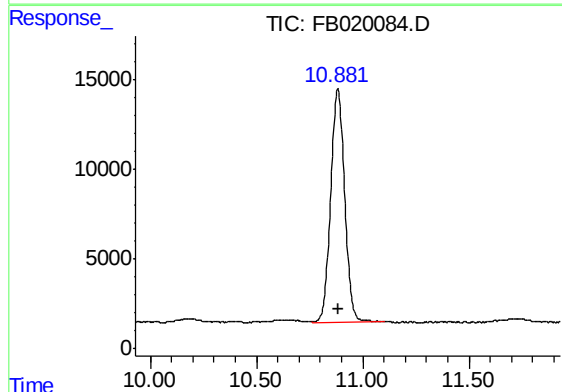


#6 Toluene

R.T.: 10.883 min
Delta R.T.: -0.001 min
Response: 598736
Conc: 31.59 ng/ml

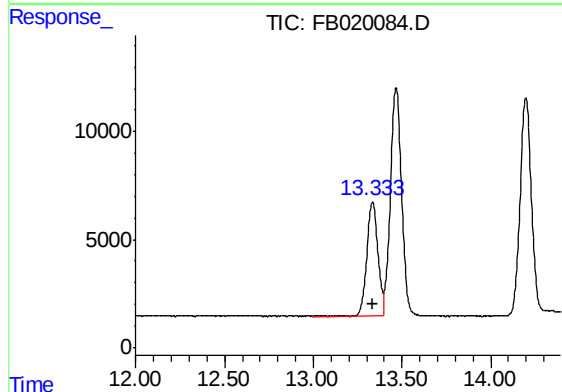


#7 Ethylbenzene

R.T.: 13.334 min
Delta R.T.: -0.002 min
Response: 231964
Conc: 10.21 ng/ml

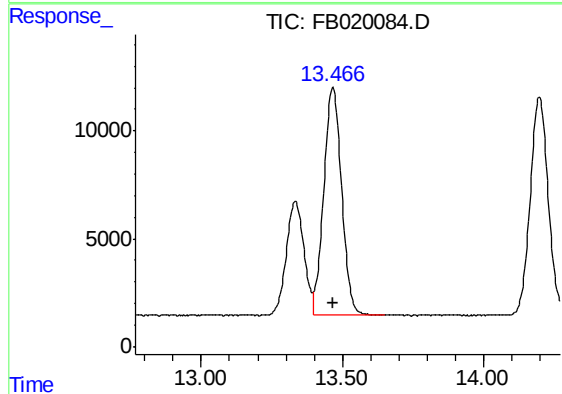


#8 m-Xylene

R.T.: 13.467 min
Delta R.T.: -0.002 min
Response: 467739
Conc: 19.95 ng/ml

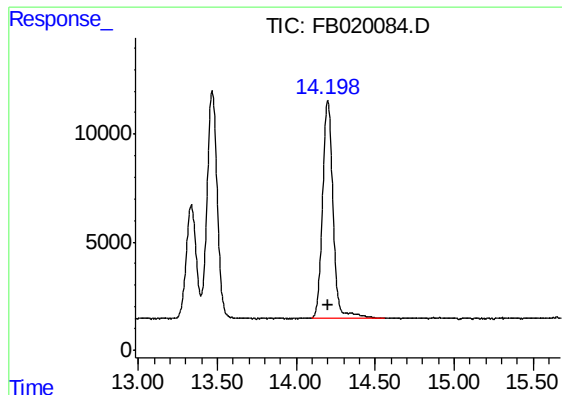

#9 O-Xylene

R.T.: 14.199 min
Delta R.T.: -0.002 min
Response: 462168
Conc: 19.85 ng/ml

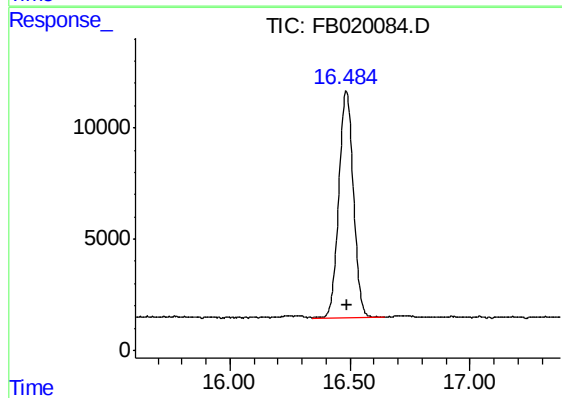

#10 1,2,4-Trimethylbenzene

R.T.: 16.485 min
Delta R.T.: -0.002 min
Response: 429339
Conc: 18.65 ng/ml