

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030719\
 Data File : FB020088.D
 Signal(s) : FID2B.CH
 Acq On : 7 Mar 2019 11:33
 Operator : MJ/SJ
 Sample : K1760-01MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Mar 08 02:33:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	232239	20.724 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.903	459033	22.062 ng/ml
2) t 2,2,4-Trimethylpentane	7.661	447143	22.210 ng/ml
3) t n-Heptane	7.994	143296	7.683 ng/ml
4) t Benzene	8.131	186920	8.917 ng/ml
6) t Toluene	10.884	582455	30.733 ng/ml
7) t Ethylbenzene	13.336	215196	9.475 ng/ml
8) t m-Xylene	13.469	439370	18.738 ng/ml
9) t O-Xylene	14.201	424096	18.214 ng/ml
10) t 1,2,4-Trimethylbenzene	16.487	396218	17.209 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030719\
Data File : FB020088.D
Signal(s) : FID2B.CH
Acq On : 7 Mar 2019 11:33
Operator : MJ/SJ
Sample : K1760-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Mar 08 02:33:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

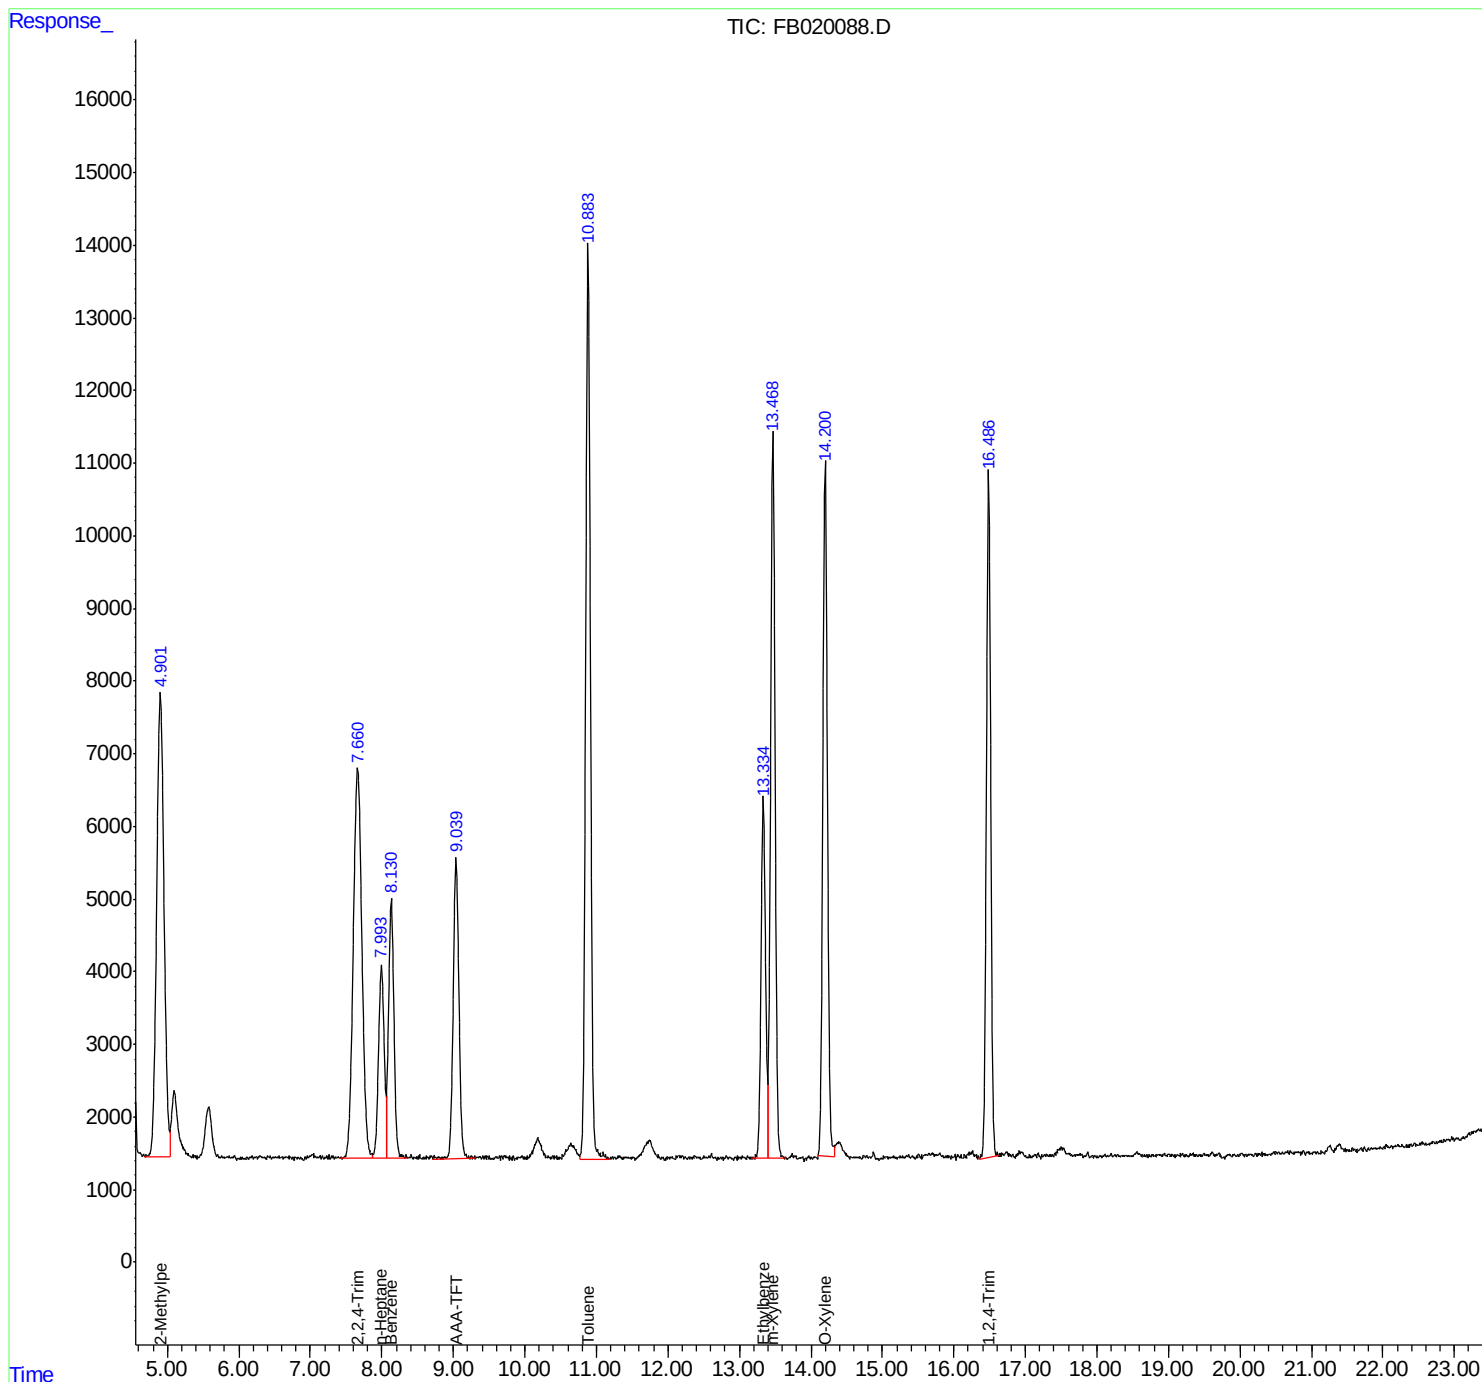

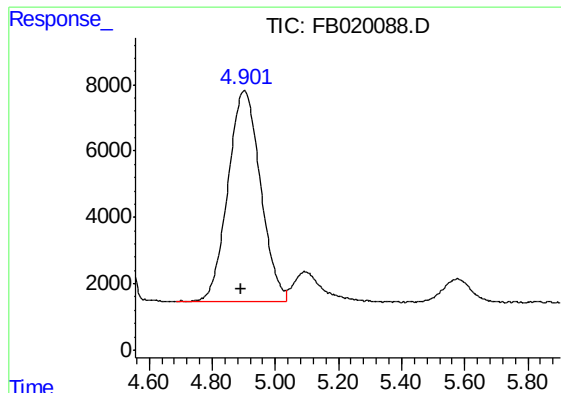


#1 2-Methylpentane

R.T.: 4.903 min
Delta R.T.: 0.012 min
Response: 459033
Conc: 22.06 ng/ml

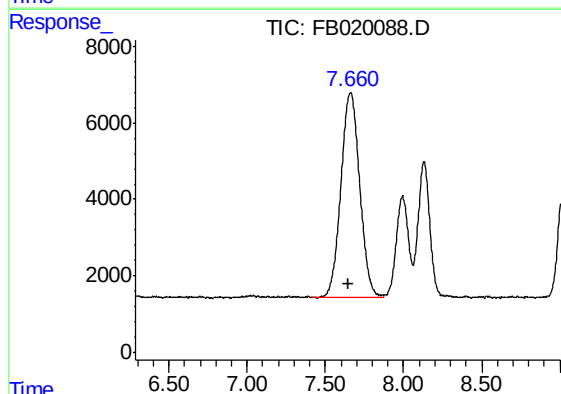


#2 2,2,4-Trimethylpentane

R.T.: 7.661 min
Delta R.T.: 0.010 min
Response: 447143
Conc: 22.21 ng/ml

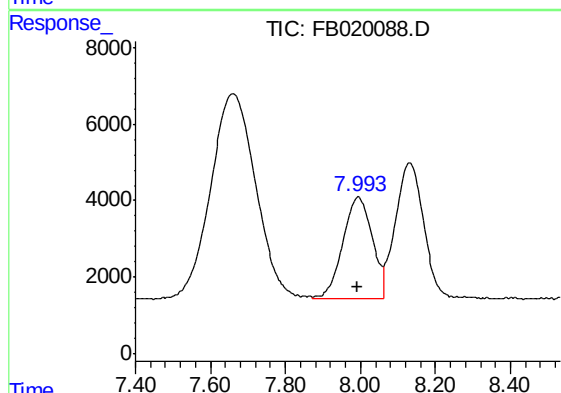


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: 0.003 min
Response: 143296
Conc: 7.68 ng/ml

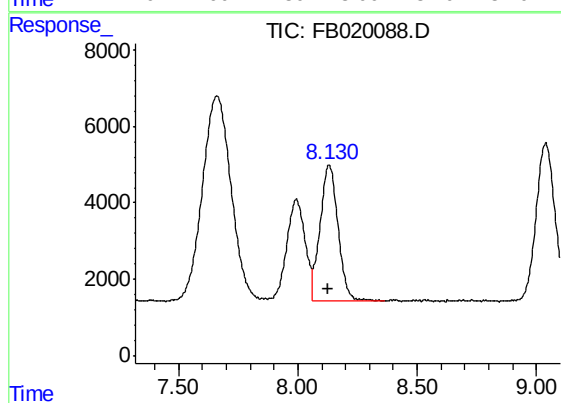


#4 Benzene

R.T.: 8.131 min
Delta R.T.: 0.002 min
Response: 186920
Conc: 8.92 ng/ml

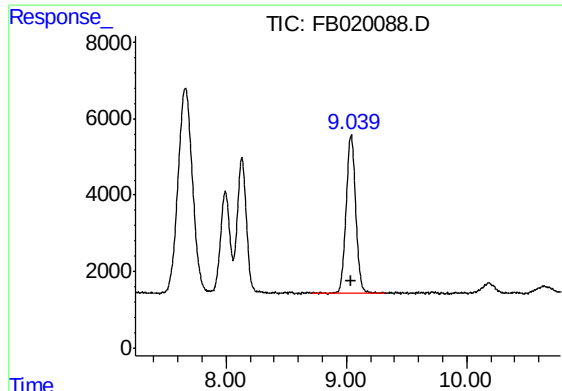


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.002 min
Response: 232239
Conc: 20.72 ng/ml

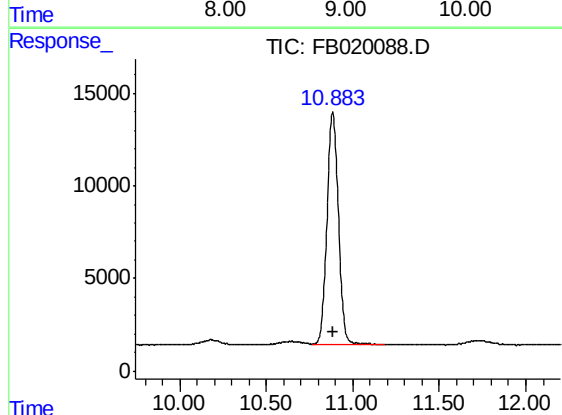


#6 Toluene

R.T.: 10.884 min
Delta R.T.: 0.000 min
Response: 582455
Conc: 30.73 ng/ml

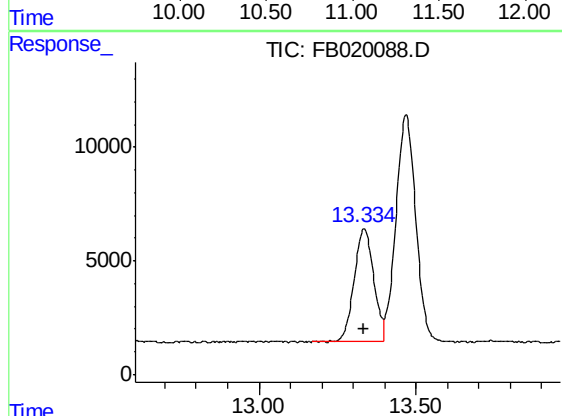


#7 Ethylbenzene

R.T.: 13.336 min
Delta R.T.: 0.000 min
Response: 215196
Conc: 9.47 ng/ml

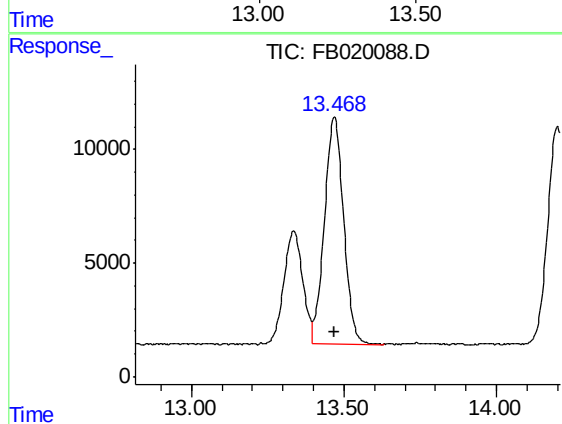

#8 m-Xylene

R.T.: 13.469 min
Delta R.T.: 0.000 min
Response: 439370
Conc: 18.74 ng/ml

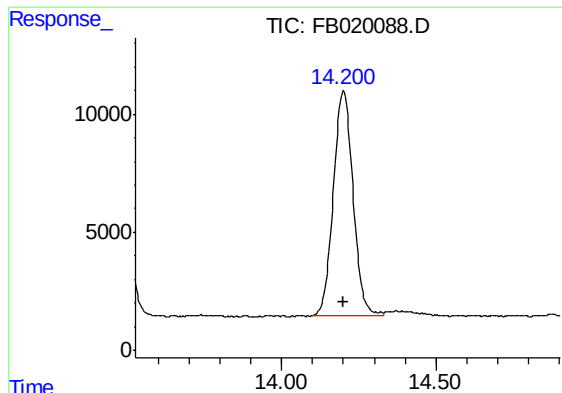


#9 O-Xylene

R.T.: 14.201 min

Delta R.T.: 0.000 min

Response: 424096

Conc: 18.21 ng/ml

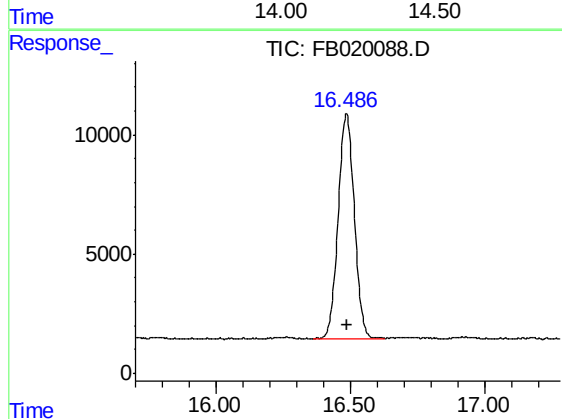

#10 1,2,4-Trimethylbenzene

R.T.: 16.487 min

Delta R.T.: 0.000 min

Response: 396218

Conc: 17.21 ng/ml