

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030819\
 Data File : FB020119.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2019 12:33
 Operator : MJ/SJ
 Sample : K1787-02MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Mar 08 23:14:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:28:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.037	241153	21.520 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	505850	24.313 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	511101	25.387 ng/ml
3) t n-Heptane	7.993	162071	8.689 ng/ml
4) t Benzene	8.130	196470	9.372 ng/ml
6) t Toluene	10.884	590304	31.147 ng/ml
7) t Ethylbenzene	13.335	219950	9.684 ng/ml
8) t m-Xylene	13.468	446999	19.064 ng/ml
9) t O-Xylene	14.199	430591	18.493 ng/ml
10) t 1,2,4-Trimethylbenzene	16.486	412618	17.921 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030819\
Data File : FB020119.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2019 12:33
Operator : MJ/SJ
Sample : K1787-02MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Mar 08 23:14:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:28:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

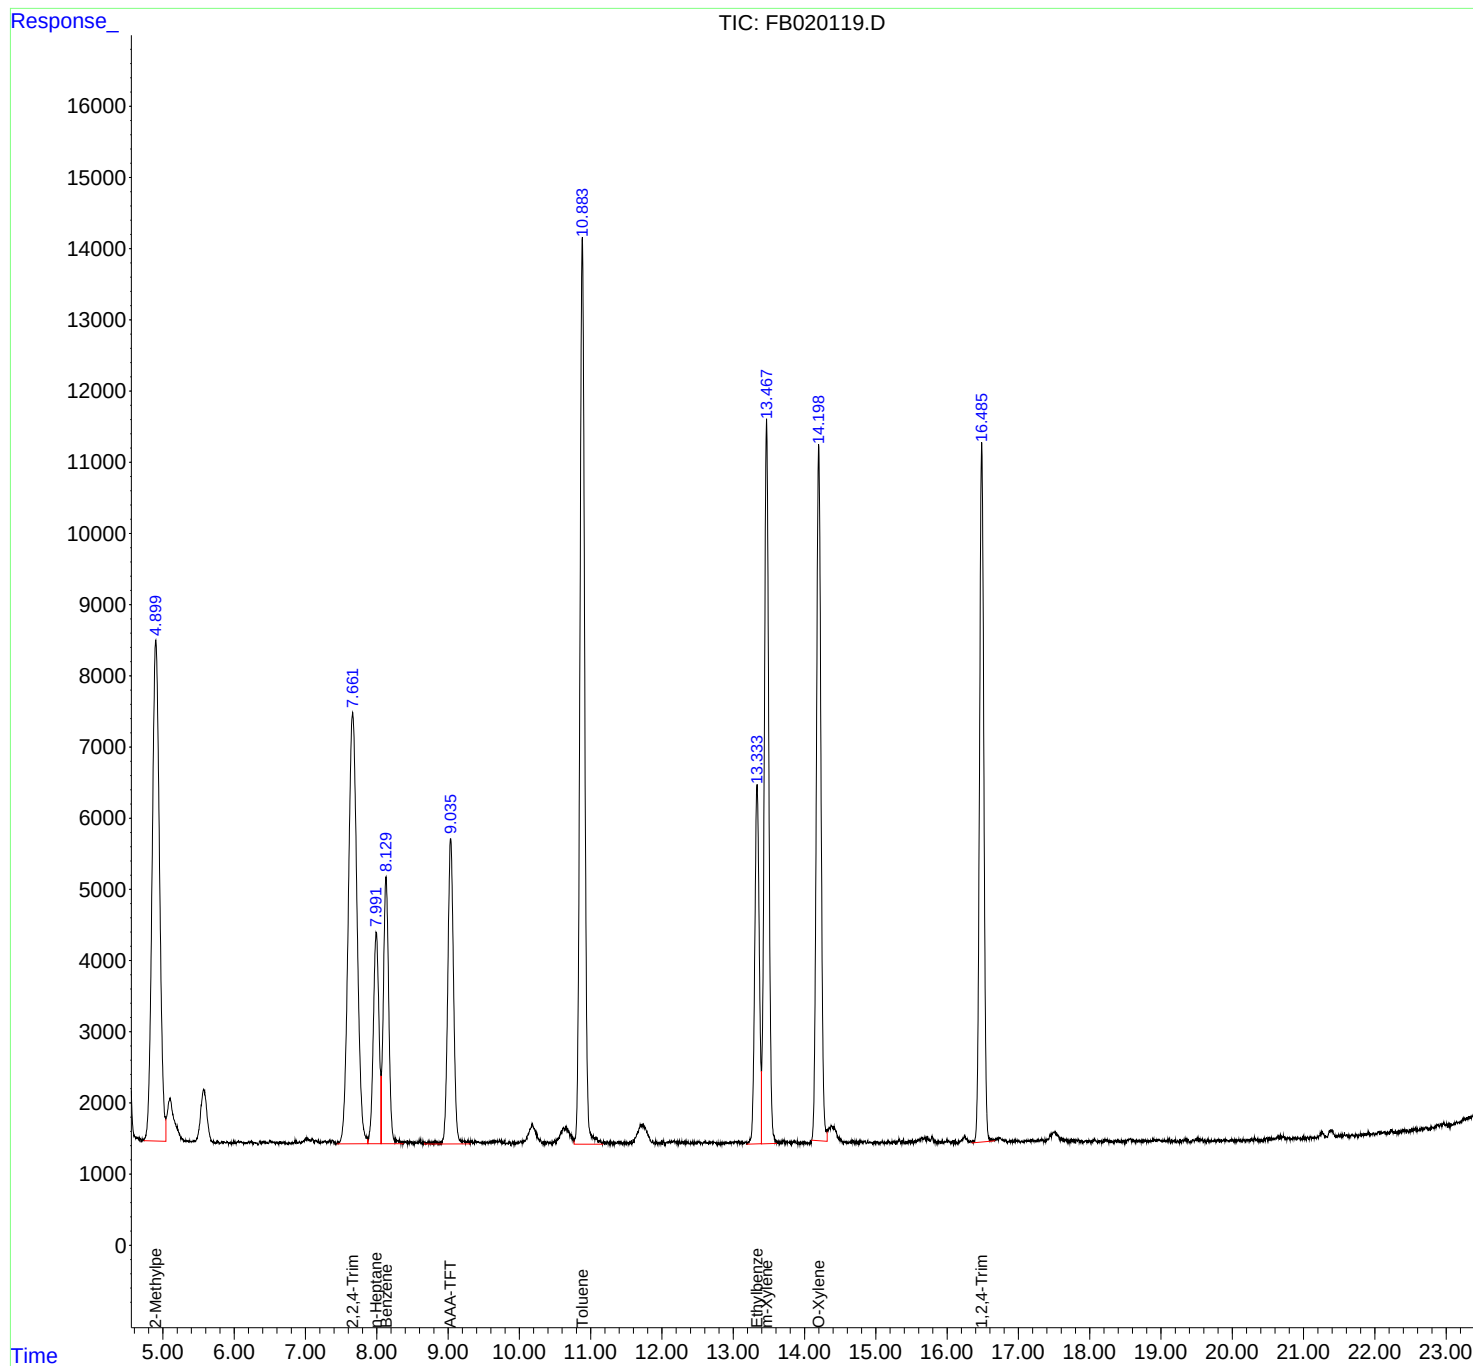

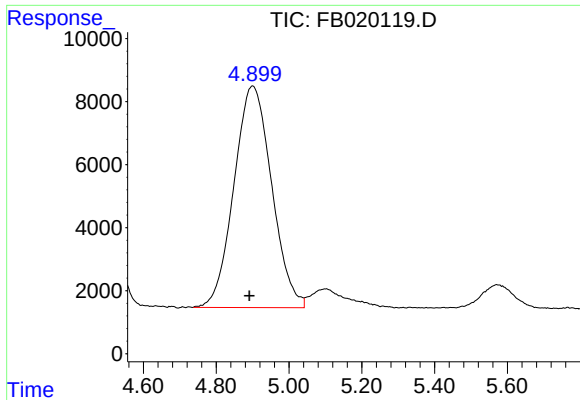


#1 2-Methylpentane

R.T.: 4.901 min
Delta R.T.: 0.010 min
Response: 505850
Conc: 24.31 ng/ml

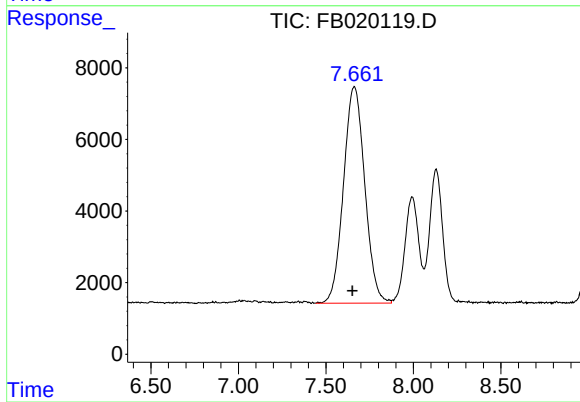


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: 0.011 min
Response: 511101
Conc: 25.39 ng/ml

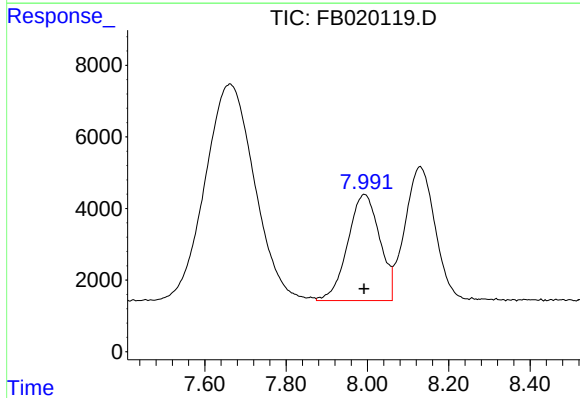


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.002 min
Response: 162071
Conc: 8.69 ng/ml

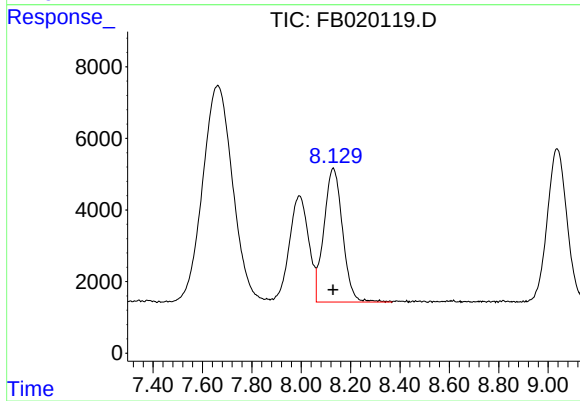


#4 Benzene

R.T.: 8.130 min
Delta R.T.: 0.001 min
Response: 196470
Conc: 9.37 ng/ml

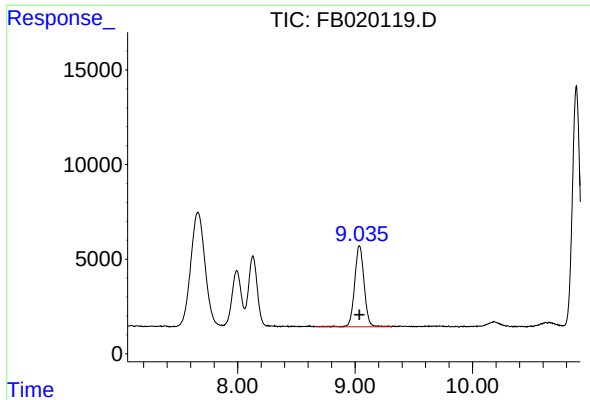


#5 AAA-TFT

R.T.: 9.037 min
Delta R.T.: 0.000 min
Response: 241153
Conc: 21.52 ng/ml

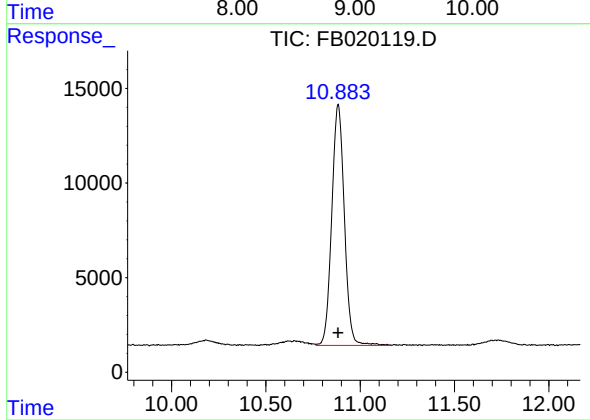


#6 Toluene

R.T.: 10.884 min
Delta R.T.: 0.000 min
Response: 590304
Conc: 31.15 ng/ml

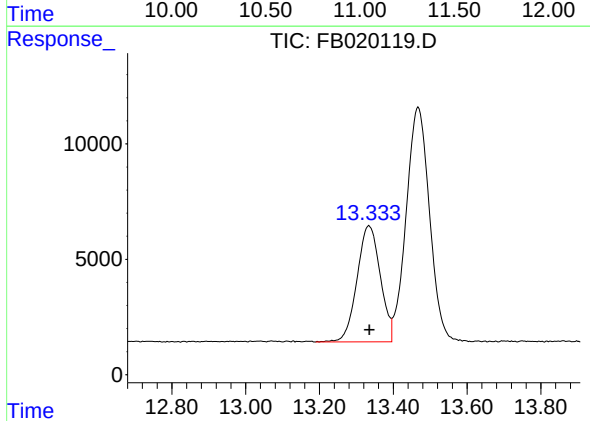


#7 Ethylbenzene

R.T.: 13.335 min
Delta R.T.: -0.001 min
Response: 219950
Conc: 9.68 ng/ml

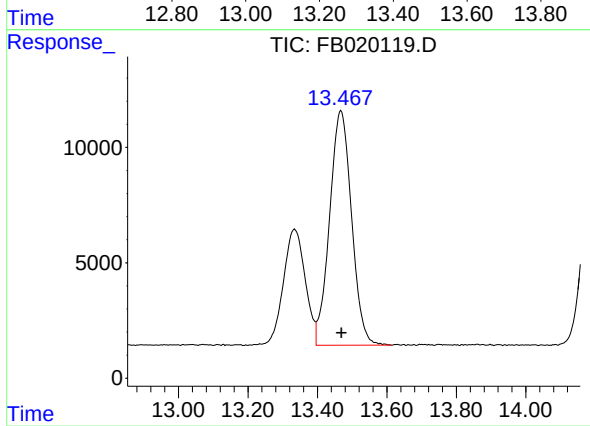

#8 m-Xylene

R.T.: 13.468 min
Delta R.T.: -0.001 min
Response: 446999
Conc: 19.06 ng/ml

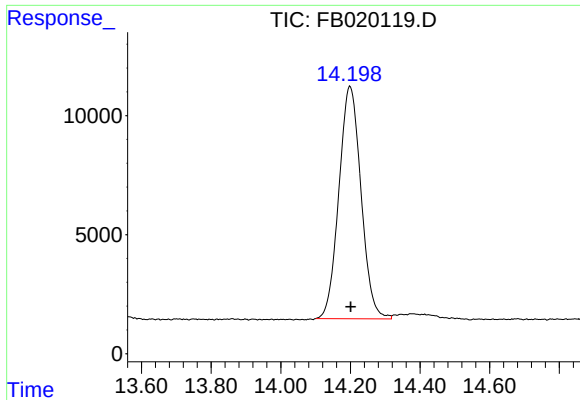


#9 O-Xylene

R.T.: 14.199 min

Delta R.T.: -0.001 min

Response: 430591

Conc: 18.49 ng/ml

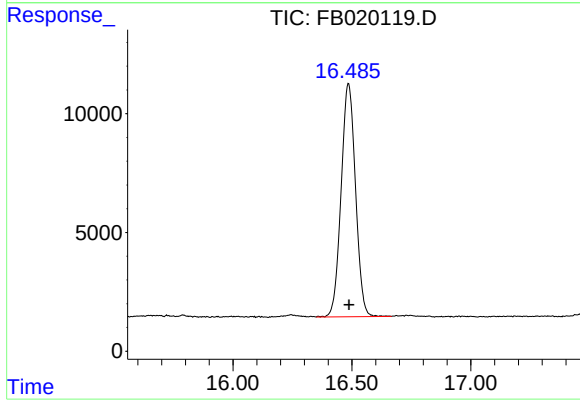

#10 1,2,4-Trimethylbenzene

R.T.: 16.486 min

Delta R.T.: -0.001 min

Response: 412618

Conc: 17.92 ng/ml