

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
Data File : FB025499.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2021 11:42
Operator : DD/AJ
Sample : M1576-04
Misc : 6.96g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 09 01:09:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	567016	22.354 ng/ml
Target Compounds			
9) t O-Xylene	13.880	20379	0.526 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
Data File : FB025499.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2021 11:42
Operator : DD/AJ
Sample : M1576-04
Misc : 6.96g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 09 01:09:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

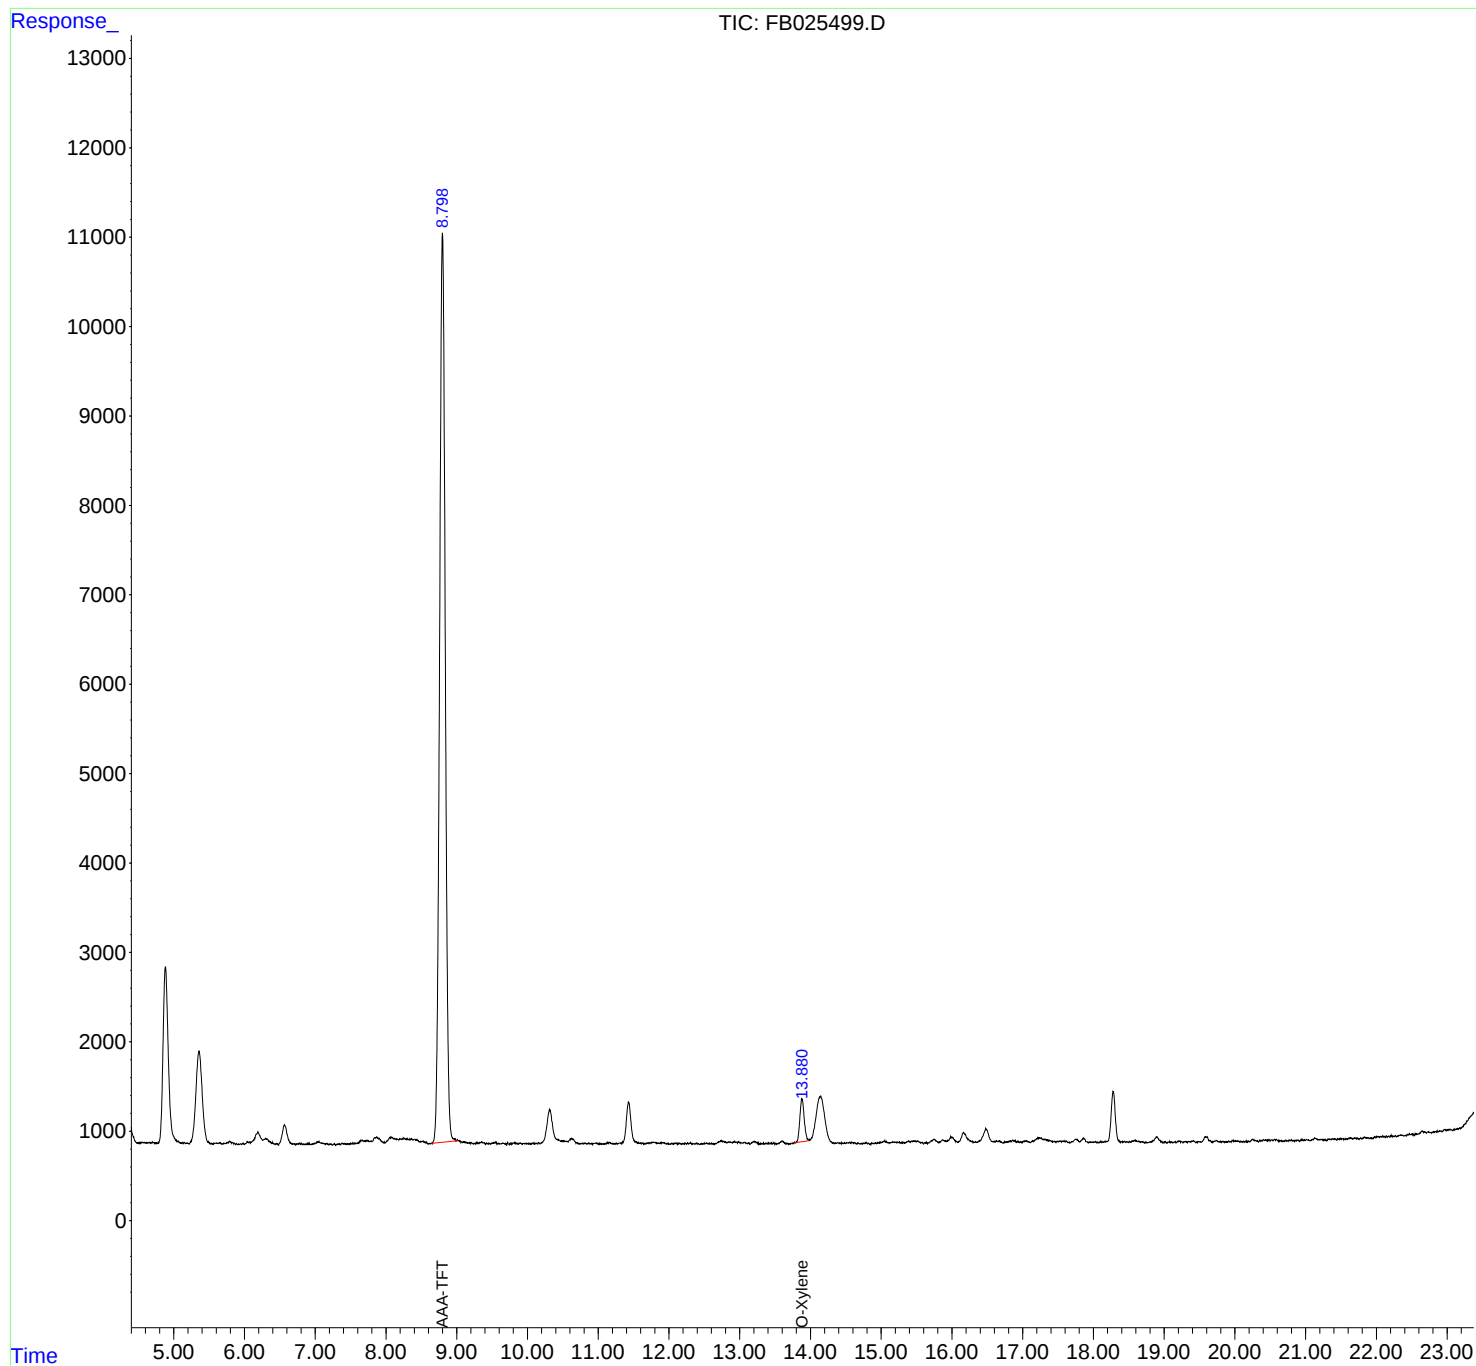


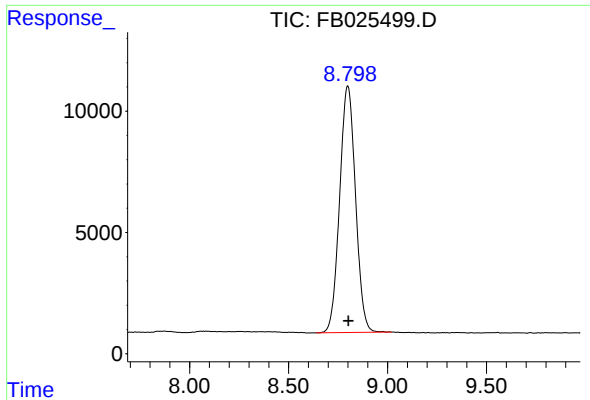

#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.003 min
Response: 567016
Conc: 22.35 ng/ml

Instrument :
FID_B
ClientSampleId :

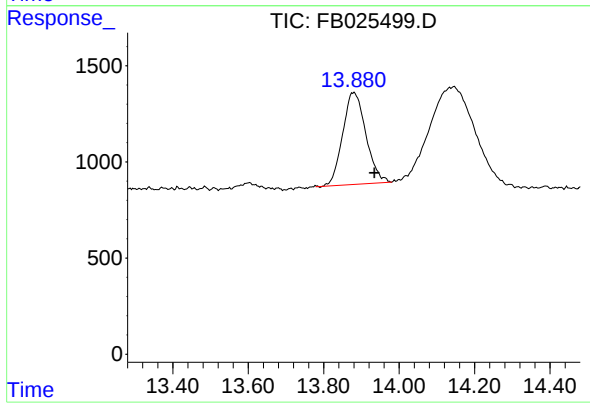

#9 O-Xylene

R.T.: 13.880 min
Delta R.T.: -0.054 min
Response: 20379
Conc: 0.53 ng/ml