

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
 Data File : FB025495.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2021 9:41
 Operator : DD/AJ
 Sample : BSF0308S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0308S1

Integration File: Calibration.e
 Quant Time: Mar 09 01:08:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	523113	20.623 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	1010061	28.658 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1132081	30.488 ng/ml
3) t n-Heptane	7.755	367001	10.138 ng/ml
4) t Benzene	7.890	447689	9.691 ng/ml
6) t Toluene	10.628	1303101	29.146 ng/ml
7) t Ethylbenzene	13.069	403018	9.985 ng/ml
8) t m-Xylene	13.201	806547	20.049 ng/ml
9) t O-Xylene	13.929	774528	20.010 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	678593	20.215 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
Data File : FB025495.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2021 9:41
Operator : DD/AJ
Sample : BSF0308S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0308S1

Integration File: Calibration.e
Quant Time: Mar 09 01:08:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

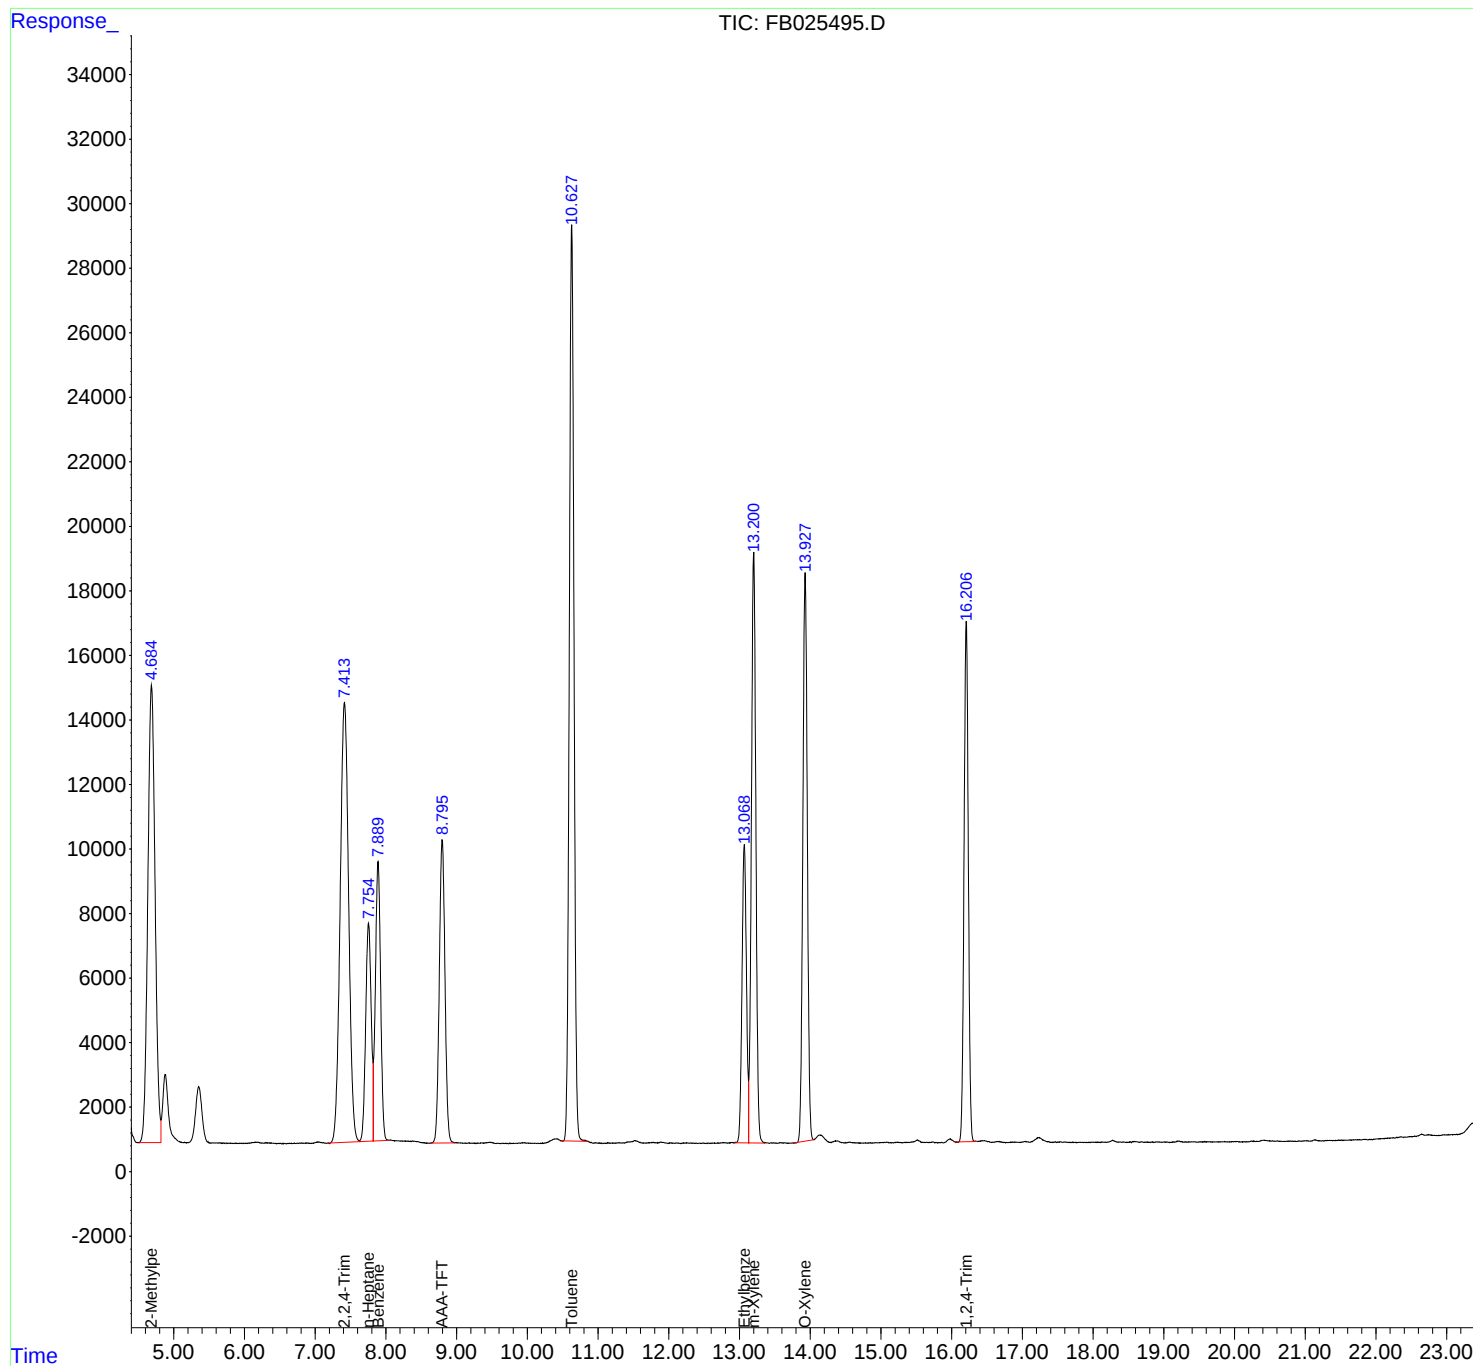


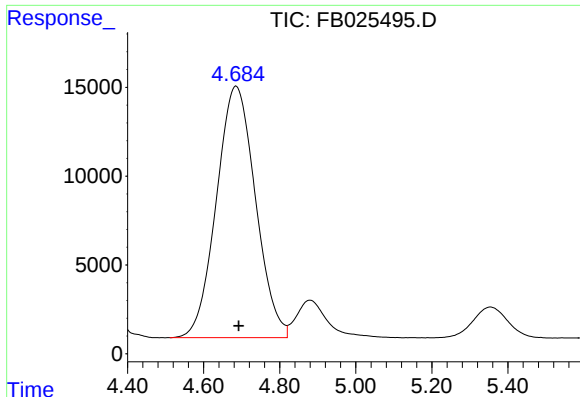

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: -0.007 min
Response: 1010061
Conc: 28.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S1

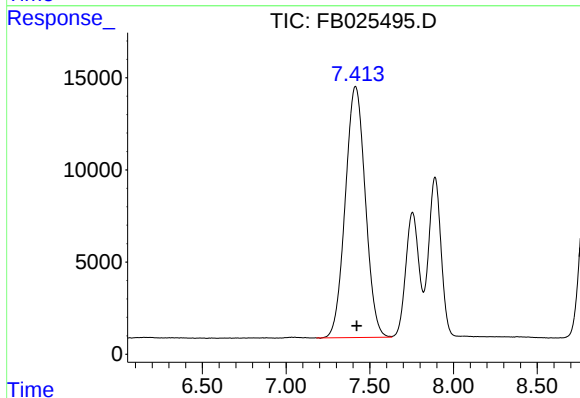


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.007 min
Response: 1132081
Conc: 30.49 ng/ml

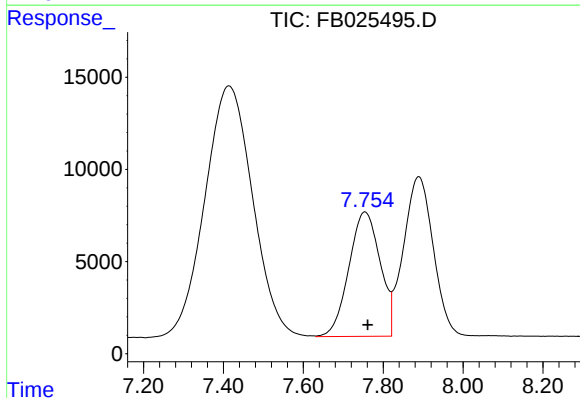


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.006 min
Response: 367001
Conc: 10.14 ng/ml

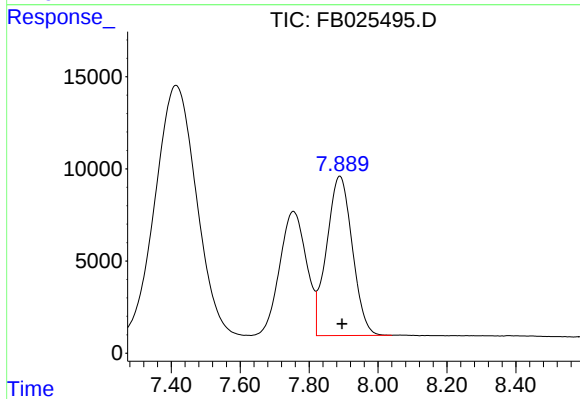

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.006 min
Response: 447689
Conc: 9.69 ng/ml

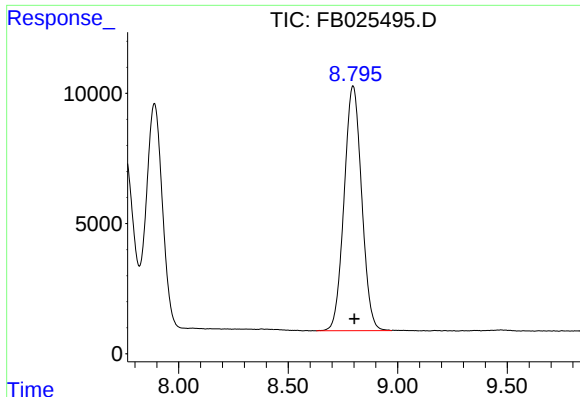

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.006 min
Response: 523113
Conc: 20.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S1

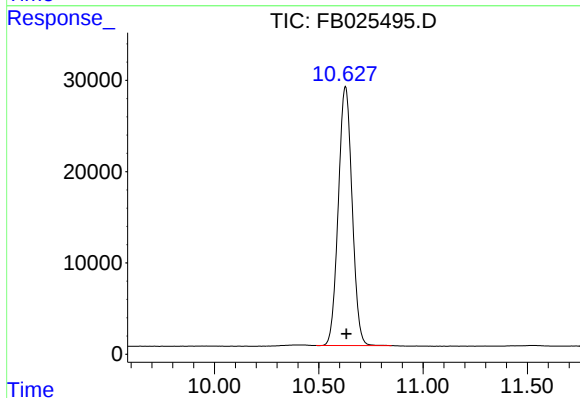


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.005 min
Response: 1303101
Conc: 29.15 ng/ml

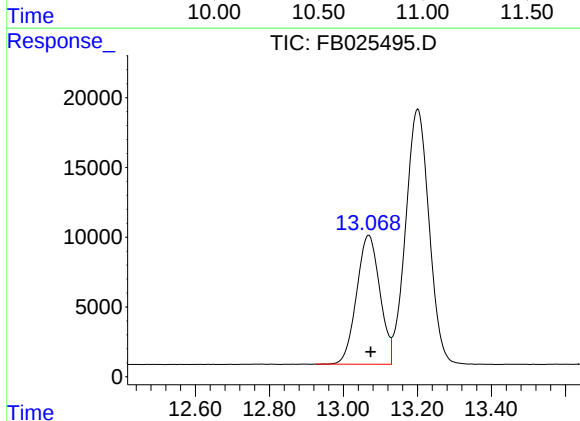


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.005 min
Response: 403018
Conc: 9.99 ng/ml

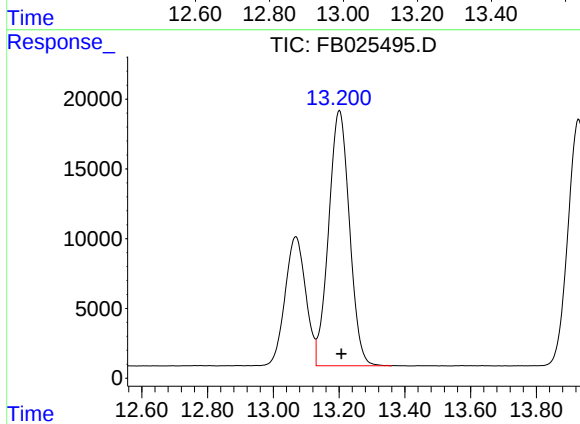

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.005 min
Response: 806547
Conc: 20.05 ng/ml

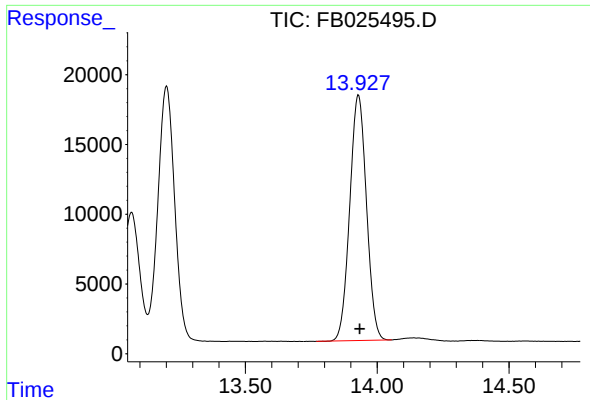

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.005 min
Response: 774528
Conc: 20.01 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S1

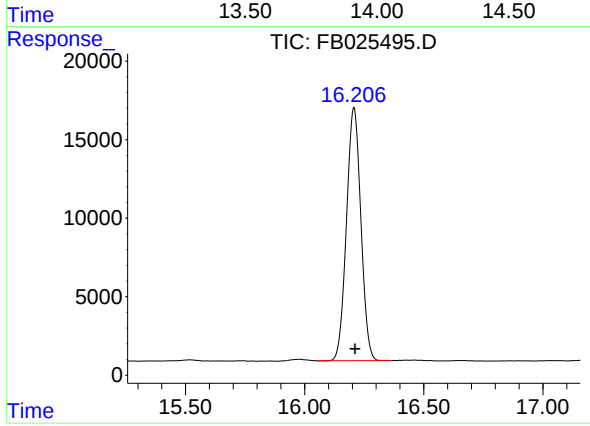

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.005 min
Response: 678593
Conc: 20.22 ng/ml