

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
 Data File : FB025501.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2021 12:42
 Operator : DD/AJ
 Sample : BSF0308S2
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0308S2

Integration File: Calibration.e
 Quant Time: Mar 09 01:09:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	469441	18.507 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	814332	23.105 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	917973	24.722 ng/ml
3) t n-Heptane	7.757	293719	8.113 ng/ml
4) t Benzene	7.892	397132	8.597 ng/ml
6) t Toluene	10.629	1133847	25.360 ng/ml
7) t Ethylbenzene	13.070	354437	8.782 ng/ml
8) t m-Xylene	13.203	707404	17.585 ng/ml
9) t O-Xylene	13.930	691319	17.860 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	608525	18.128 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
Data File : FB025501.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2021 12:42
Operator : DD/AJ
Sample : BSF0308S2
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0308S2

Integration File: Calibration.e
Quant Time: Mar 09 01:09:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

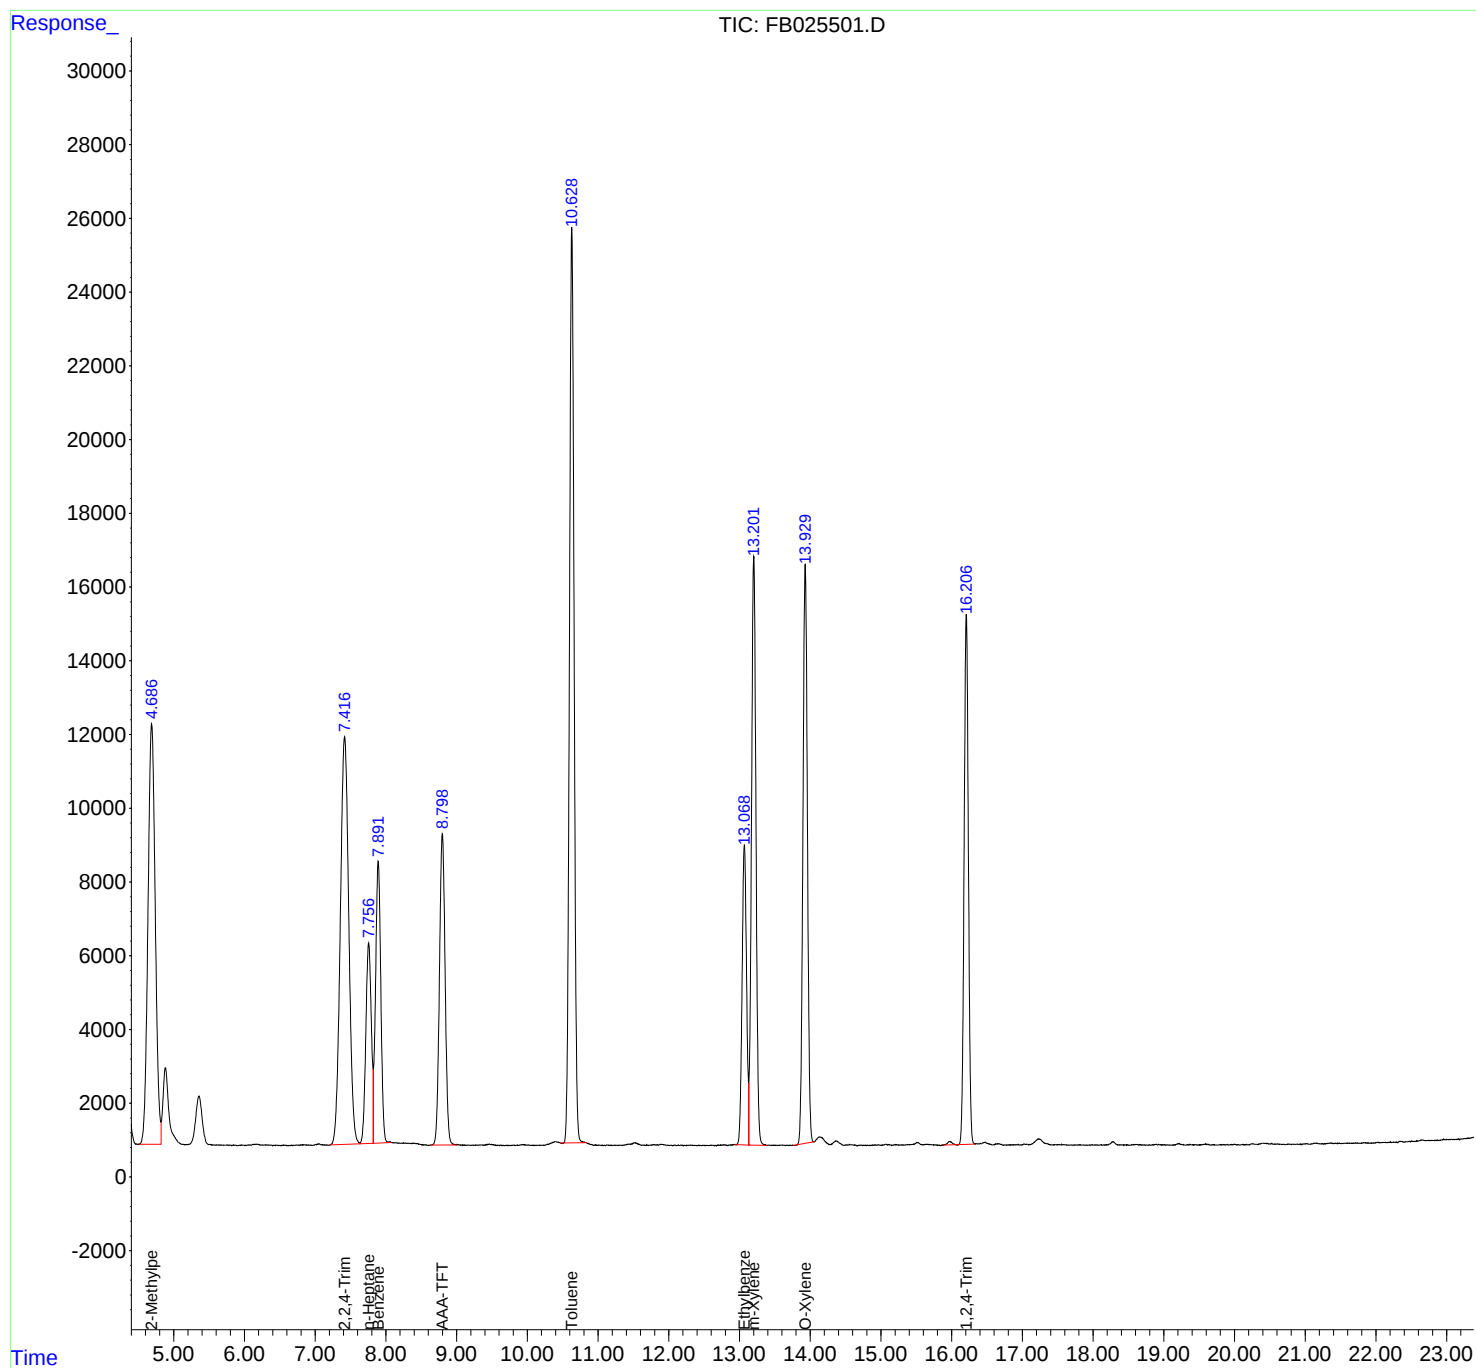


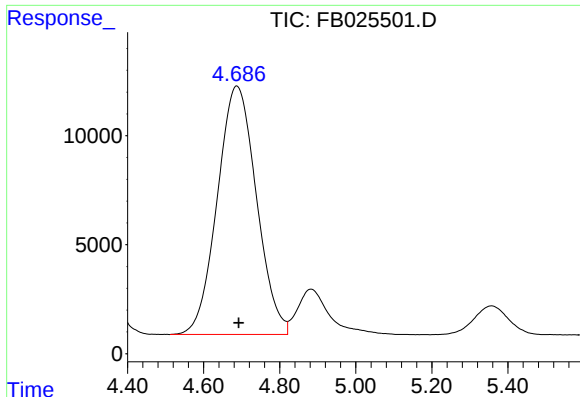

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.004 min
Response: 814332
Conc: 23.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S2

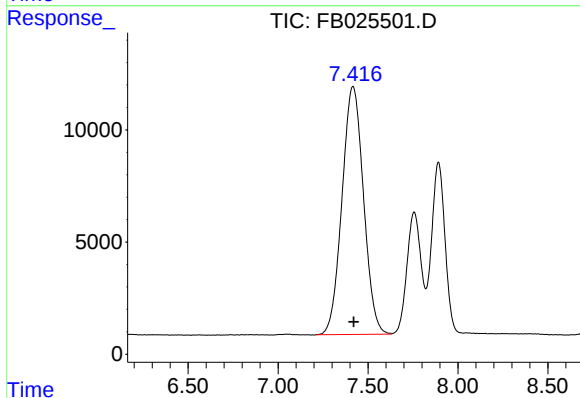


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.005 min
Response: 917973
Conc: 24.72 ng/ml

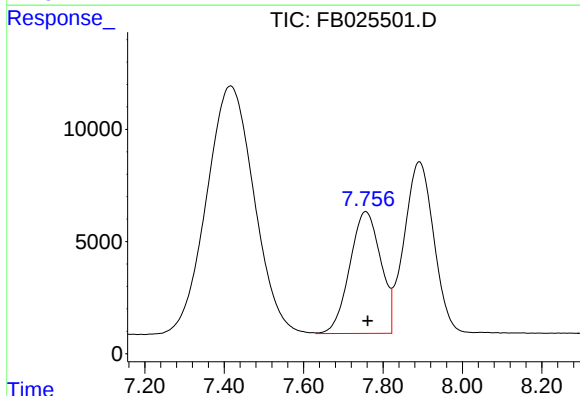


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.004 min
Response: 293719
Conc: 8.11 ng/ml

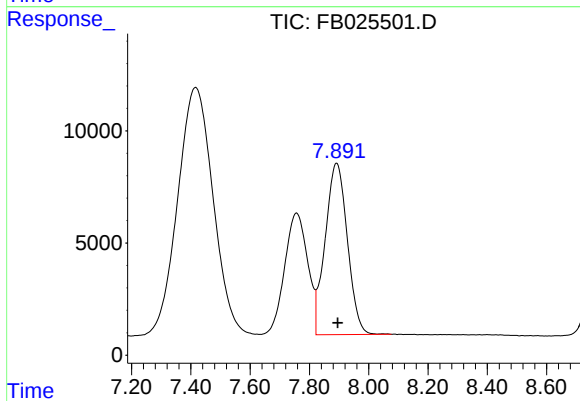

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 397132
Conc: 8.60 ng/ml

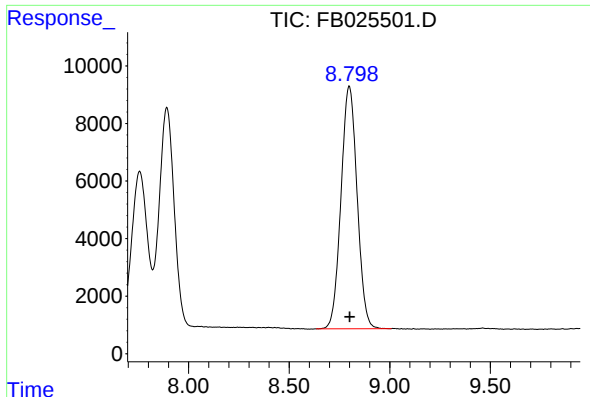

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: -0.004 min
Response: 469441
Conc: 18.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S2

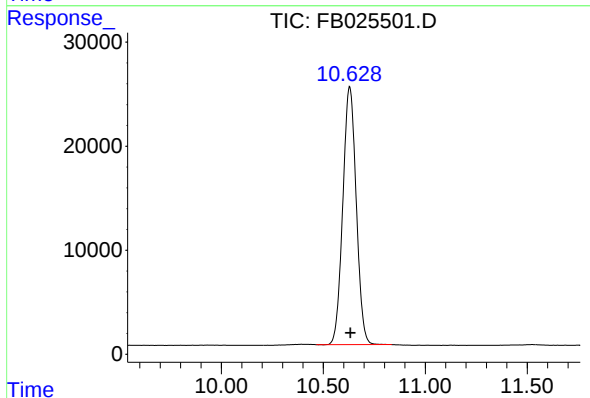


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.004 min
Response: 1133847
Conc: 25.36 ng/ml

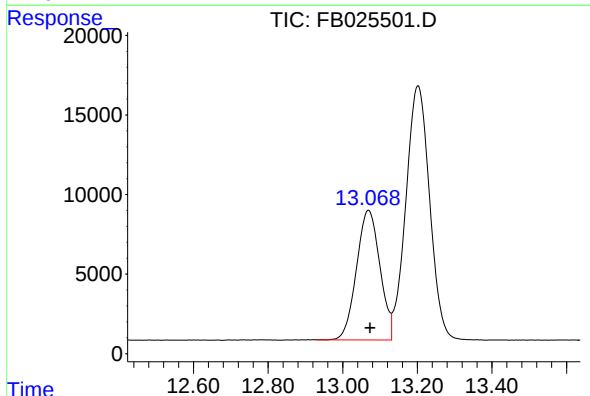


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.004 min
Response: 354437
Conc: 8.78 ng/ml

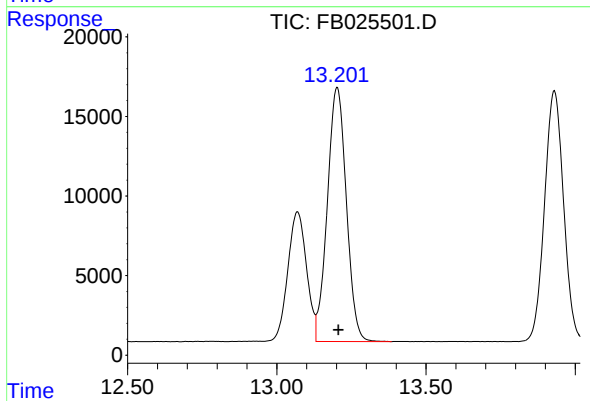

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.004 min
Response: 707404
Conc: 17.58 ng/ml

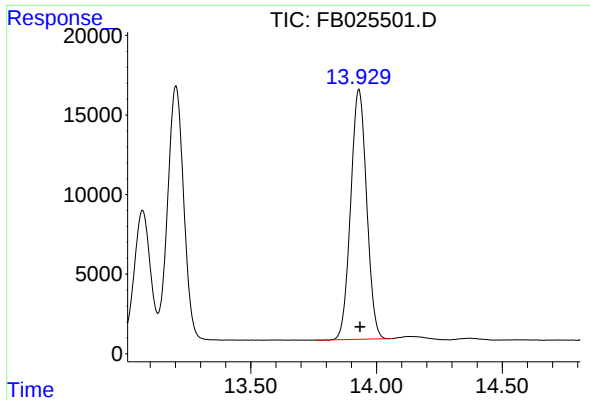

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.004 min
Response: 691319
Conc: 17.86 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S2

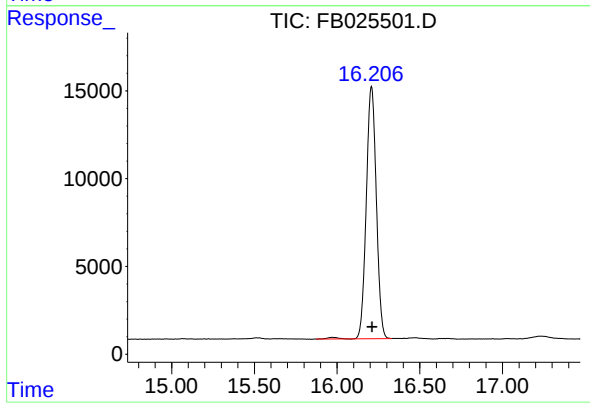

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.004 min
Response: 608525
Conc: 18.13 ng/ml