

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
 Data File : FB025504.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2021 14:17
 Operator : DD/AJ
 Sample : BSF0308W1
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0308W1

Integration File: Calibration.e
 Quant Time: Mar 09 01:09:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	522316	20.592 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	999445	28.357 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1121700	30.208 ng/ml
3) t n-Heptane	7.758	365184	10.088 ng/ml
4) t Benzene	7.894	448458	9.708 ng/ml
6) t Toluene	10.631	1290612	28.867 ng/ml
7) t Ethylbenzene	13.072	397355	9.845 ng/ml
8) t m-Xylene	13.204	792953	19.711 ng/ml
9) t O-Xylene	13.932	760593	19.650 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	659646	19.651 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030821\
Data File : FB025504.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2021 14:17
Operator : DD/AJ
Sample : BSF0308W1
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0308W1

Integration File: Calibration.e
Quant Time: Mar 09 01:09:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

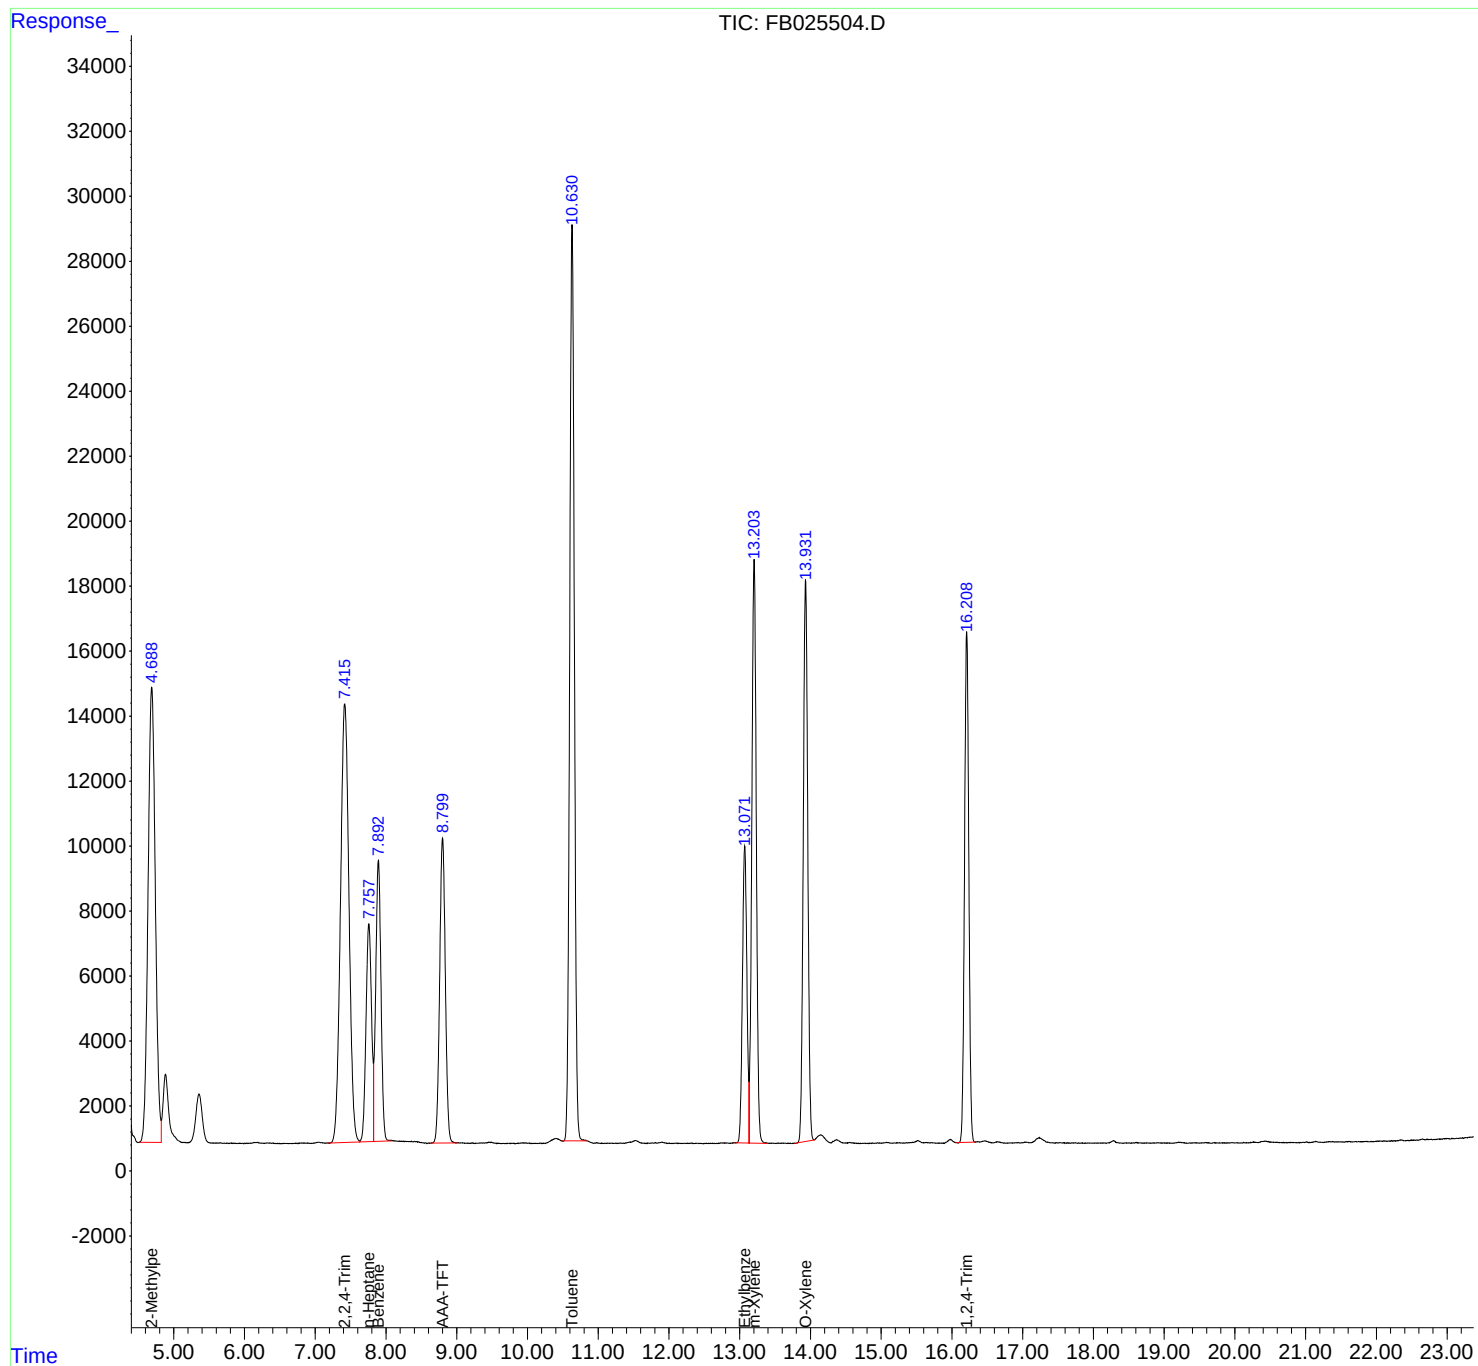


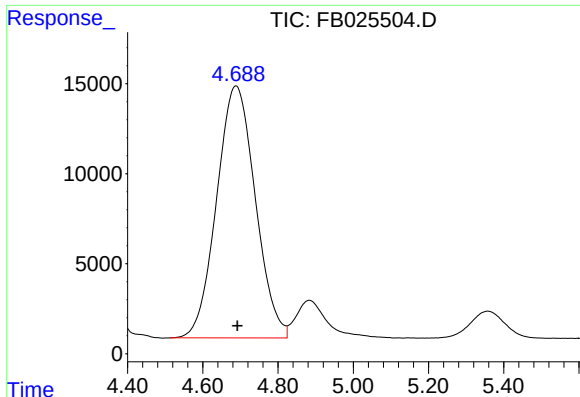

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: -0.003 min
Response: 999445
Conc: 28.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308W1

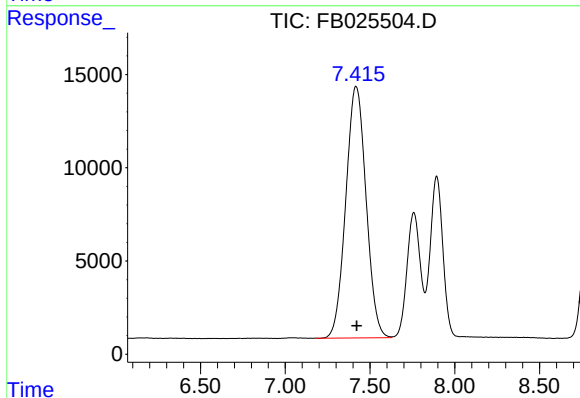


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.005 min
Response: 1121700
Conc: 30.21 ng/ml

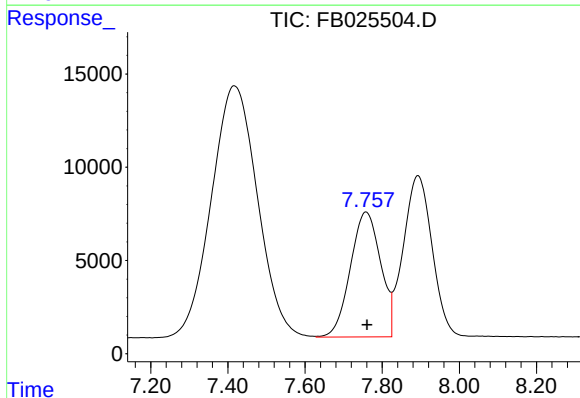


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 365184
Conc: 10.09 ng/ml

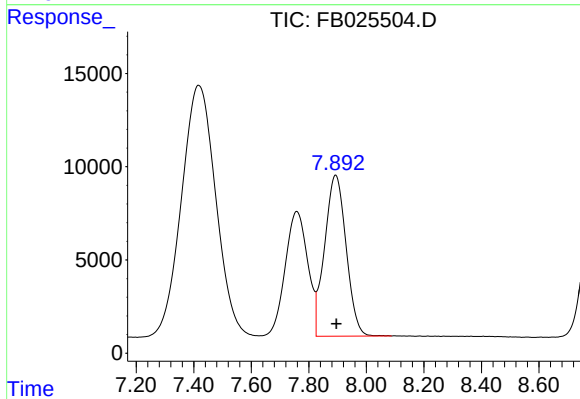

#4 Benzene


R.T.: 7.894 min
Delta R.T.: -0.002 min
Response: 448458
Conc: 9.71 ng/ml

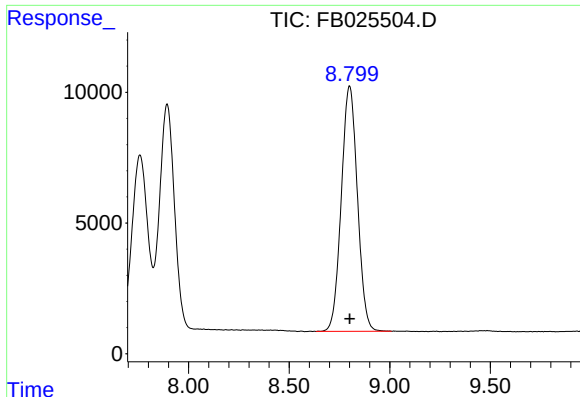

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: -0.002 min
Response: 522316
Conc: 20.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308W1

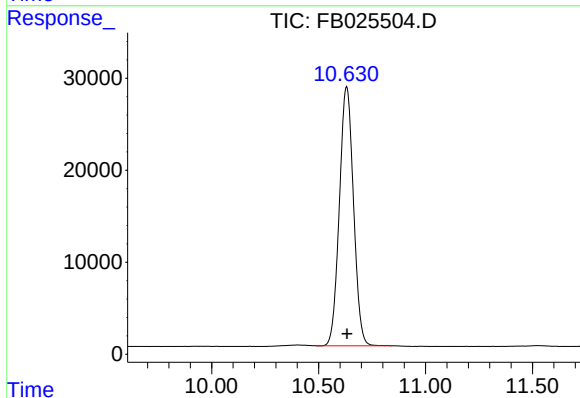


#6 Toluene

R.T.: 10.631 min
Delta R.T.: -0.002 min
Response: 1290612
Conc: 28.87 ng/ml

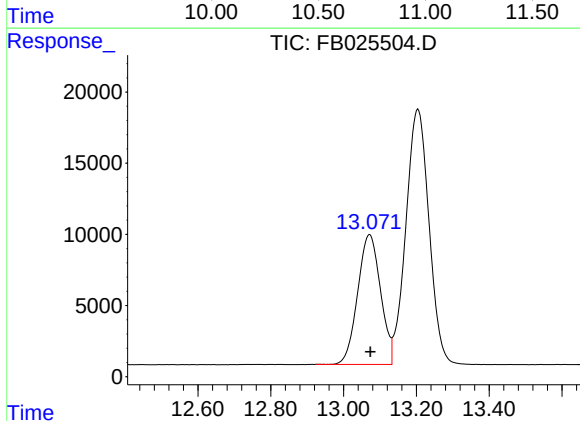


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: -0.002 min
Response: 397355
Conc: 9.85 ng/ml

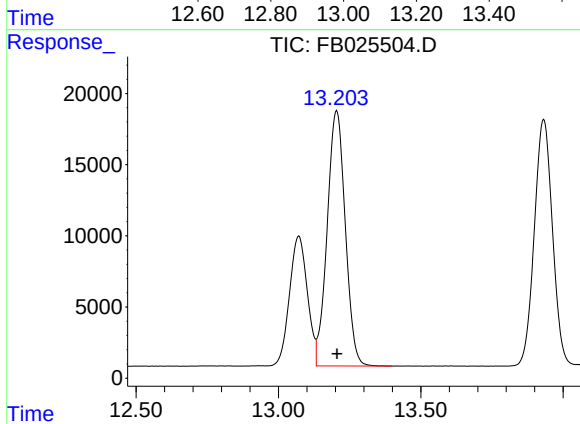

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: -0.002 min
Response: 792953
Conc: 19.71 ng/ml

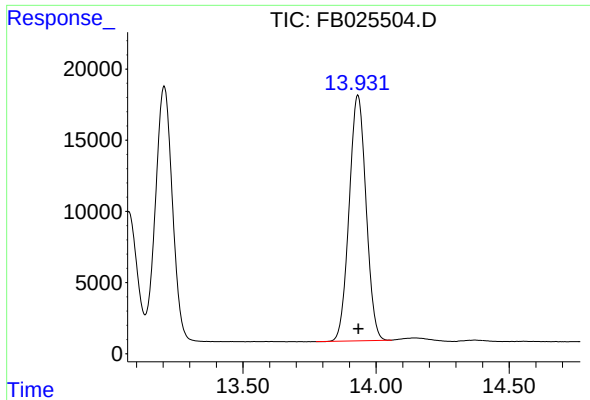

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: -0.002 min
Response: 760593
Conc: 19.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308W1

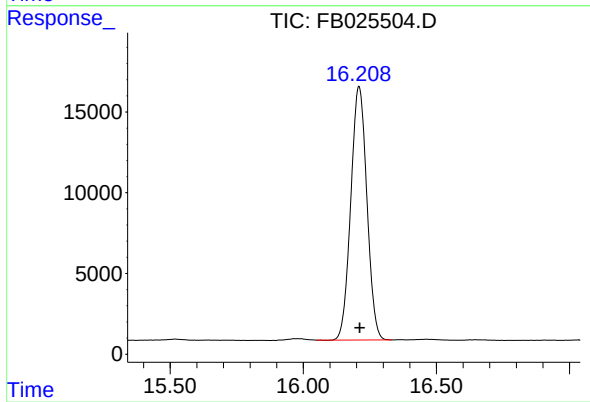

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.002 min
Response: 659646
Conc: 19.65 ng/ml