

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
 Data File : FB026650.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2022 16:19
 Operator : AJ/MA
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 09 03:09:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:05:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	538918	45.491 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	1377483	68.656 ng/ml
2) t 2,2,4-Trimethylpentane	7.444	1539623	72.346 ng/ml
3) t n-Heptane	7.751	469206	21.411 ng/ml
4) t Benzene	7.887	559068	22.428 ng/ml
6) t Toluene	10.622	1597609	68.129 ng/ml
7) t Ethylbenzene	13.059	493434	23.094 ng/ml
8) t m-Xylene	13.192	982929	46.303 ng/ml
9) t O-Xylene	13.919	980708	47.589 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	979144	49.209 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
Data File : FB026650.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2022 16:19
Operator : AJ/MA
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 09 03:09:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:05:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

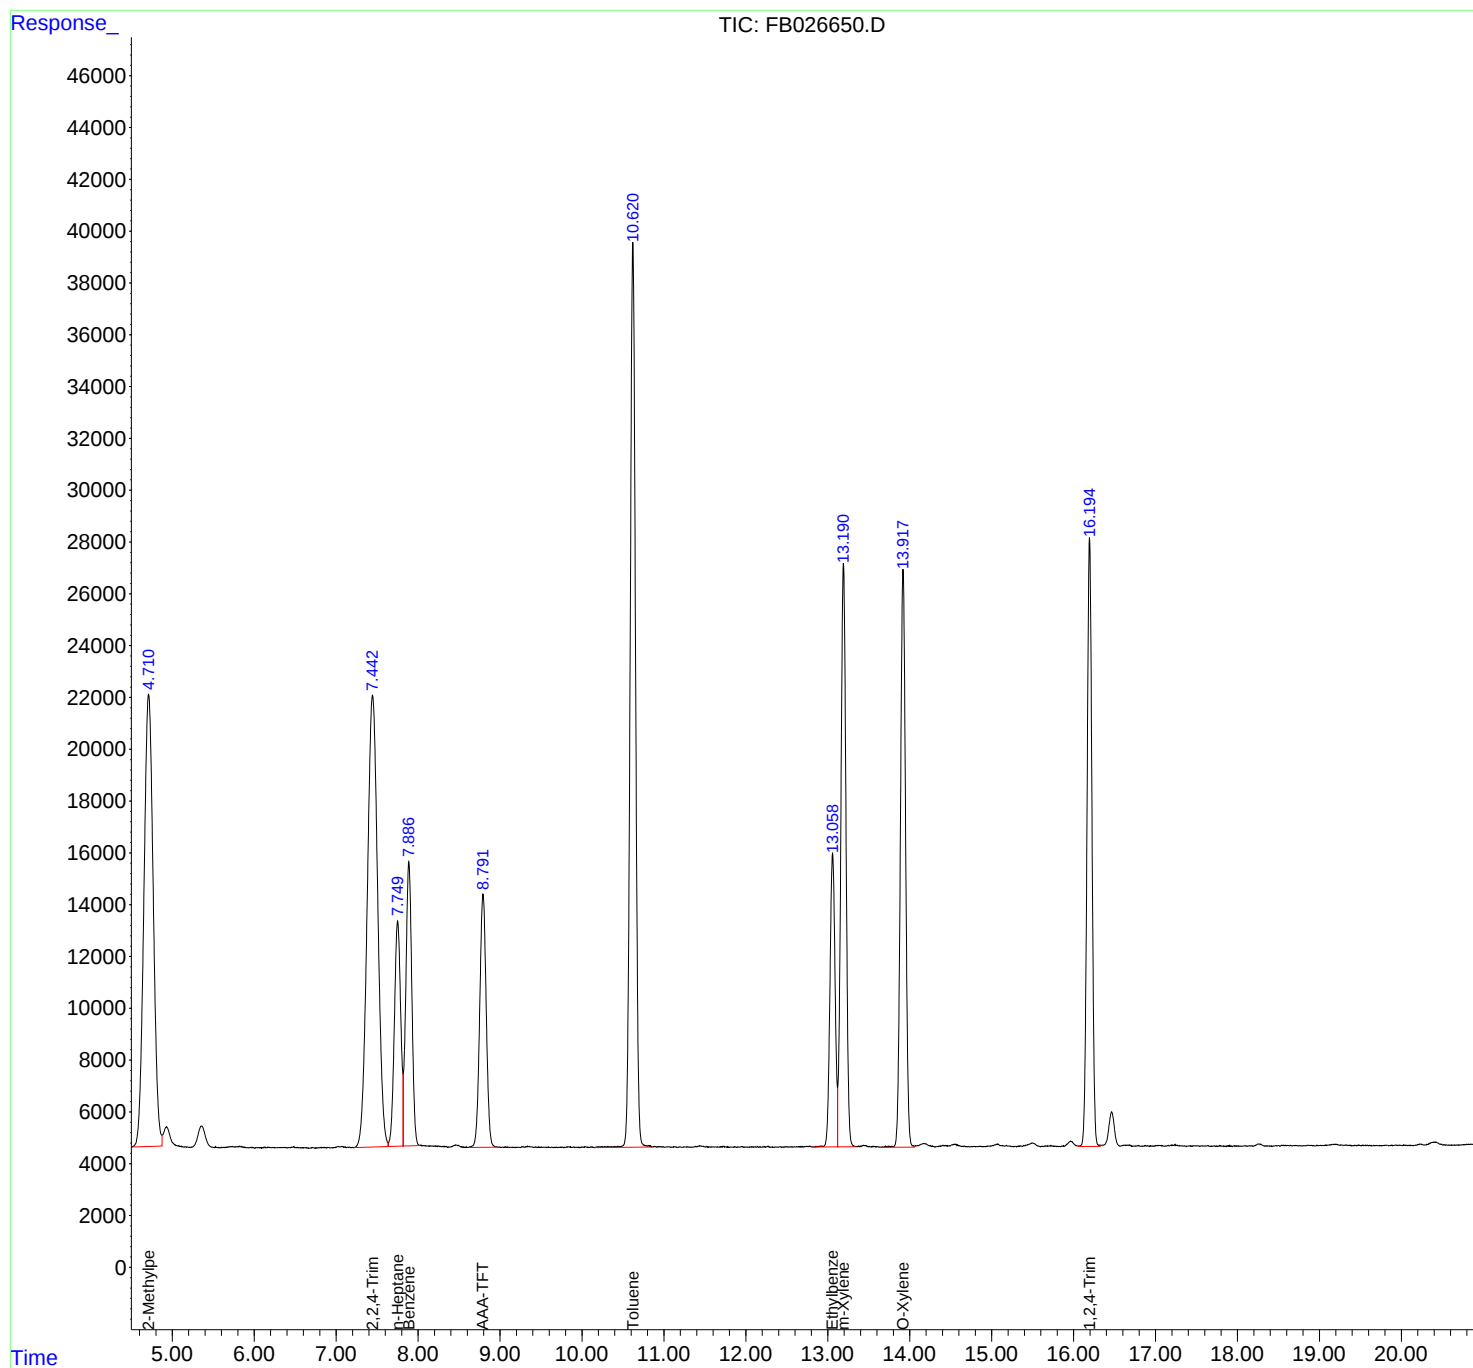


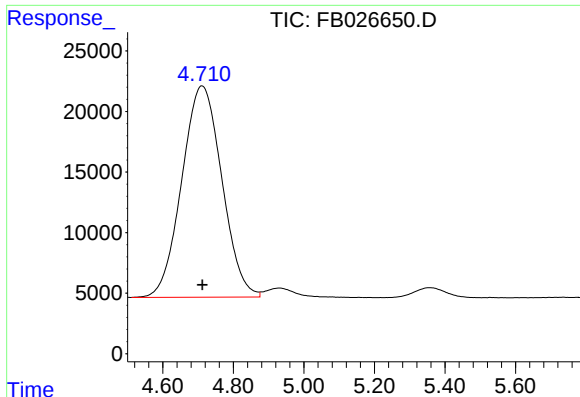

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 1377483
Conc: 68.66 ng/ml

Instrument :
FID_B
ClientSampleId :

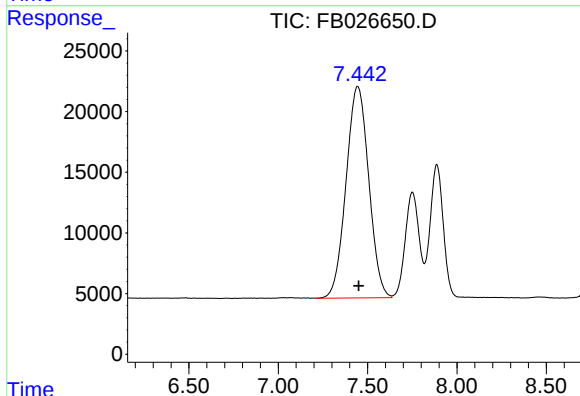


#2 2,2,4-Trimethylpentane

R.T.: 7.444 min
Delta R.T.: -0.007 min
Response: 1539623
Conc: 72.35 ng/ml

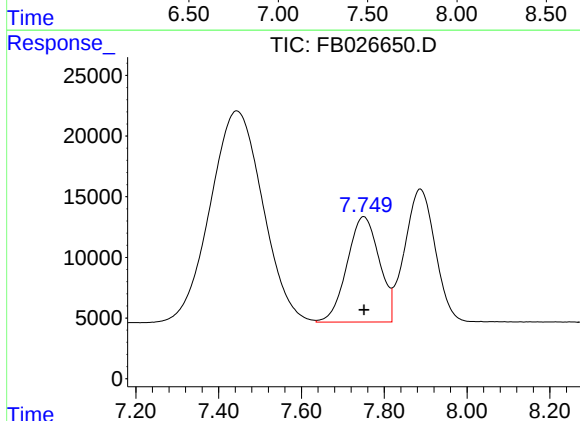


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 469206
Conc: 21.41 ng/ml

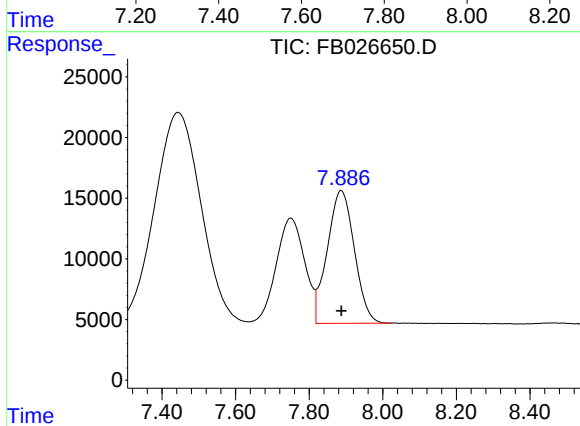

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 559068
Conc: 22.43 ng/ml

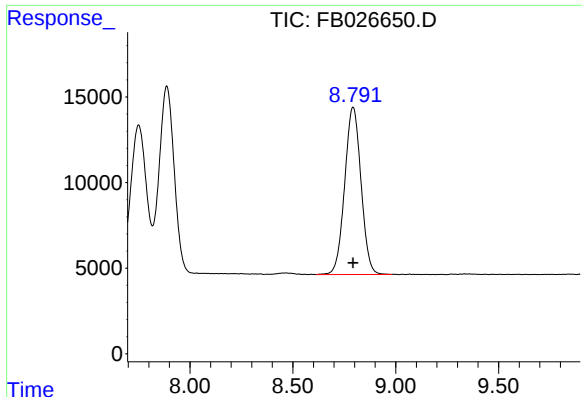

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 538918
Conc: 45.49 ng/ml

Instrument :
FID_B
ClientSampleId :

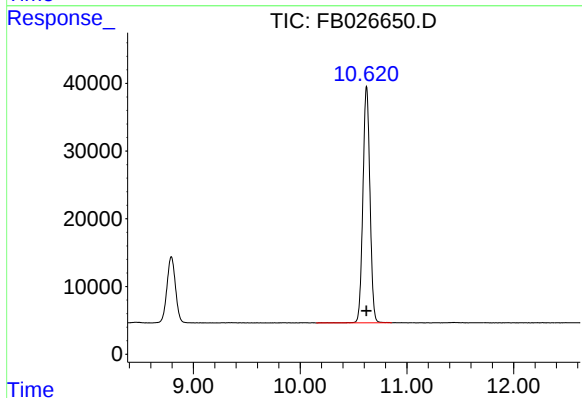


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 1597609
Conc: 68.13 ng/ml

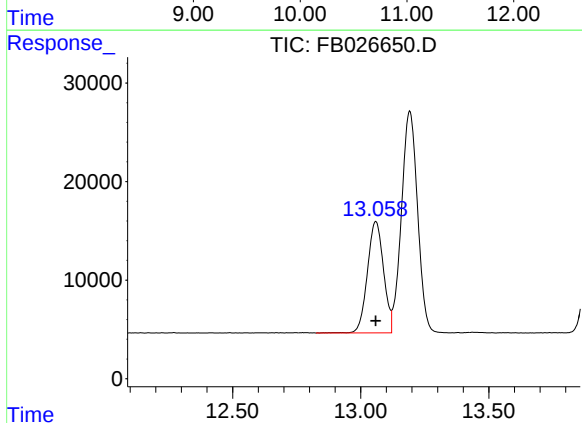


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 493434
Conc: 23.09 ng/ml

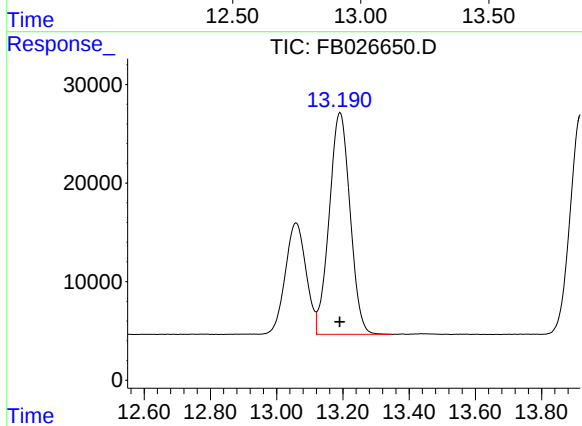

#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: 0.000 min
Response: 982929
Conc: 46.30 ng/ml

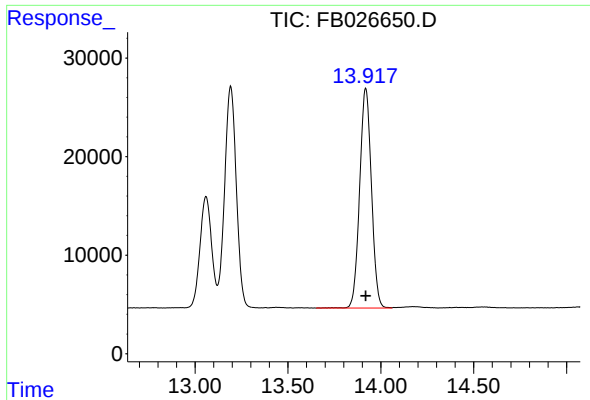


#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.000 min
Response: 980708
Conc: 47.59 ng/ml

Instrument :

FID_B

ClientSampleId :

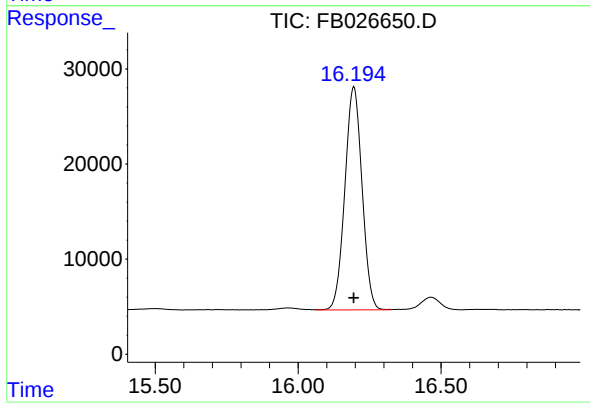

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.000 min
Response: 979144
Conc: 49.21 ng/ml