

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
 Data File : FB026647.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2022 14:23
 Operator : AJ/MA
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 5 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 09 03:09:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:05:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	45517	3.842 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	134226	6.690 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	150269	7.061 ng/ml
3) t n-Heptane	7.752	43680	1.993 ng/ml
4) t Benzene	7.887	50427	2.023 ng/ml
6) t Toluene	10.620	147864	6.306 ng/ml
7) t Ethylbenzene	13.057	45287	2.120 ng/ml
8) t m-Xylene	13.191	93985	4.427 ng/ml
9) t O-Xylene	13.917	95888	4.653 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	102344	5.143 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
Data File : FB026647.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2022 14:23
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Mar 09 03:09:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:05:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

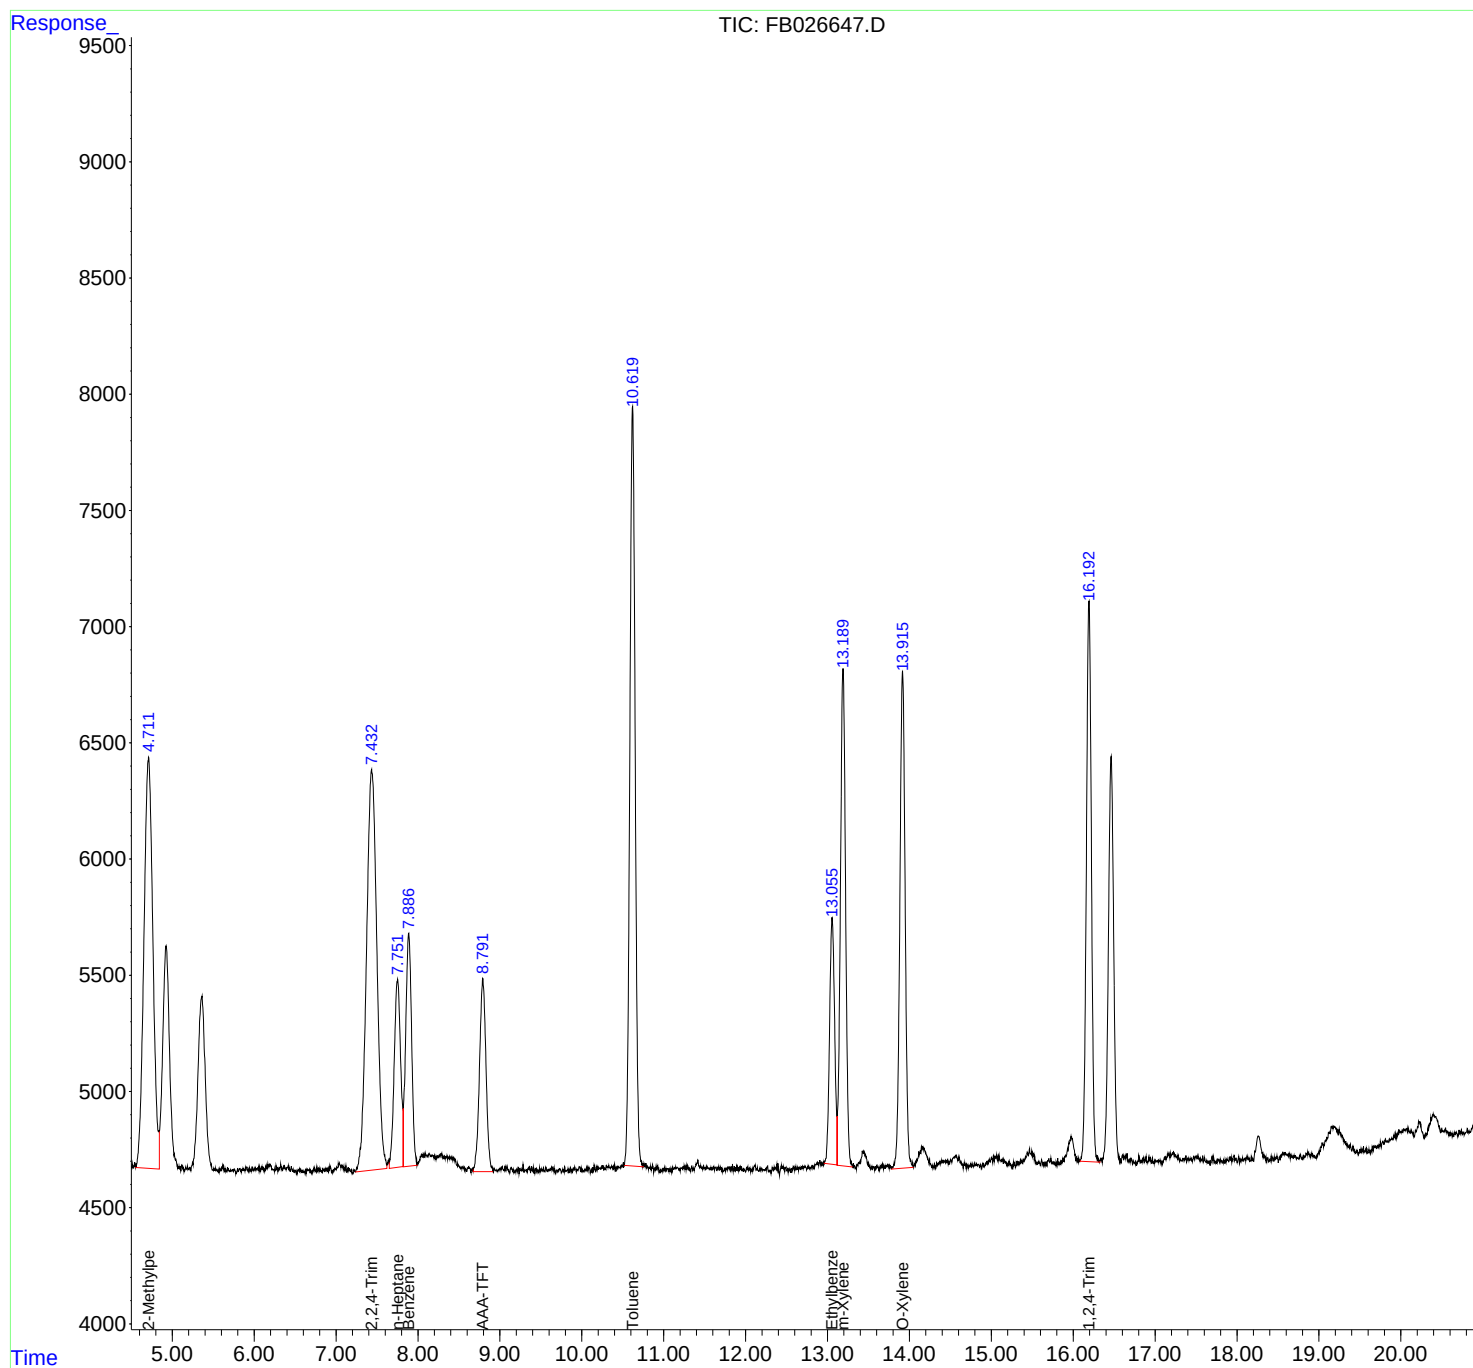


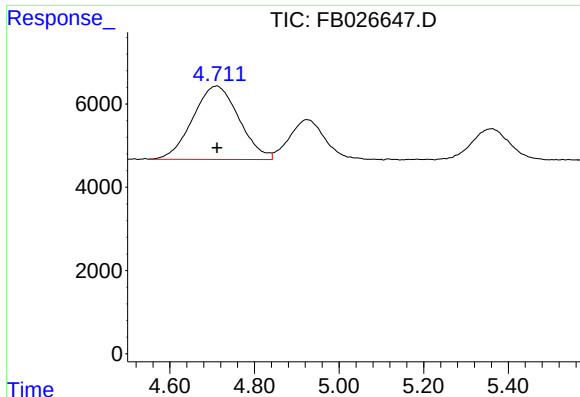

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 134226
Conc: 6.69 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

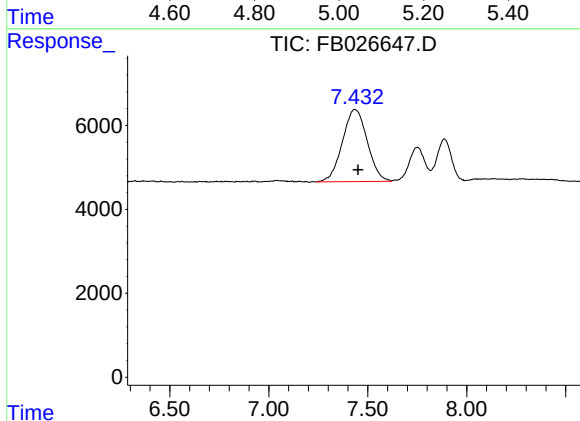


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.018 min
Response: 150269
Conc: 7.06 ng/ml

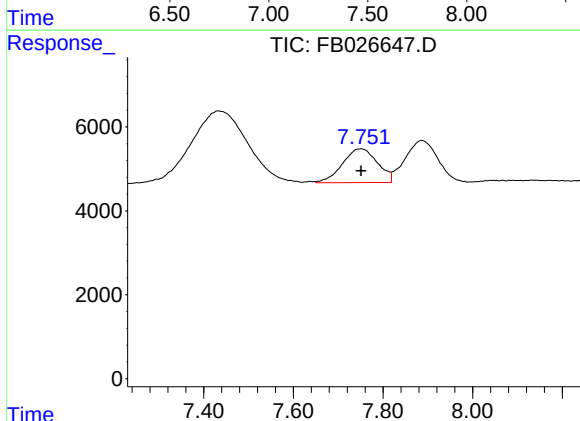


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.001 min
Response: 43680
Conc: 1.99 ng/ml

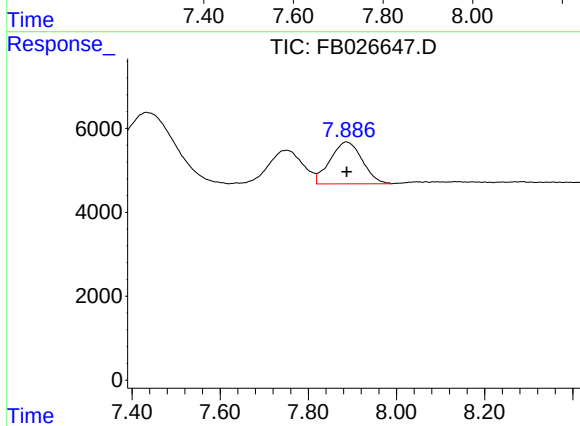

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 50427
Conc: 2.02 ng/ml

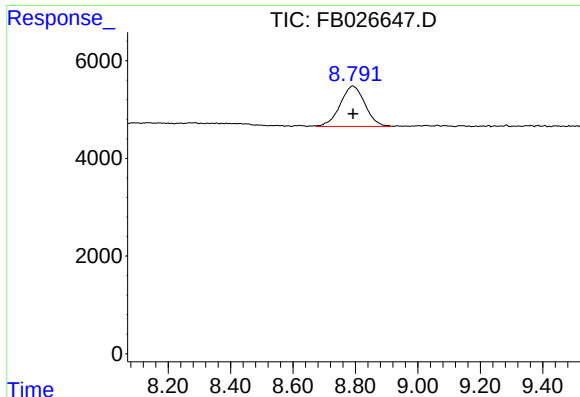

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 45517
Conc: 3.84 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

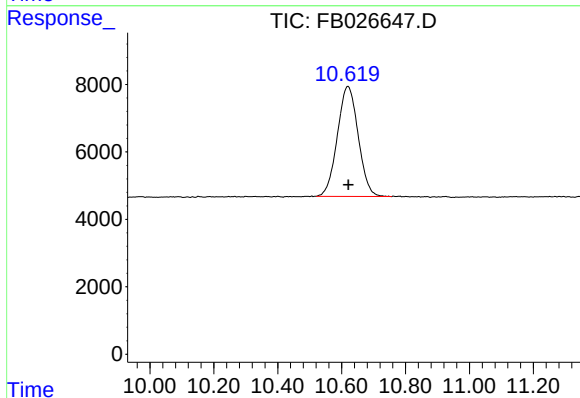


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.001 min
Response: 147864
Conc: 6.31 ng/ml

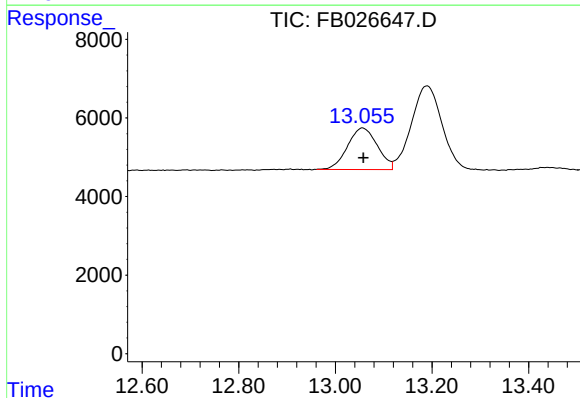


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.002 min
Response: 45287
Conc: 2.12 ng/ml

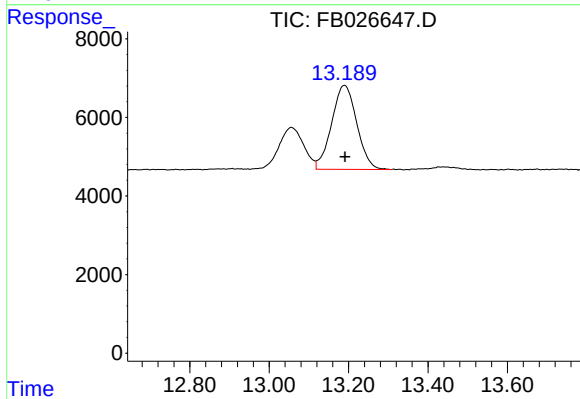

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 93985
Conc: 4.43 ng/ml

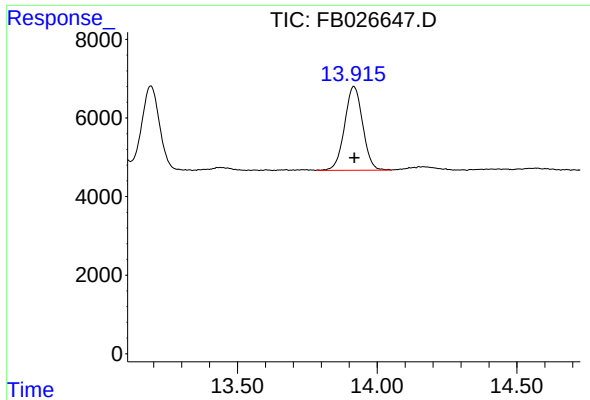

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.002 min
Response: 95888
Conc: 4.65 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

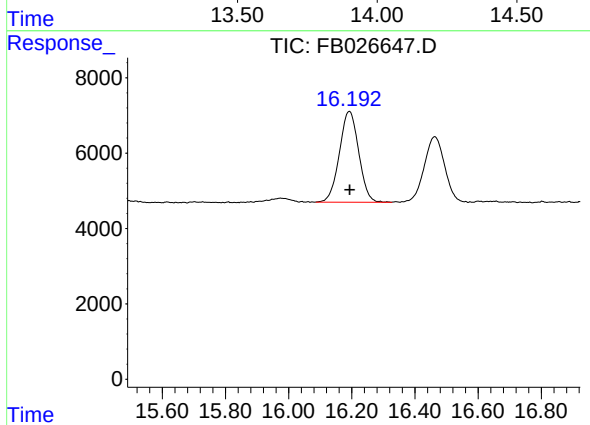

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: -0.001 min
Response: 102344
Conc: 5.14 ng/ml