

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
 Data File : FB026648.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2022 15:01
 Operator : AJ/MA
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 10 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 09 03:09:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:05:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	83421	7.042 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	279049	13.908 ng/ml
2) t 2,2,4-Trimethylpentane	7.441	311021	14.615 ng/ml
3) t n-Heptane	7.751	93209	4.253 ng/ml
4) t Benzene	7.887	110692	4.441 ng/ml
6) t Toluene	10.621	317190	13.526 ng/ml
7) t Ethylbenzene	13.058	98949	4.631 ng/ml
8) t m-Xylene	13.191	198563	9.354 ng/ml
9) t O-Xylene	13.919	198636	9.639 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	206999	10.403 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
Data File : FB026648.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2022 15:01
Operator : AJ/MA
Sample : 10 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
10 GRO STD

Integration File: Calibration.e
Quant Time: Mar 09 03:09:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:05:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

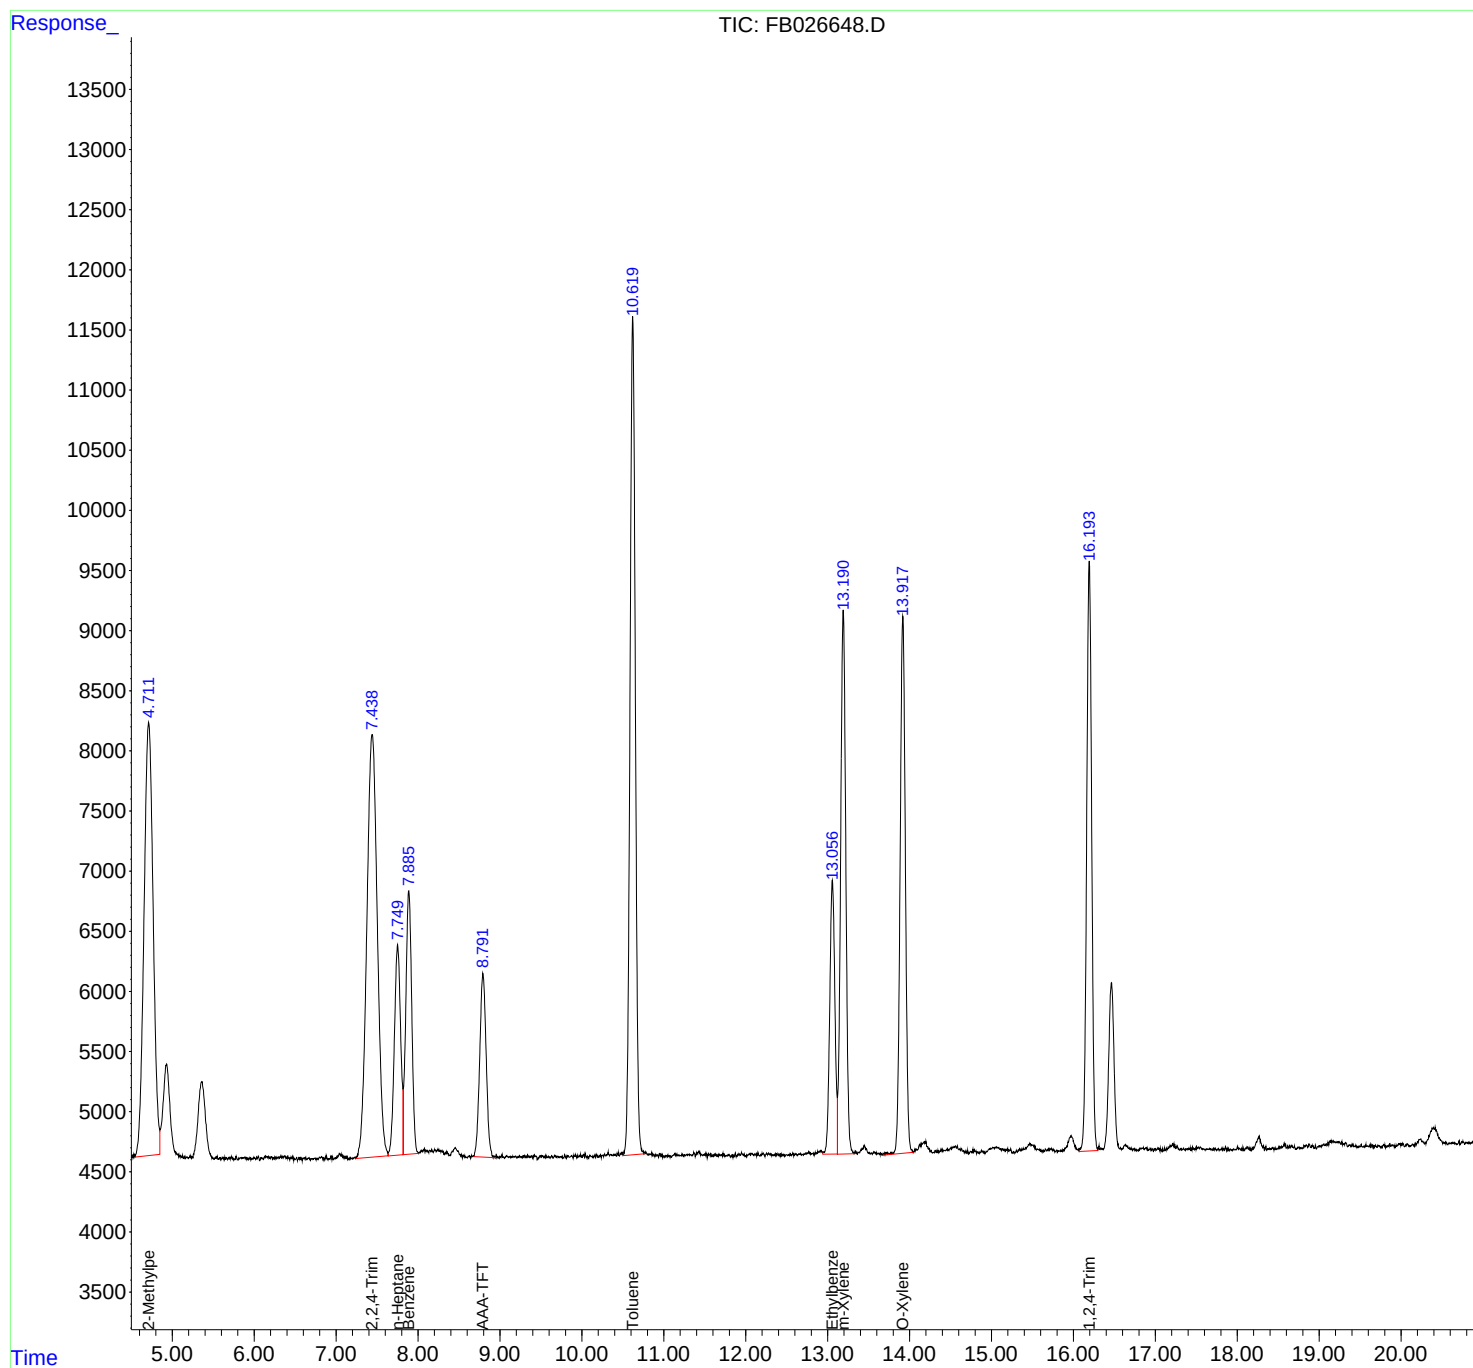


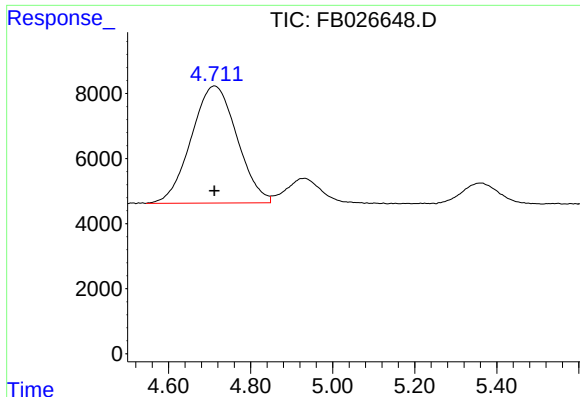

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 279049
Conc: 13.91 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

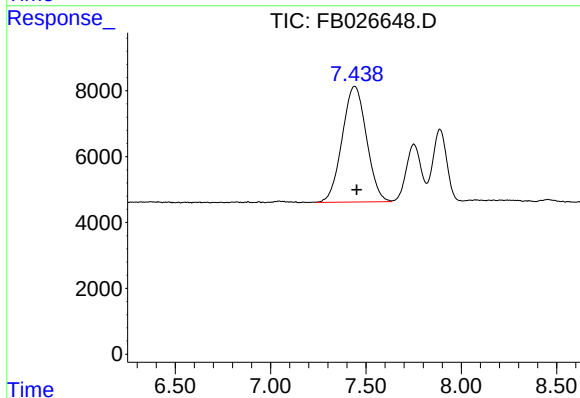


#2 2,2,4-Trimethylpentane

R.T.: 7.441 min
Delta R.T.: -0.010 min
Response: 311021
Conc: 14.61 ng/ml

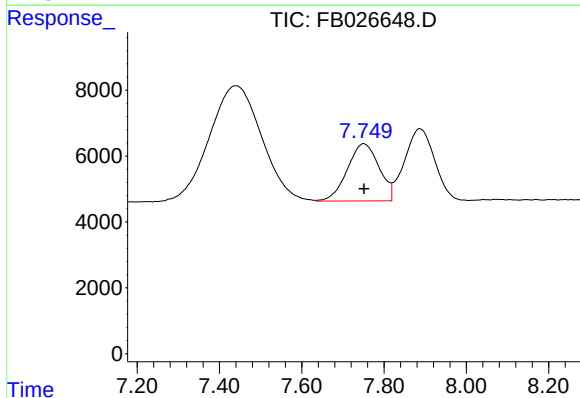


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 93209
Conc: 4.25 ng/ml

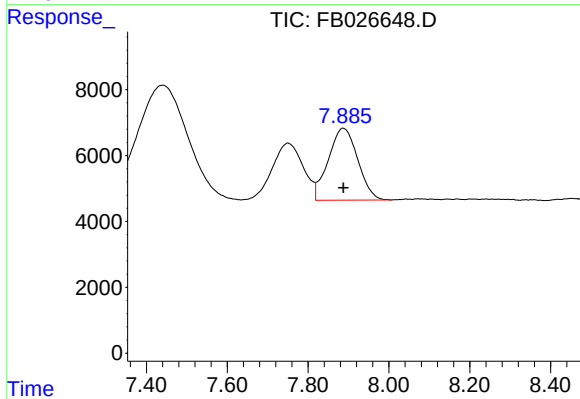

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 110692
Conc: 4.44 ng/ml

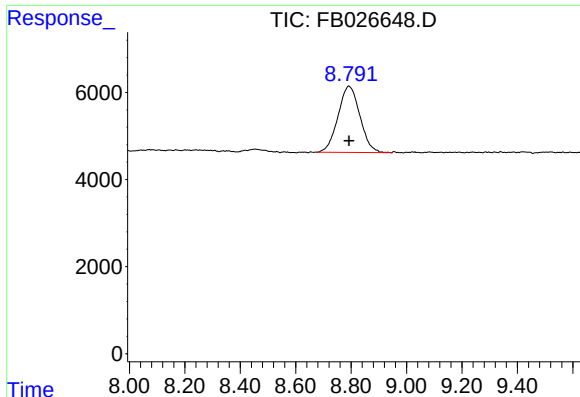

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 83421
Conc: 7.04 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

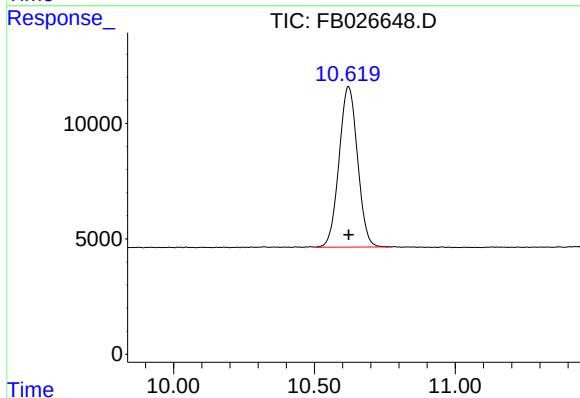


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 317190
Conc: 13.53 ng/ml

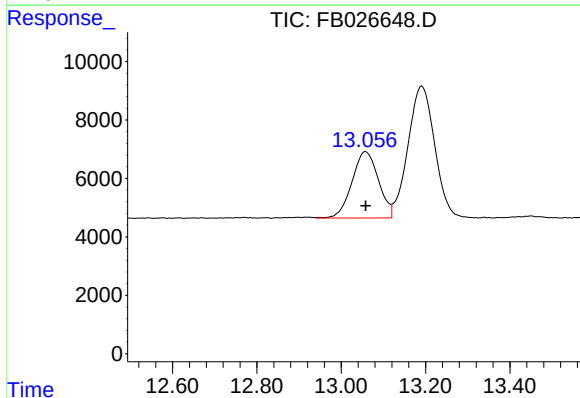


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 98949
Conc: 4.63 ng/ml

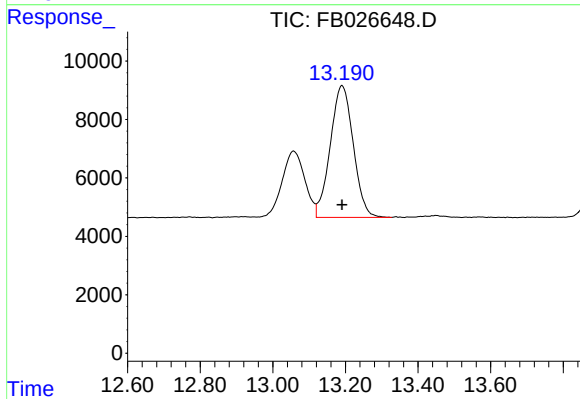

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 198563
Conc: 9.35 ng/ml

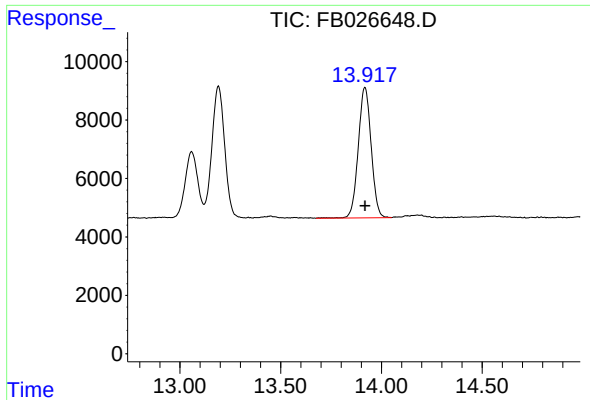

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.000 min
Response: 198636
Conc: 9.64 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

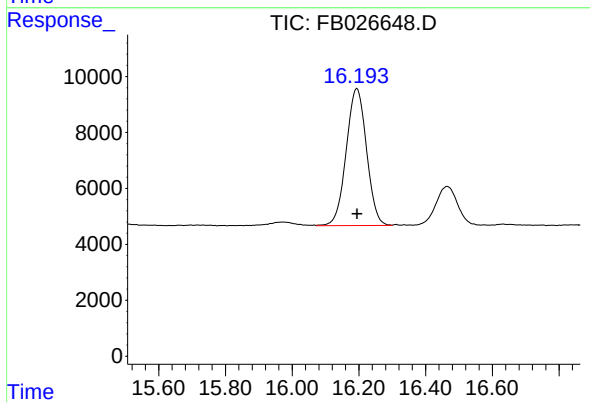

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 206999
Conc: 10.40 ng/ml