

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
 Data File : FB026651.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2022 16:57
 Operator : AJ/MA
 Sample : 100 GRO STD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 100 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 09 03:09:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:05:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	1239644	104.639 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	2960617	147.561 ng/ml
2) t 2,2,4-Trimethylpentane	7.447	3158481	148.416 ng/ml
3) t n-Heptane	7.749	1108453	50.582 ng/ml
4) t Benzene	7.886	1288689	51.698 ng/ml
6) t Toluene	10.621	3577688	152.567 ng/ml
7) t Ethylbenzene	13.059	1074027	50.267 ng/ml
8) t m-Xylene	13.192	2122298	99.974 ng/ml
9) t O-Xylene	13.919	2048728	99.415 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	1897335	95.354 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030822\
Data File : FB026651.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2022 16:57
Operator : AJ/MA
Sample : 100 GRO STD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
100 GRO STD

Integration File: Calibration.e
Quant Time: Mar 09 03:09:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:05:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

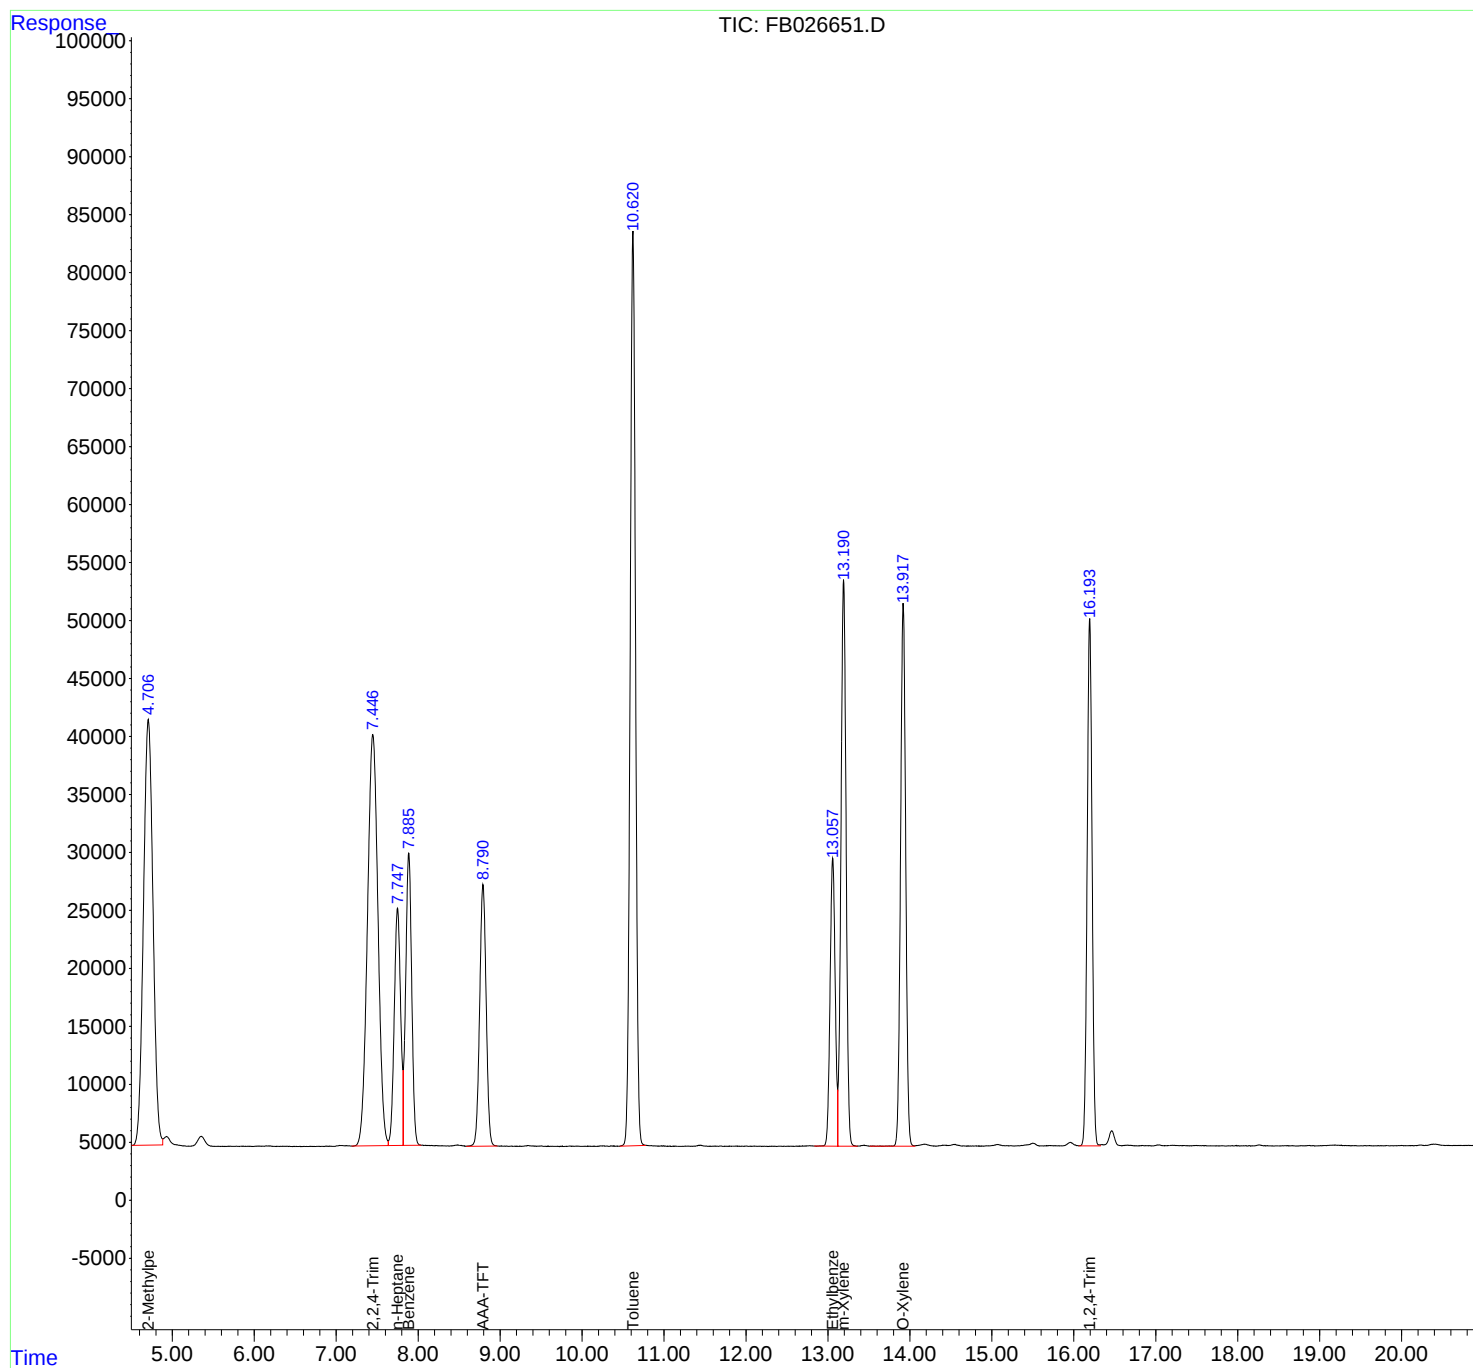


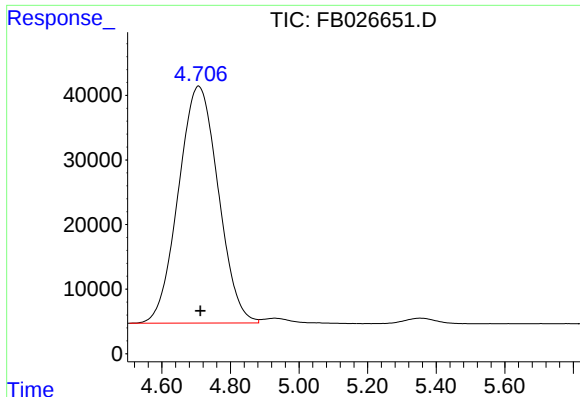

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.005 min
Response: 2960617
Conc: 147.56 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

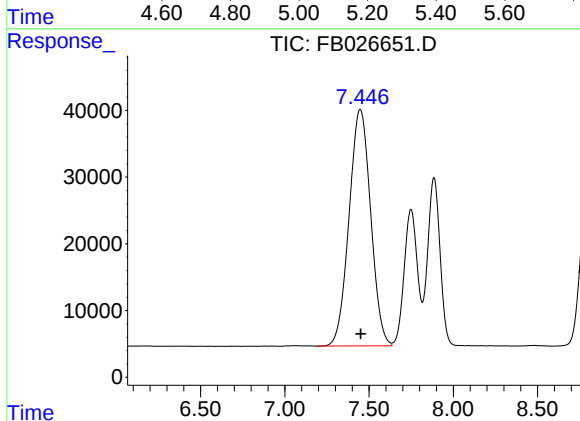


#2 2,2,4-Trimethylpentane

R.T.: 7.447 min
Delta R.T.: -0.004 min
Response: 3158481
Conc: 148.42 ng/ml

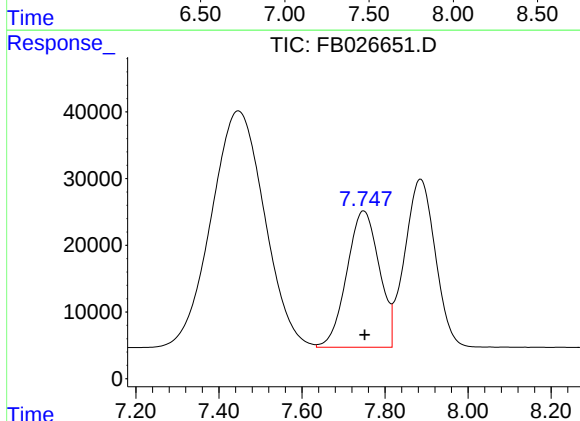


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 1108453
Conc: 50.58 ng/ml

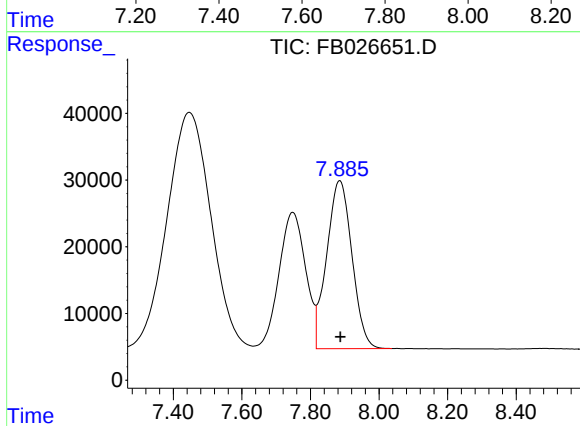

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.002 min
Response: 1288689
Conc: 51.70 ng/ml

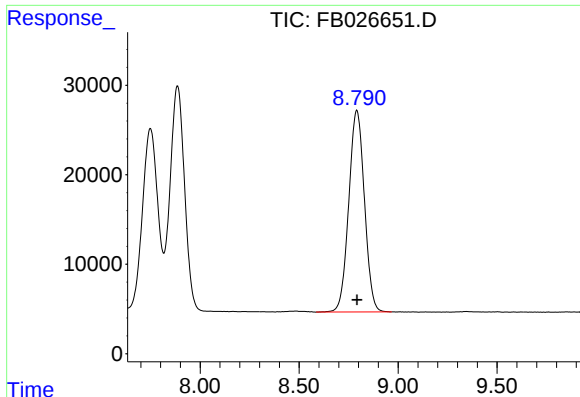

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.001 min
Response: 1239644
Conc: 104.64 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

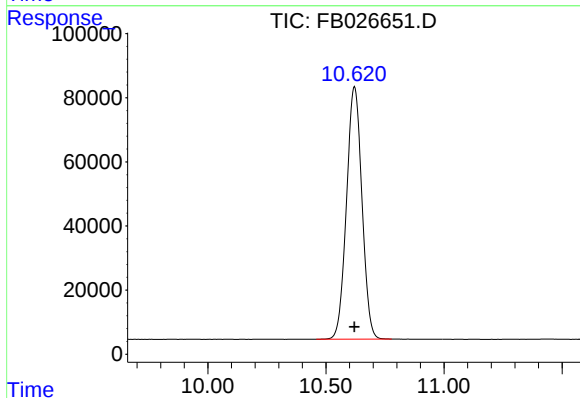


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 3577688
Conc: 152.57 ng/ml

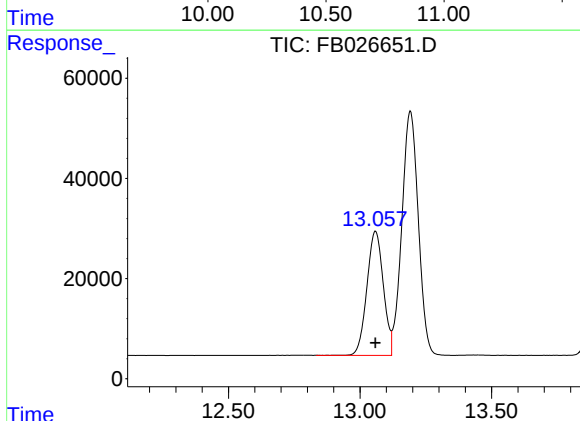


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 1074027
Conc: 50.27 ng/ml

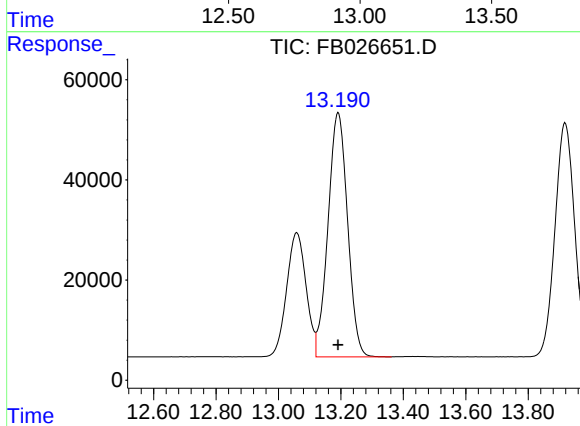

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.000 min
Response: 2122298
Conc: 99.97 ng/ml

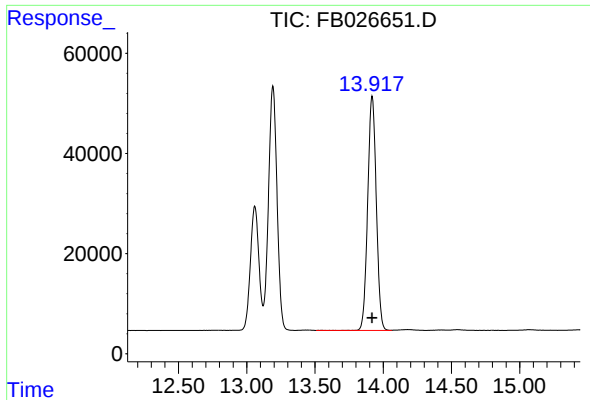

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.000 min
Response: 2048728
Conc: 99.41 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

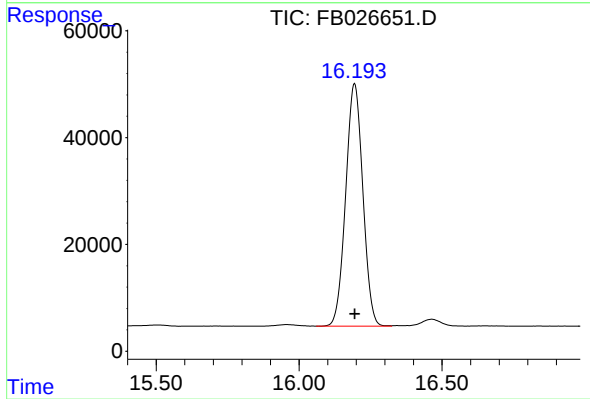

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 1897335
Conc: 95.35 ng/ml