

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030823\
 Data File : FB029442.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2023 4:45
 Operator : YP/AJ
 Sample : 01829-13
 Misc : 5.08G/5.00 ML DI WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 09 05:36:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	114011	9.410 ng/ml
Target Compounds			
4) t Benzene	7.889	22290	1.098 ng/ml
6) t Toluene	10.618	65720	3.329 ng/ml
7) t Ethylbenzene	13.056	54034	2.902 ng/ml
8) t m-Xylene	13.185	89099	4.789 ng/ml
9) t O-Xylene	13.914	35302	1.917 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	18338	0.985 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030823\
Data File : FB029442.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2023 4:45
Operator : YP/AJ
Sample : 01829-13
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 09 05:36:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

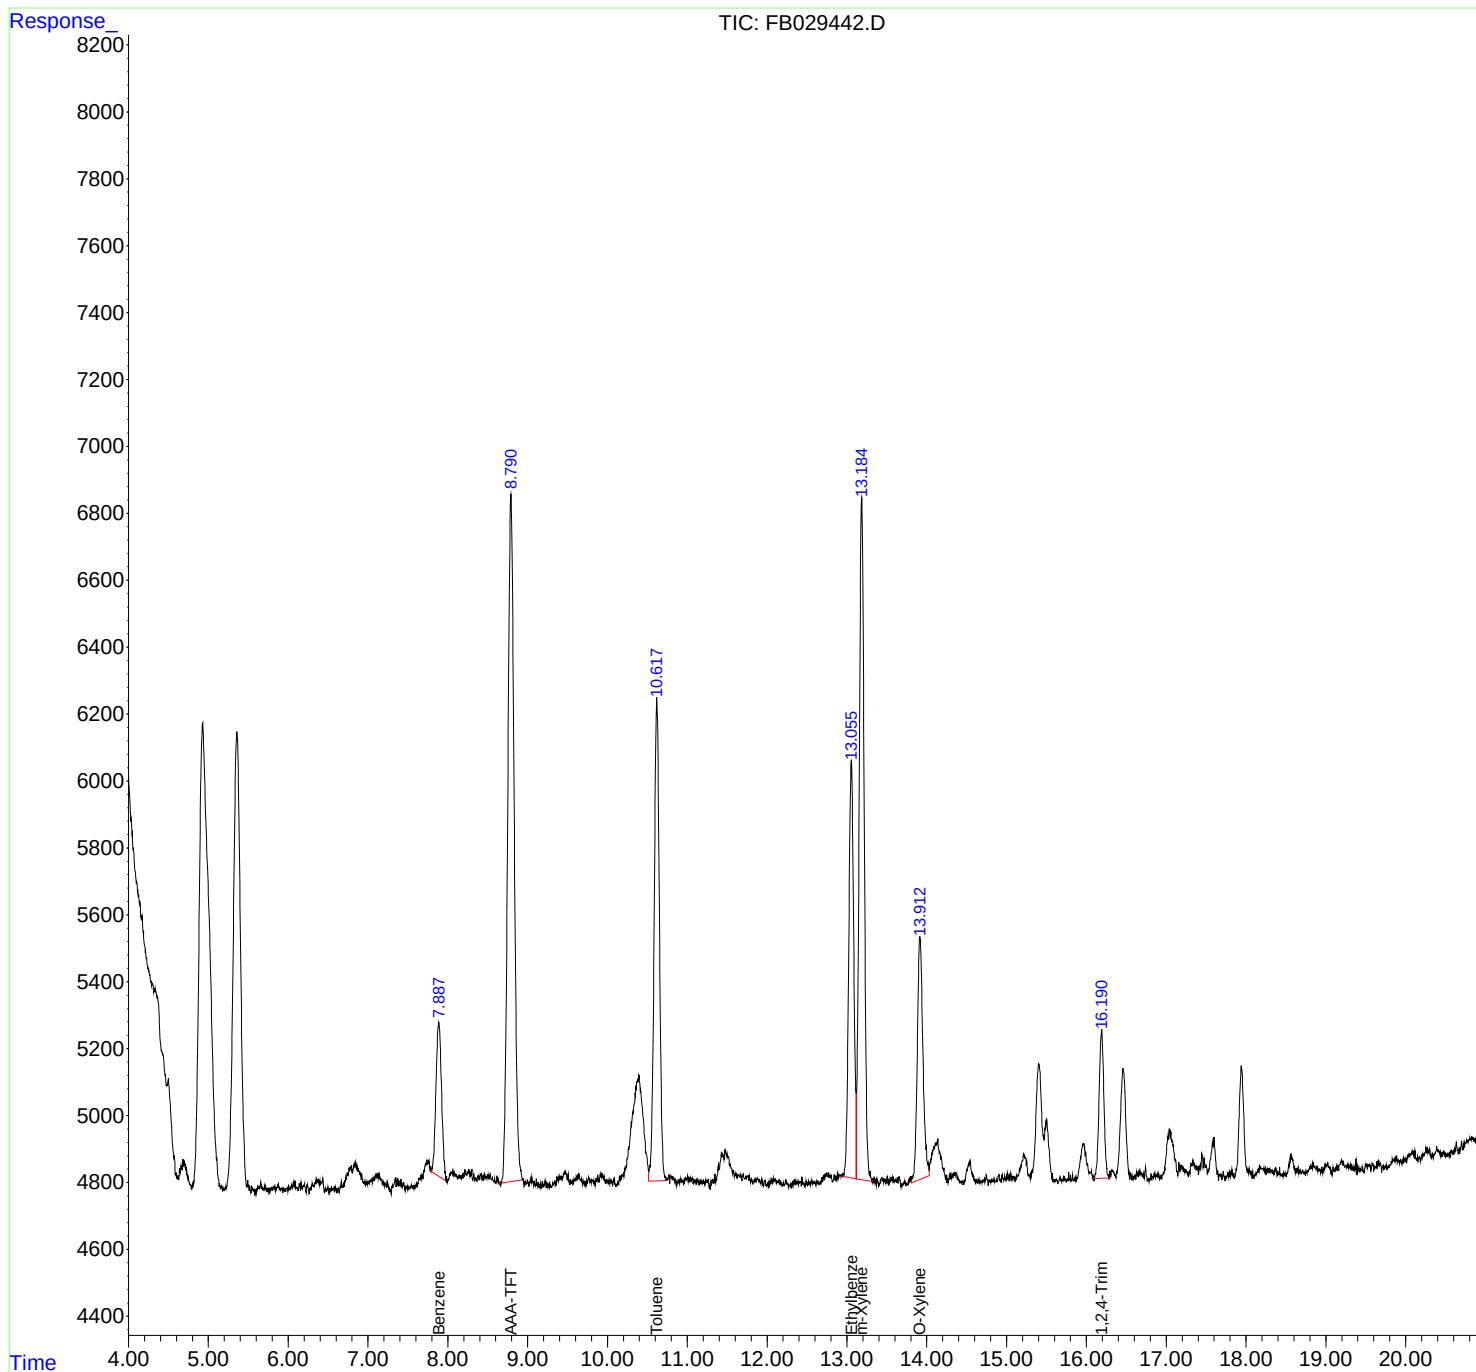


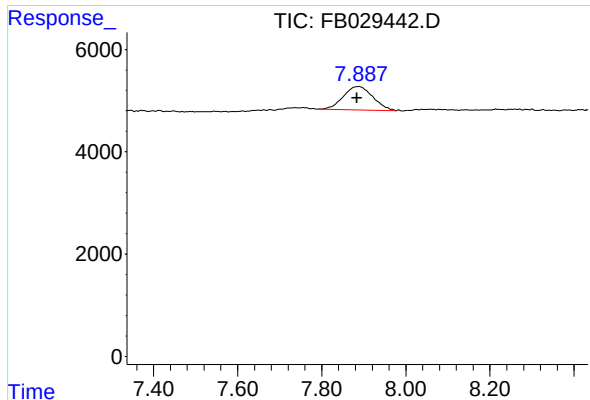

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.006 min
Response: 22290
Conc: 1.10 ng/ml

Instrument :
FID_B
ClientSampleId :

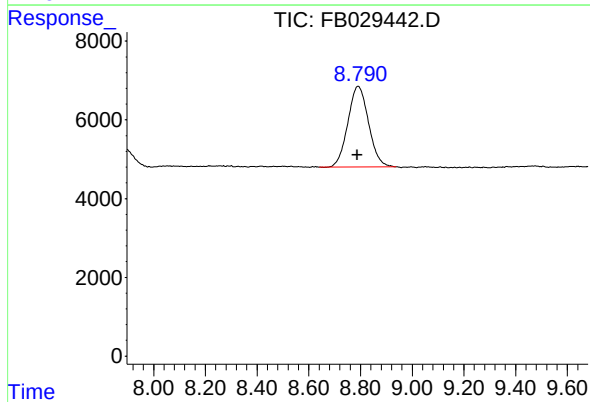


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.003 min
Response: 114011
Conc: 9.41 ng/ml

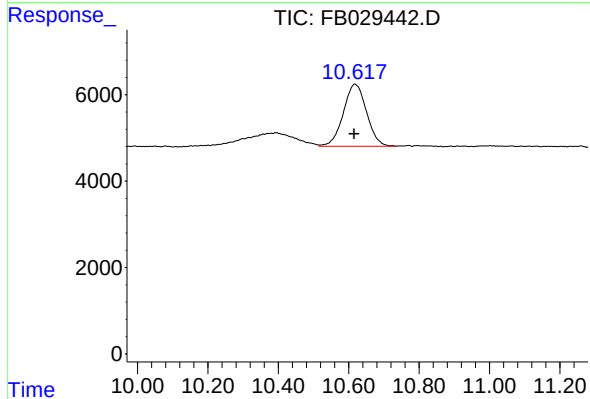


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.002 min
Response: 65720
Conc: 3.33 ng/ml

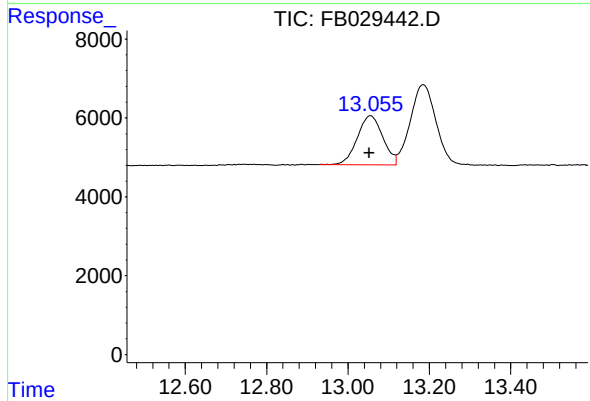

#7 Ethylbenzene


R.T.: 13.056 min
Delta R.T.: 0.004 min
Response: 54034
Conc: 2.90 ng/ml

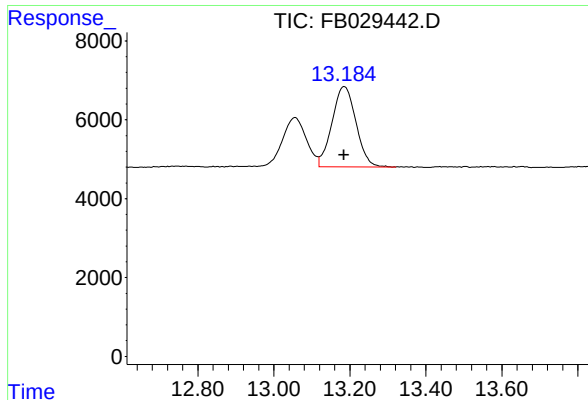

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 89099
Conc: 4.79 ng/ml

Instrument :
FID_B
ClientSampleId :

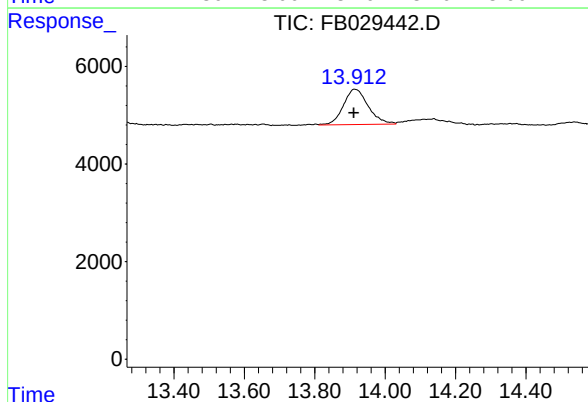

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.002 min
Response: 35302
Conc: 1.92 ng/ml

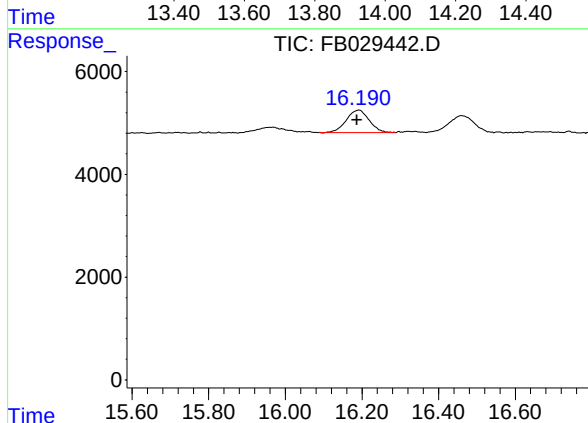

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.005 min
Response: 18338
Conc: 0.98 ng/ml