

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030823\
 Data File : FB029416.D
 Signal(s) : FID2B.CH
 Acq On : 8 Mar 2023 10:25
 Operator : YP/AJ
 Sample : BSF0308S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0308S1

Integration File: Calibration.e
 Quant Time: Mar 09 00:48:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	264329	21.817 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	479442	31.246 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	534027	31.703 ng/ml
3) t n-Heptane	7.751	185618	10.732 ng/ml
4) t Benzene	7.887	218729	10.776 ng/ml
6) t Toluene	10.620	643235	32.587 ng/ml
7) t Ethylbenzene	13.057	199435	10.712 ng/ml
8) t m-Xylene	13.190	395095	21.238 ng/ml
9) t O-Xylene	13.917	377834	20.520 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	356082	19.118 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030823\
Data File : FB029416.D
Signal(s) : FID2B.CH
Acq On : 8 Mar 2023 10:25
Operator : YP/AJ
Sample : BSF0308S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0308S1

Integration File: Calibration.e
Quant Time: Mar 09 00:48:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

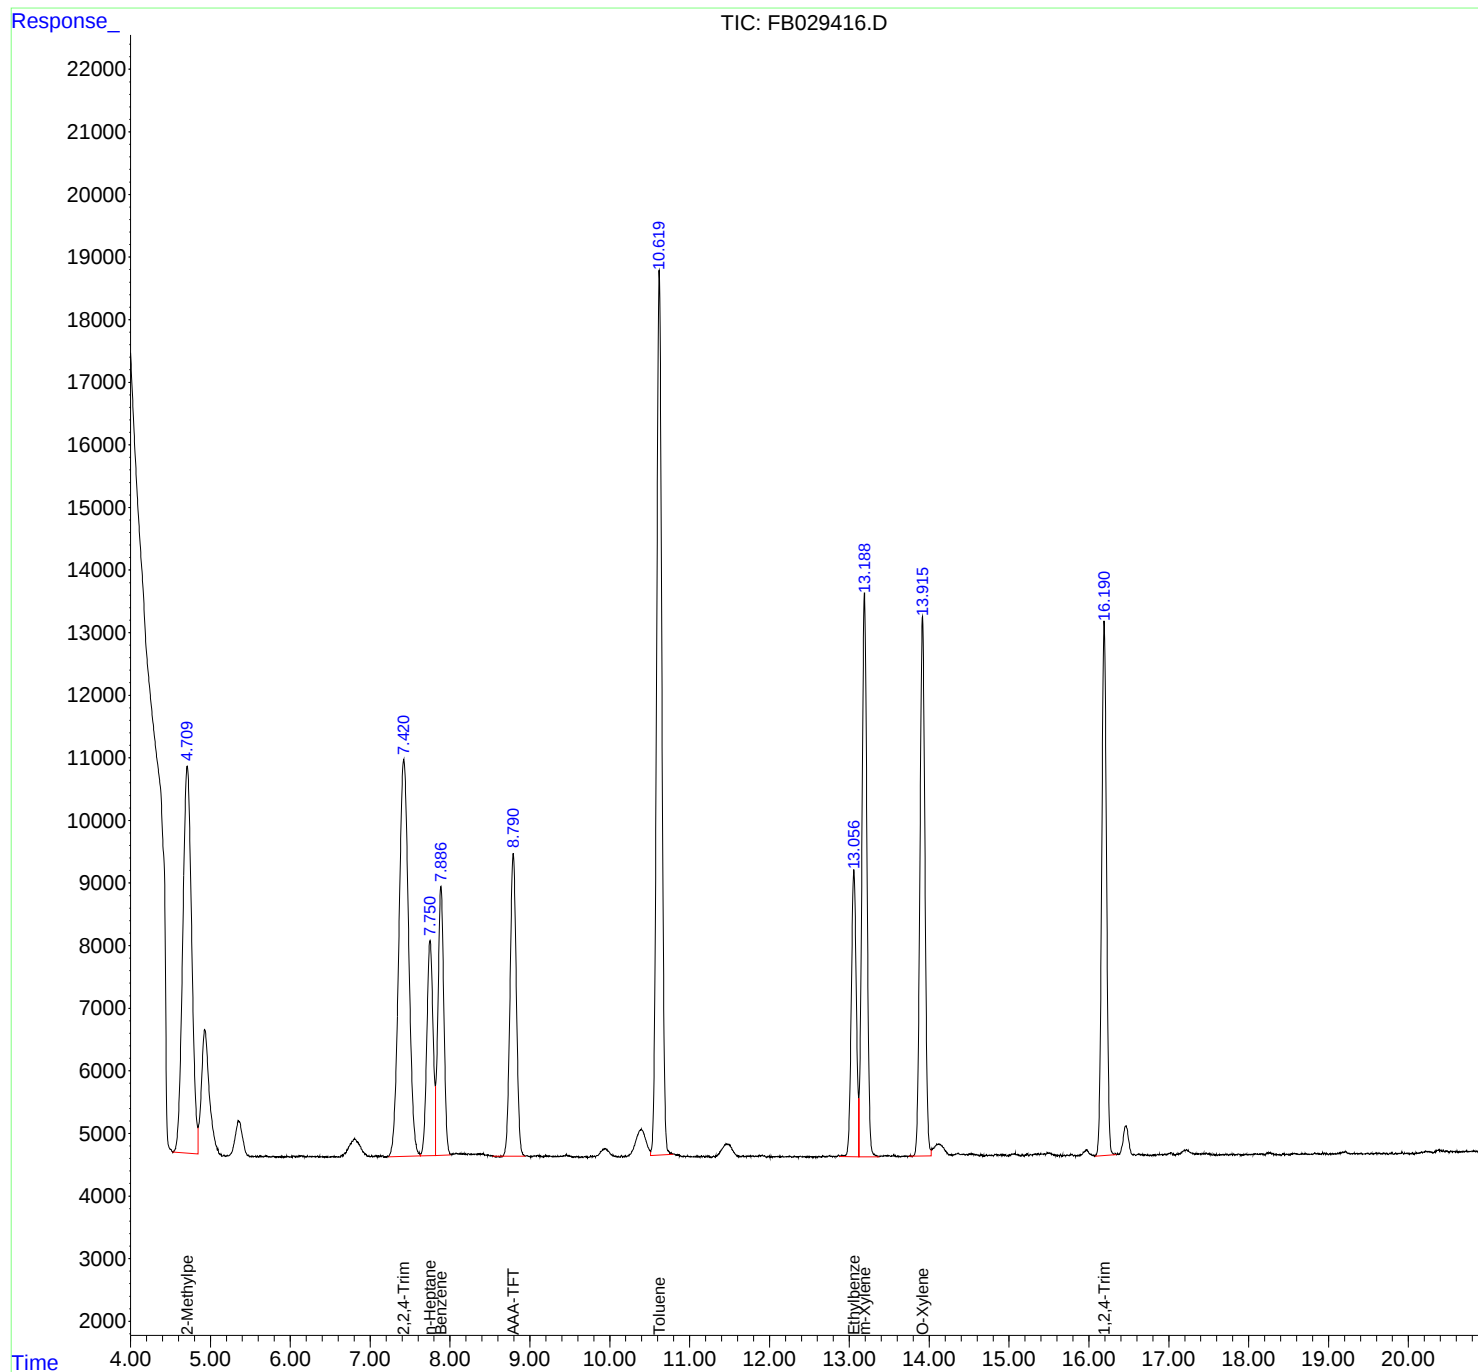


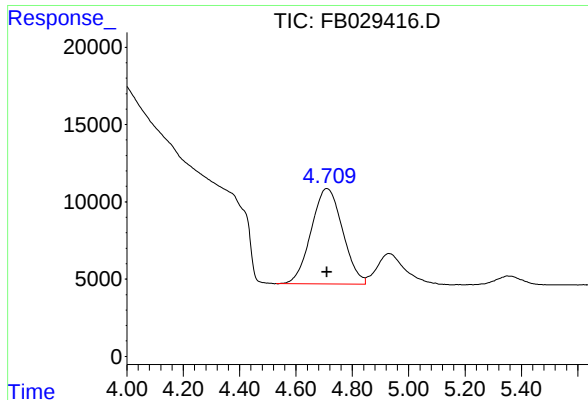

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 479442
Conc: 31.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S1

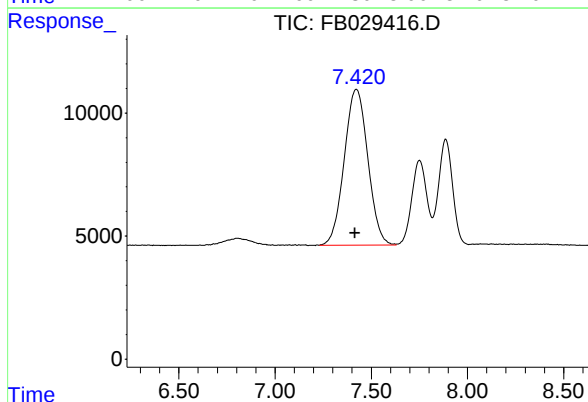


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.006 min
Response: 534027
Conc: 31.70 ng/ml

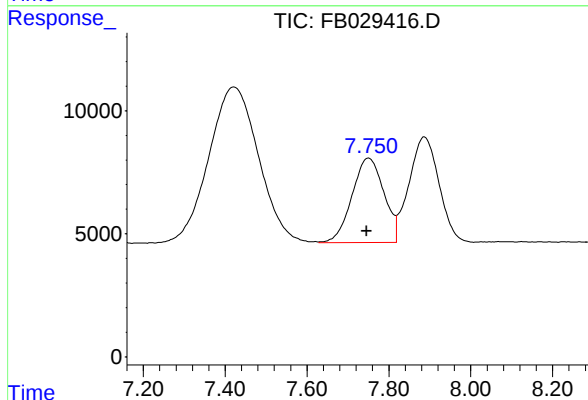


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.005 min
Response: 185618
Conc: 10.73 ng/ml

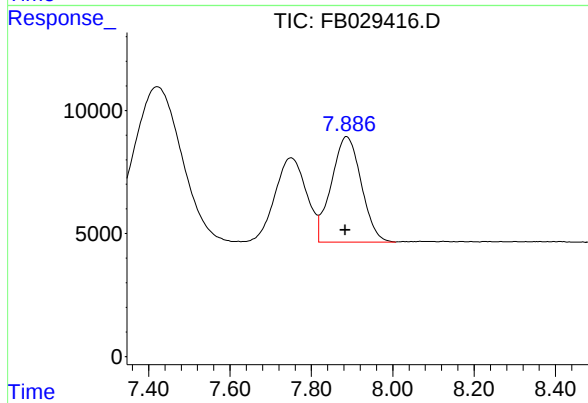

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.004 min
Response: 218729
Conc: 10.78 ng/ml

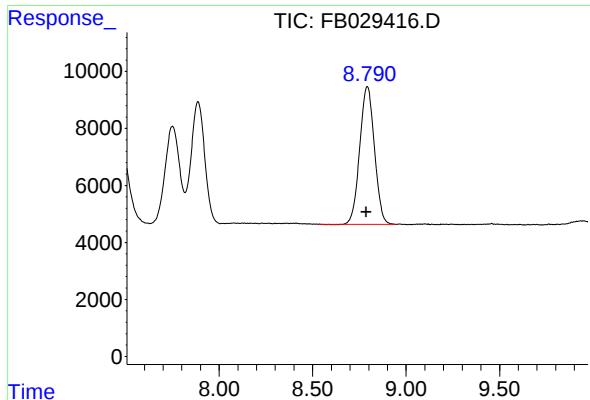

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.004 min
Response: 264329
Conc: 21.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S1

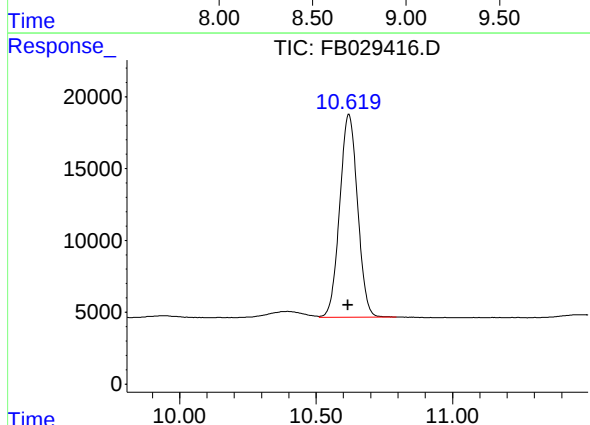


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.004 min
Response: 643235
Conc: 32.59 ng/ml

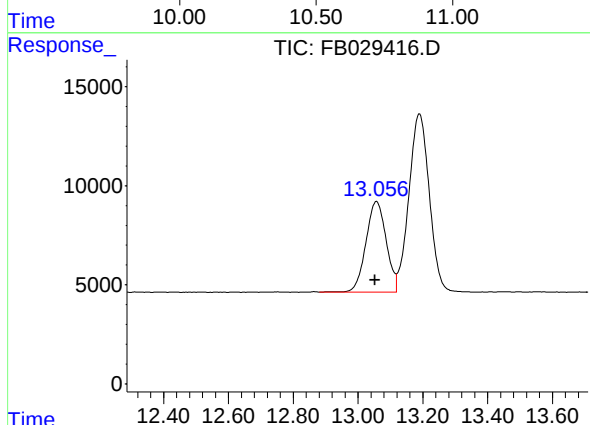


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.004 min
Response: 199435
Conc: 10.71 ng/ml

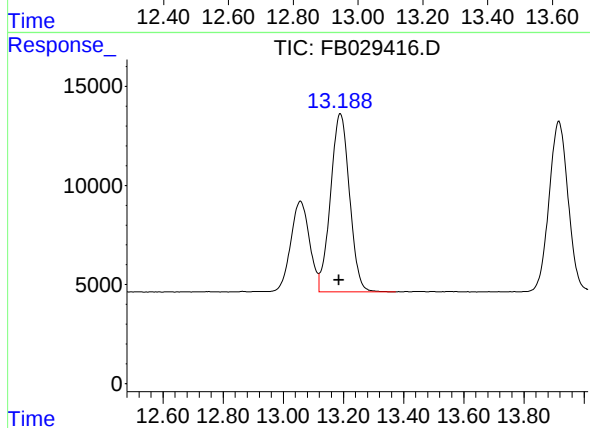

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.005 min
Response: 395095
Conc: 21.24 ng/ml

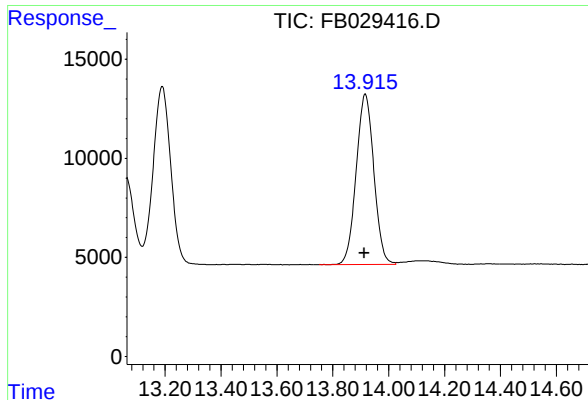

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.004 min
Response: 377834
Conc: 20.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S1

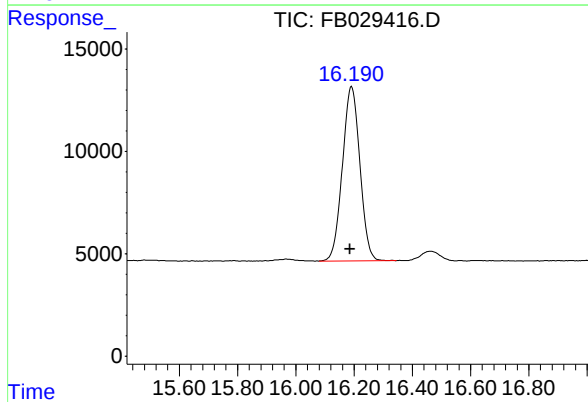

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.004 min
Response: 356082
Conc: 19.12 ng/ml