

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB030823\  
Data File : FB029419.D  
Signal(s) : FID2B.CH  
Acq On : 8 Mar 2023 12:17  
Operator : YP/AJ  
Sample : 01829-01  
Misc : 5.08G/5.00 ML DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SS-01-20230306

Integration File: Calibration.e  
Quant Time: Mar 09 00:48:53 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030123.M  
Quant Title :  
QLast Update : Wed Mar 01 12:30:24 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds  
-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB030823\  
Data File : FB029419.D  
Signal(s) : FID2B.CH  
Acq On : 8 Mar 2023 12:17  
Operator : YP/AJ  
Sample : 01829-01  
Misc : 5.08G/5.00 ML DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SS-01-20230306

Integration File: Calibration.e  
Quant Time: Mar 09 00:48:53 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030123.M  
Quant Title :  
QLast Update : Wed Mar 01 12:30:24 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

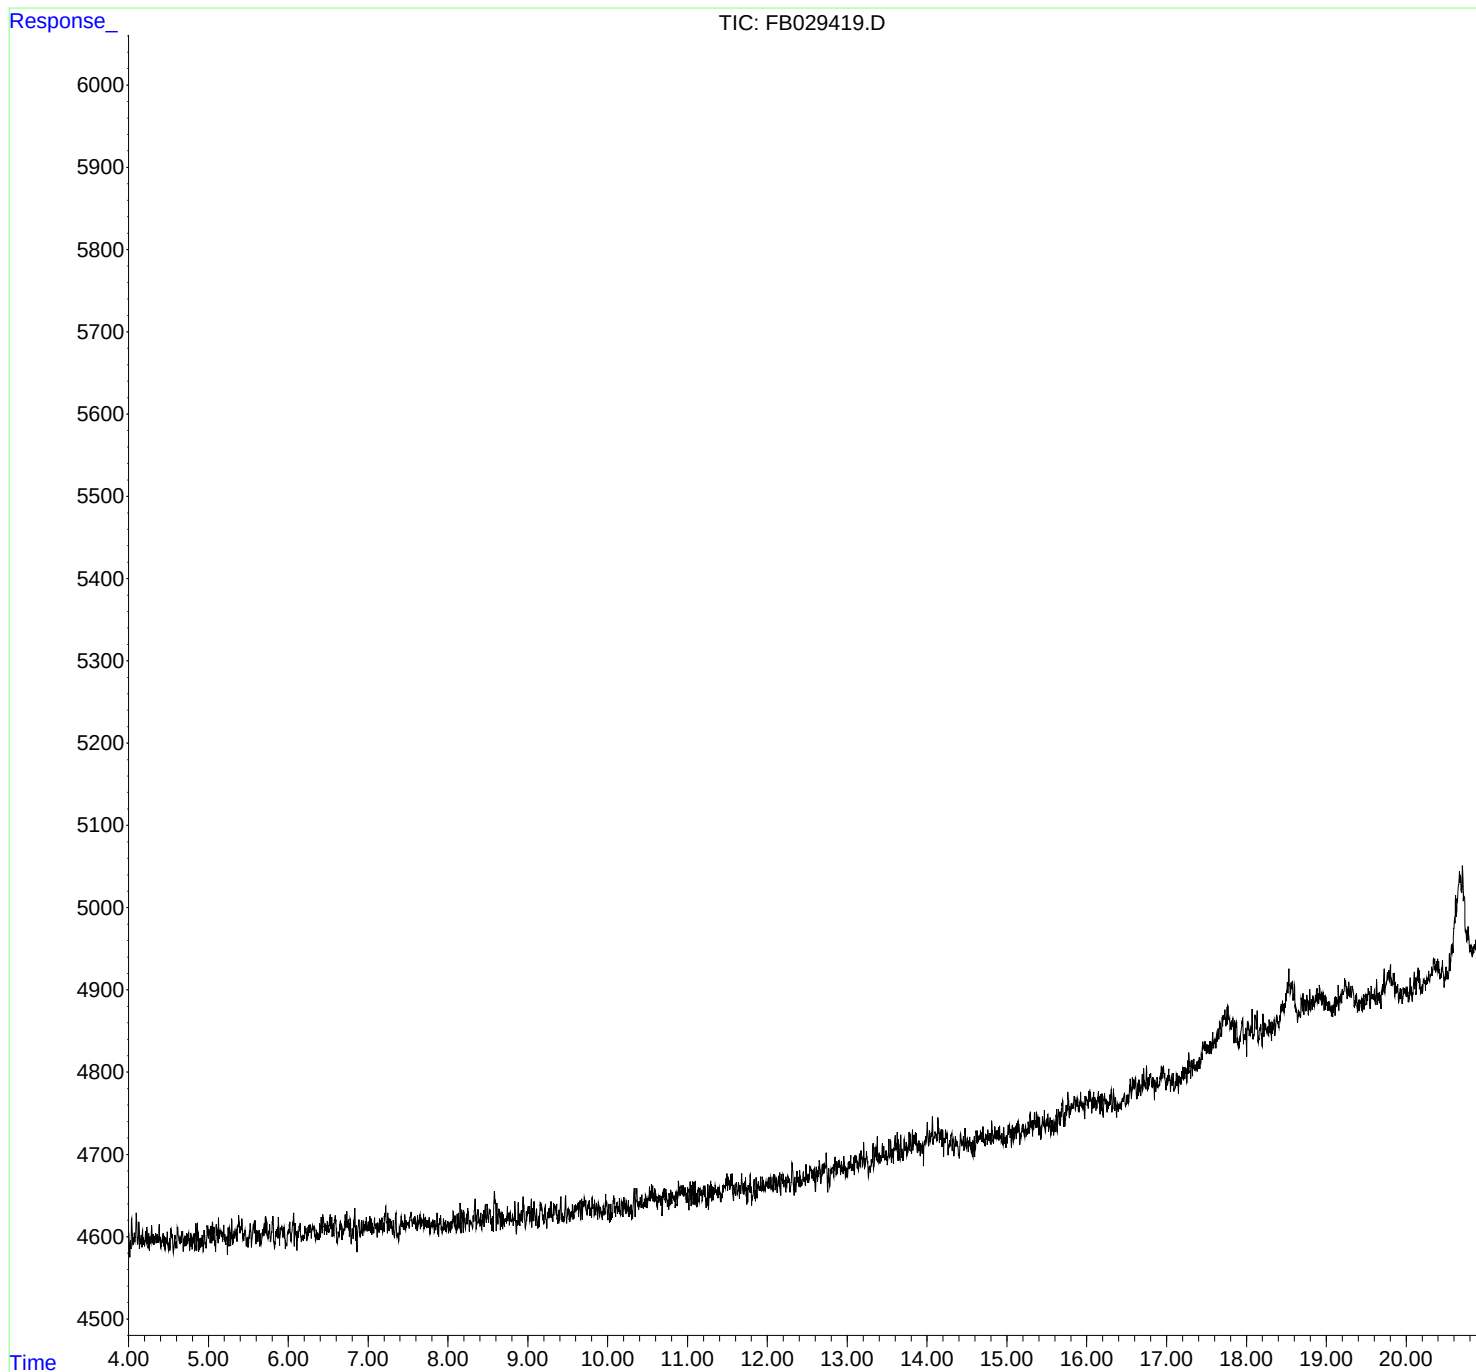

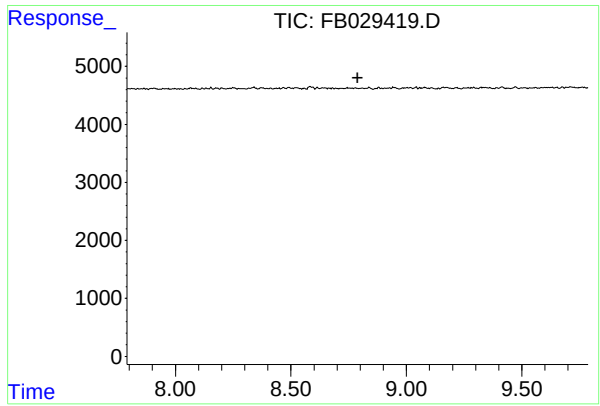

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.788 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_B  
ClientSampleId :  
SS-01-20230306