

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030823\
 Data File : FB029443.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2023 5:22
 Operator : YP/AJ
 Sample : BSF0308S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0308S2

Integration File: Calibration.e
 Quant Time: Mar 09 05:36:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
 Quant Title :
 QLast Update : Wed Mar 01 12:30:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	255418	21.082 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	484386	31.568 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	554573	32.922 ng/ml
3) t n-Heptane	7.750	184815	10.686 ng/ml
4) t Benzene	7.886	227719	11.219 ng/ml
6) t Toluene	10.619	655620	33.215 ng/ml
7) t Ethylbenzene	13.055	203828	10.948 ng/ml
8) t m-Xylene	13.188	402275	21.624 ng/ml
9) t O-Xylene	13.915	393207	21.355 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	368300	19.774 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030823\
Data File : FB029443.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2023 5:22
Operator : YP/AJ
Sample : BSF0308S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0308S2

Integration File: Calibration.e
Quant Time: Mar 09 05:36:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030123.M
Quant Title :
QLast Update : Wed Mar 01 12:30:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

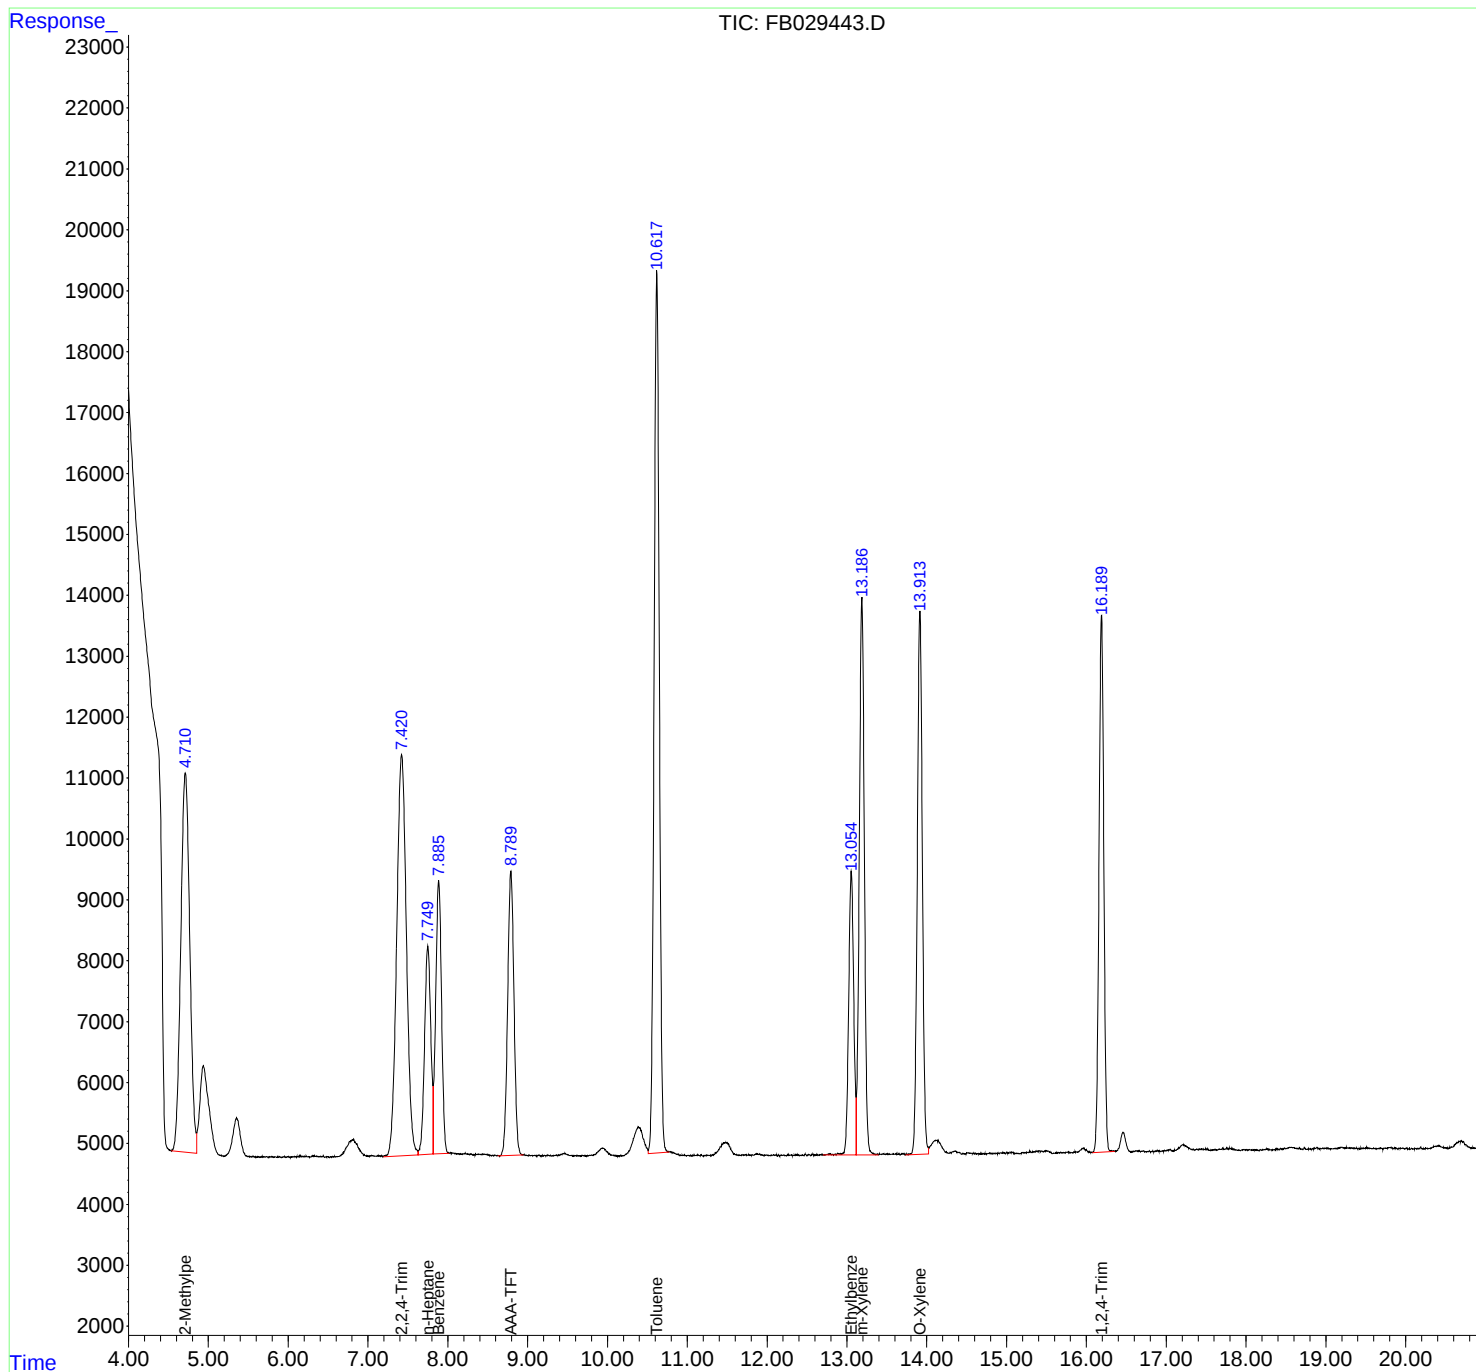


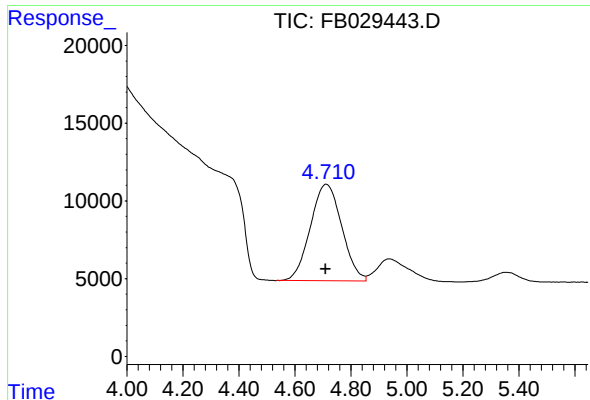

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.002 min
Response: 484386
Conc: 31.57 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S2

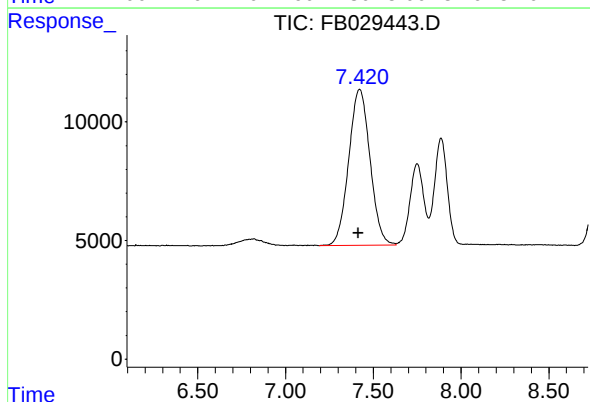


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.006 min
Response: 554573
Conc: 32.92 ng/ml

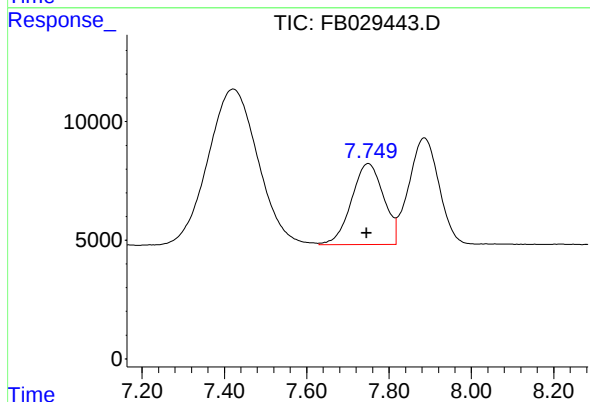


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.004 min
Response: 184815
Conc: 10.69 ng/ml

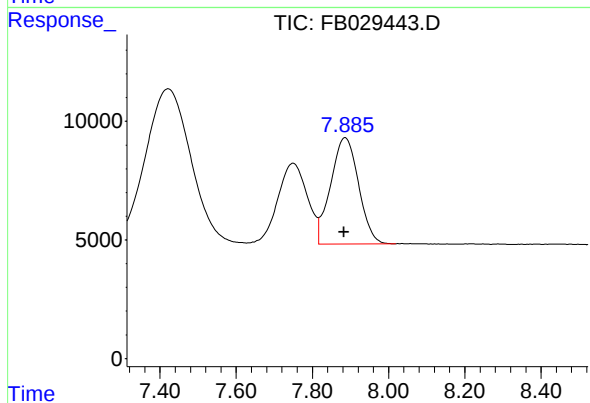

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.003 min
Response: 227719
Conc: 11.22 ng/ml

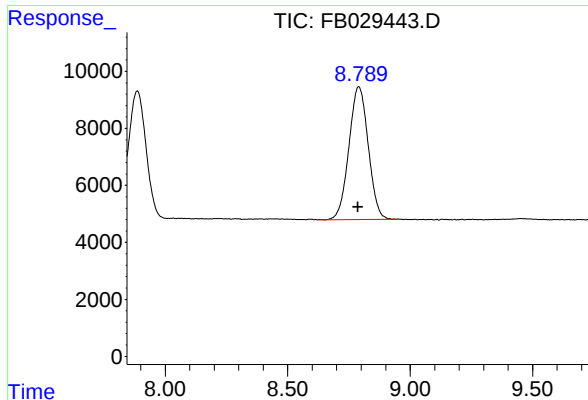

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.003 min
Response: 255418
Conc: 21.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S2

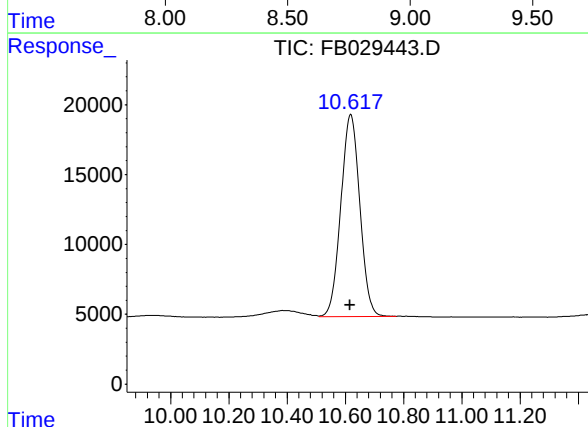


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.003 min
Response: 655620
Conc: 33.21 ng/ml

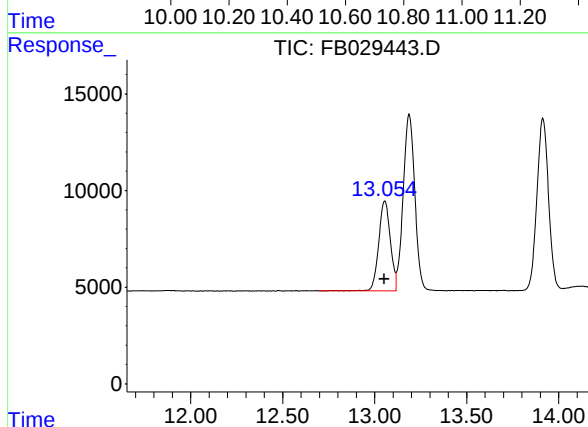


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.002 min
Response: 203828
Conc: 10.95 ng/ml

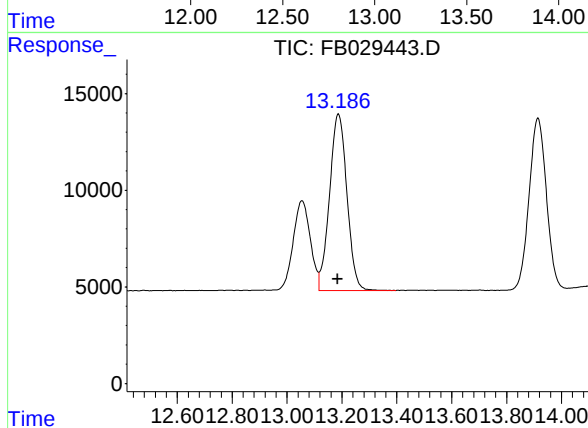

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.003 min
Response: 402275
Conc: 21.62 ng/ml

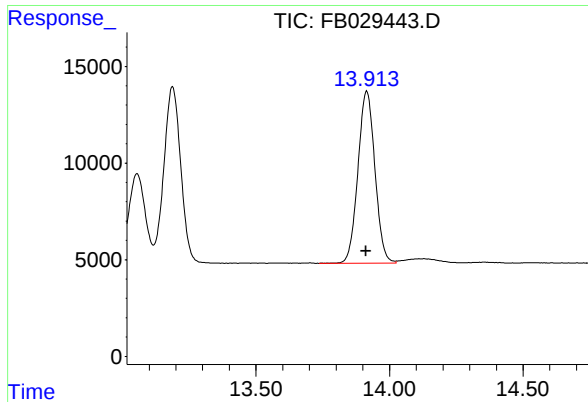

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.003 min
Response: 393207
Conc: 21.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0308S2

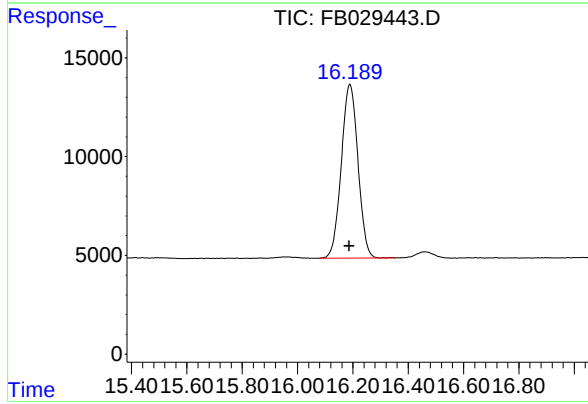

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.003 min
Response: 368300
Conc: 19.77 ng/ml