

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
 Data File : FB023810.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2020 16:52
 Operator : DD/AJ
 Sample : BSF0309S2
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 10 13:47:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	452771	21.509 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	877729	28.401 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	891004	26.423 ng/ml
3) t n-Heptane	7.759	296579	8.952 ng/ml
4) t Benzene	7.894	396875	9.478 ng/ml
6) t Toluene	10.632	1143940	28.056 ng/ml
7) t Ethylbenzene	13.072	352094	9.216 ng/ml
8) t m-Xylene	13.205	675800	18.356 ng/ml
9) t O-Xylene	13.933	662549	18.629 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	578942	19.110 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
Data File : FB023810.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2020 16:52
Operator : DD/AJ
Sample : BSF0309S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 10 13:47:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

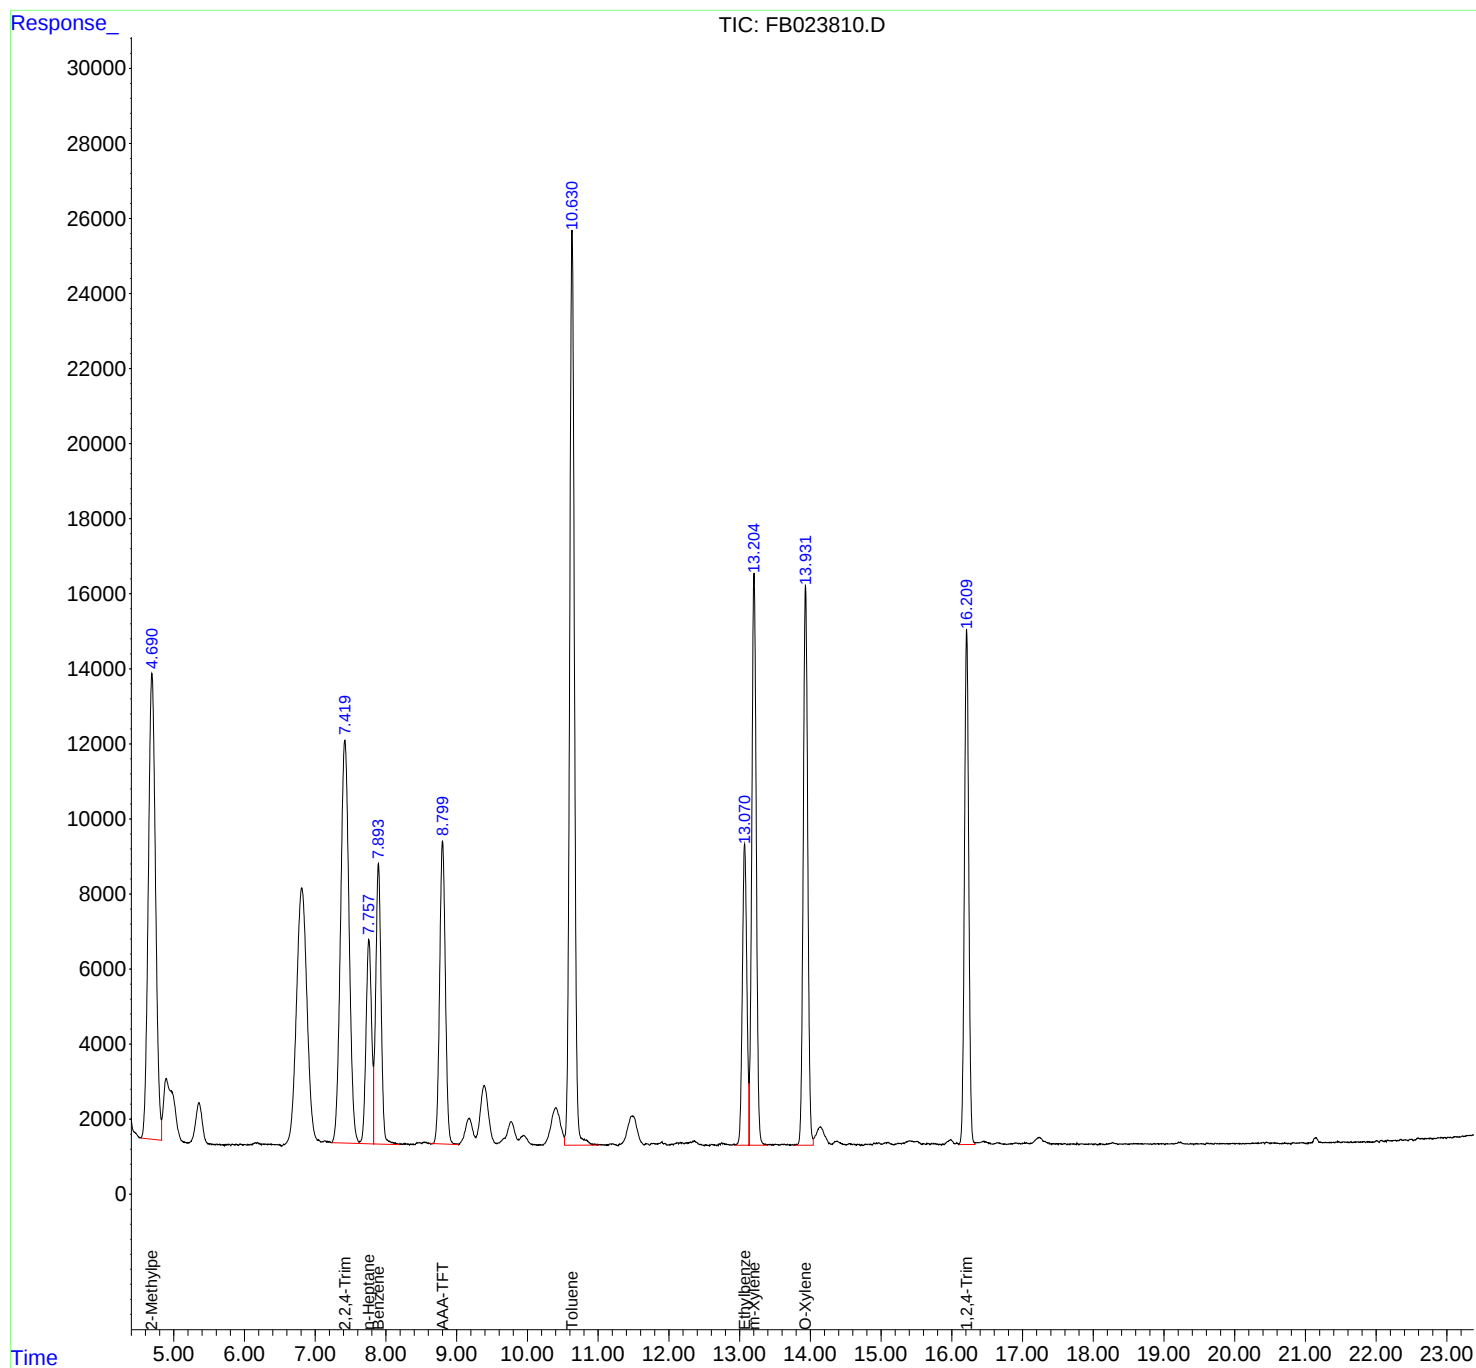


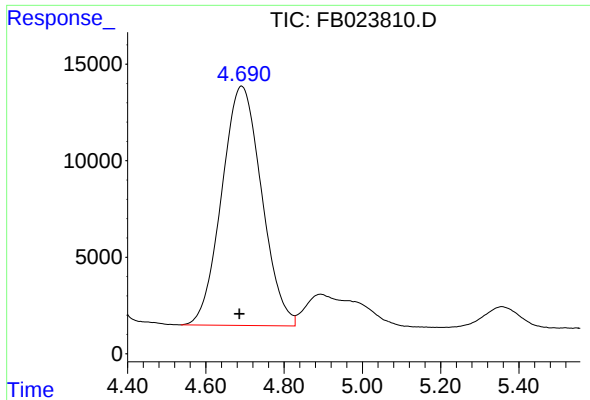

#1 2-Methylpentane


R.T.: 4.692 min
Delta R.T.: 0.006 min
Response: 877729
Conc: 28.40 ng/ml

Instrument :
FID_B
ClientSampleId :

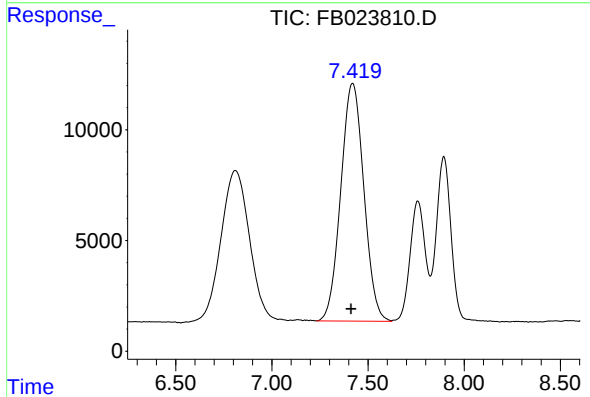


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.007 min
Response: 891004
Conc: 26.42 ng/ml

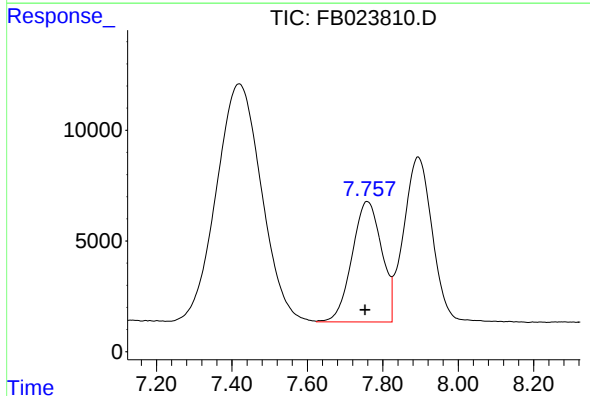


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.006 min
Response: 296579
Conc: 8.95 ng/ml

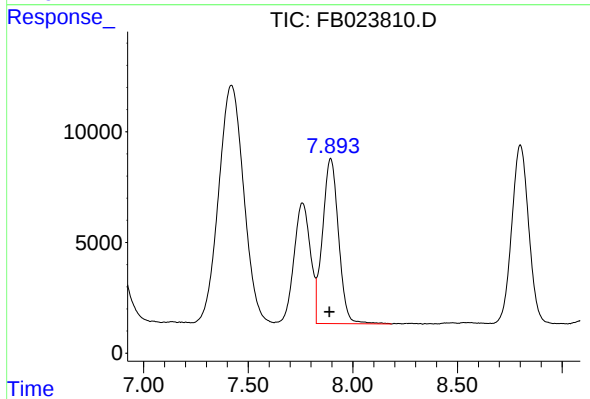

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.006 min
Response: 396875
Conc: 9.48 ng/ml

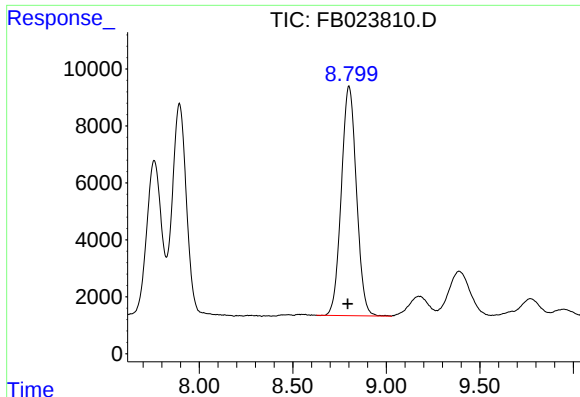

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.006 min
Response: 452771
Conc: 21.51 ng/ml

Instrument :
FID_B
ClientSampleId :

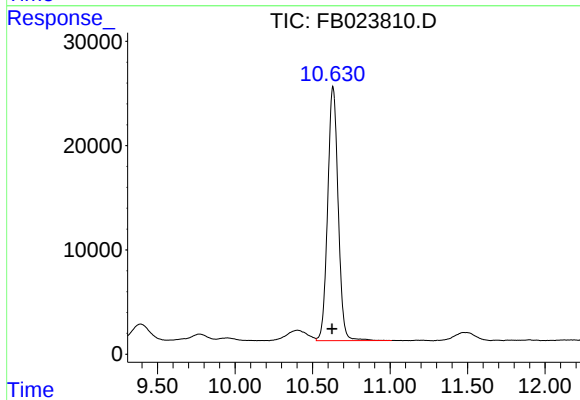


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.005 min
Response: 1143940
Conc: 28.06 ng/ml

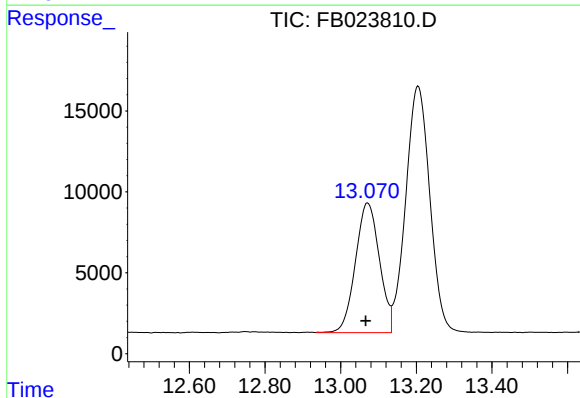


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.005 min
Response: 352094
Conc: 9.22 ng/ml

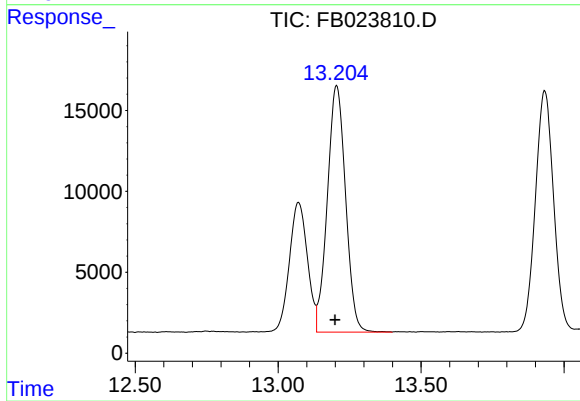

#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.005 min
Response: 675800
Conc: 18.36 ng/ml

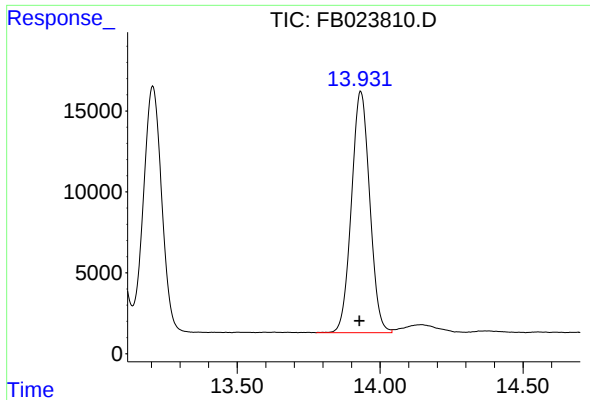

#9 O-Xylene


R.T.: 13.933 min

Delta R.T.: 0.005 min

Response: 662549

Conc: 18.63 ng/ml

Instrument :
FID_B
ClientSampleId :

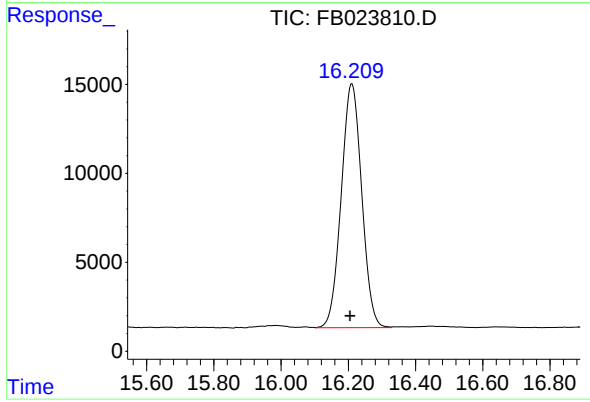

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min

Delta R.T.: 0.005 min

Response: 578942

Conc: 19.11 ng/ml