

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
Data File : FB023815.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2020 19:25
Operator : DD/AJ
Sample : L1852-05
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 10 13:47:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	340238	16.163 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	3699	0.120 ng/ml
3) t n-Heptane	7.750	230	0.007 ng/ml
6) t Toluene	10.658	1502	0.037 ng/ml
8) t m-Xylene	13.201	816	0.022 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
Data File : FB023815.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2020 19:25
Operator : DD/AJ
Sample : L1852-05
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 10 13:47:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

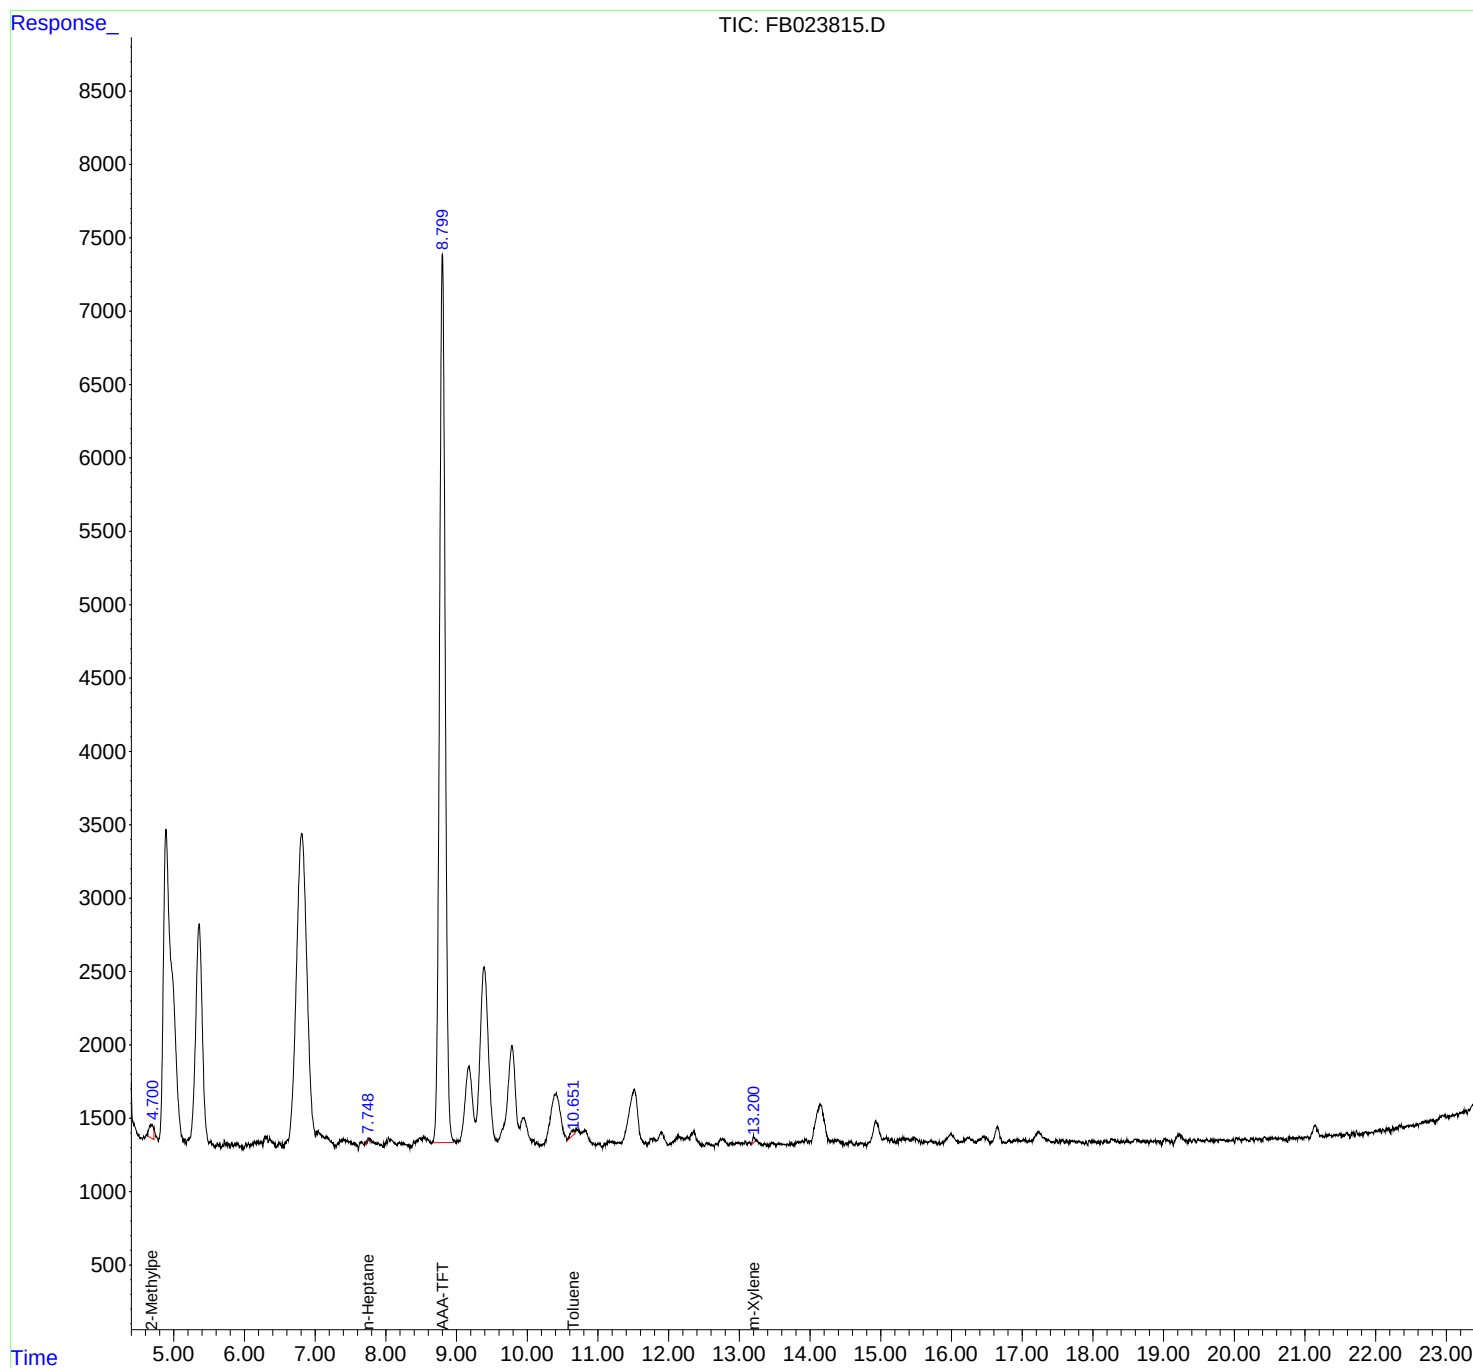


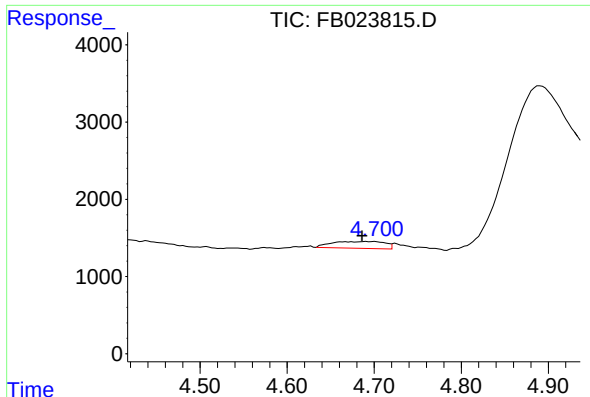

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.005 min
Response: 3699
Conc: 0.12 ng/ml

Instrument :
FID_B
ClientSampleId :

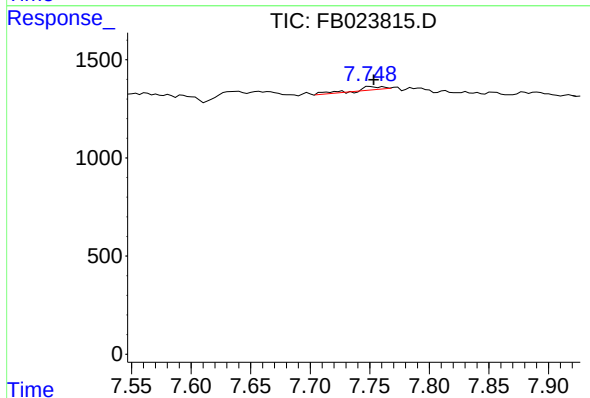


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.004 min
Response: 230
Conc: 0.01 ng/ml

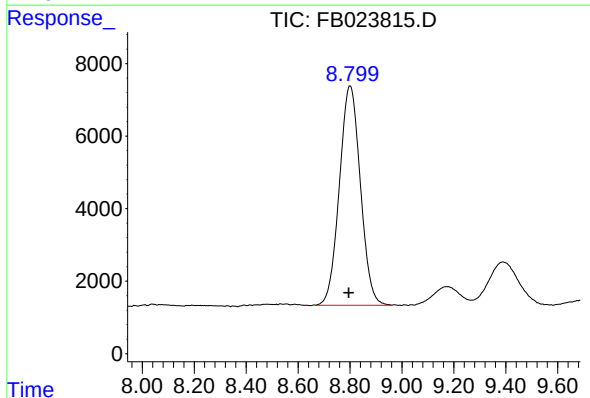


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.006 min
Response: 340238
Conc: 16.16 ng/ml

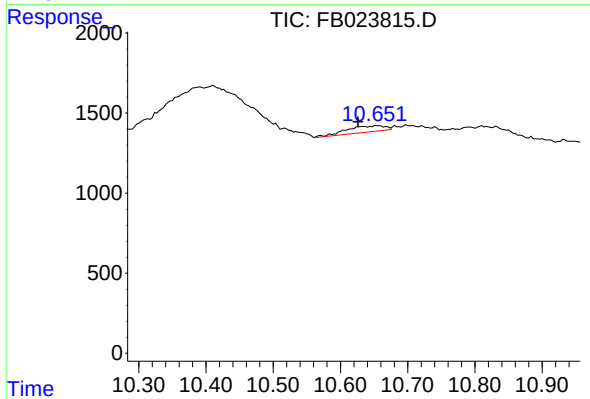

#6 Toluene

R.T.: 10.658 min
Delta R.T.: 0.032 min
Response: 1502
Conc: 0.04 ng/ml

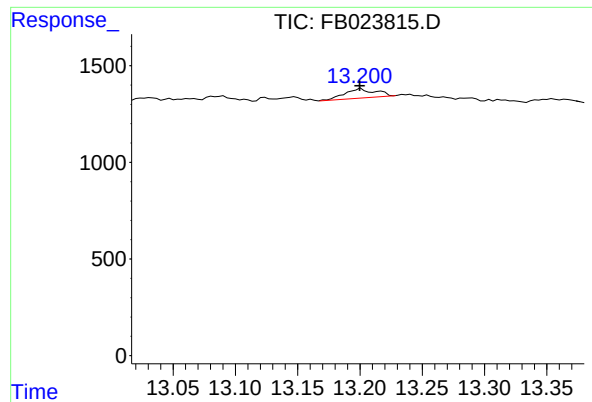

#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.001 min
Response: 816
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :