

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
 Data File : FB023821.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2020 22:59
 Operator : DD/AJ
 Sample : L1852-10
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 10 13:48:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	362623	17.226 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.686	1889	0.061 ng/ml
2) t	2,2,4-Trimethylpentane	7.407	247	0.007 ng/ml
3) t	n-Heptane	7.768	238	0.007 ng/ml
6) t	Toluene	10.632	3669	0.090 ng/ml
7) t	Ethylbenzene	13.065	3523	0.092 ng/ml
8) t	m-Xylene	13.201	4575	0.124 ng/ml
9) t	O-Xylene	13.929	6981	0.196 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	1877	0.062 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
Data File : FB023821.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2020 22:59
Operator : DD/AJ
Sample : L1852-10
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 10 13:48:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

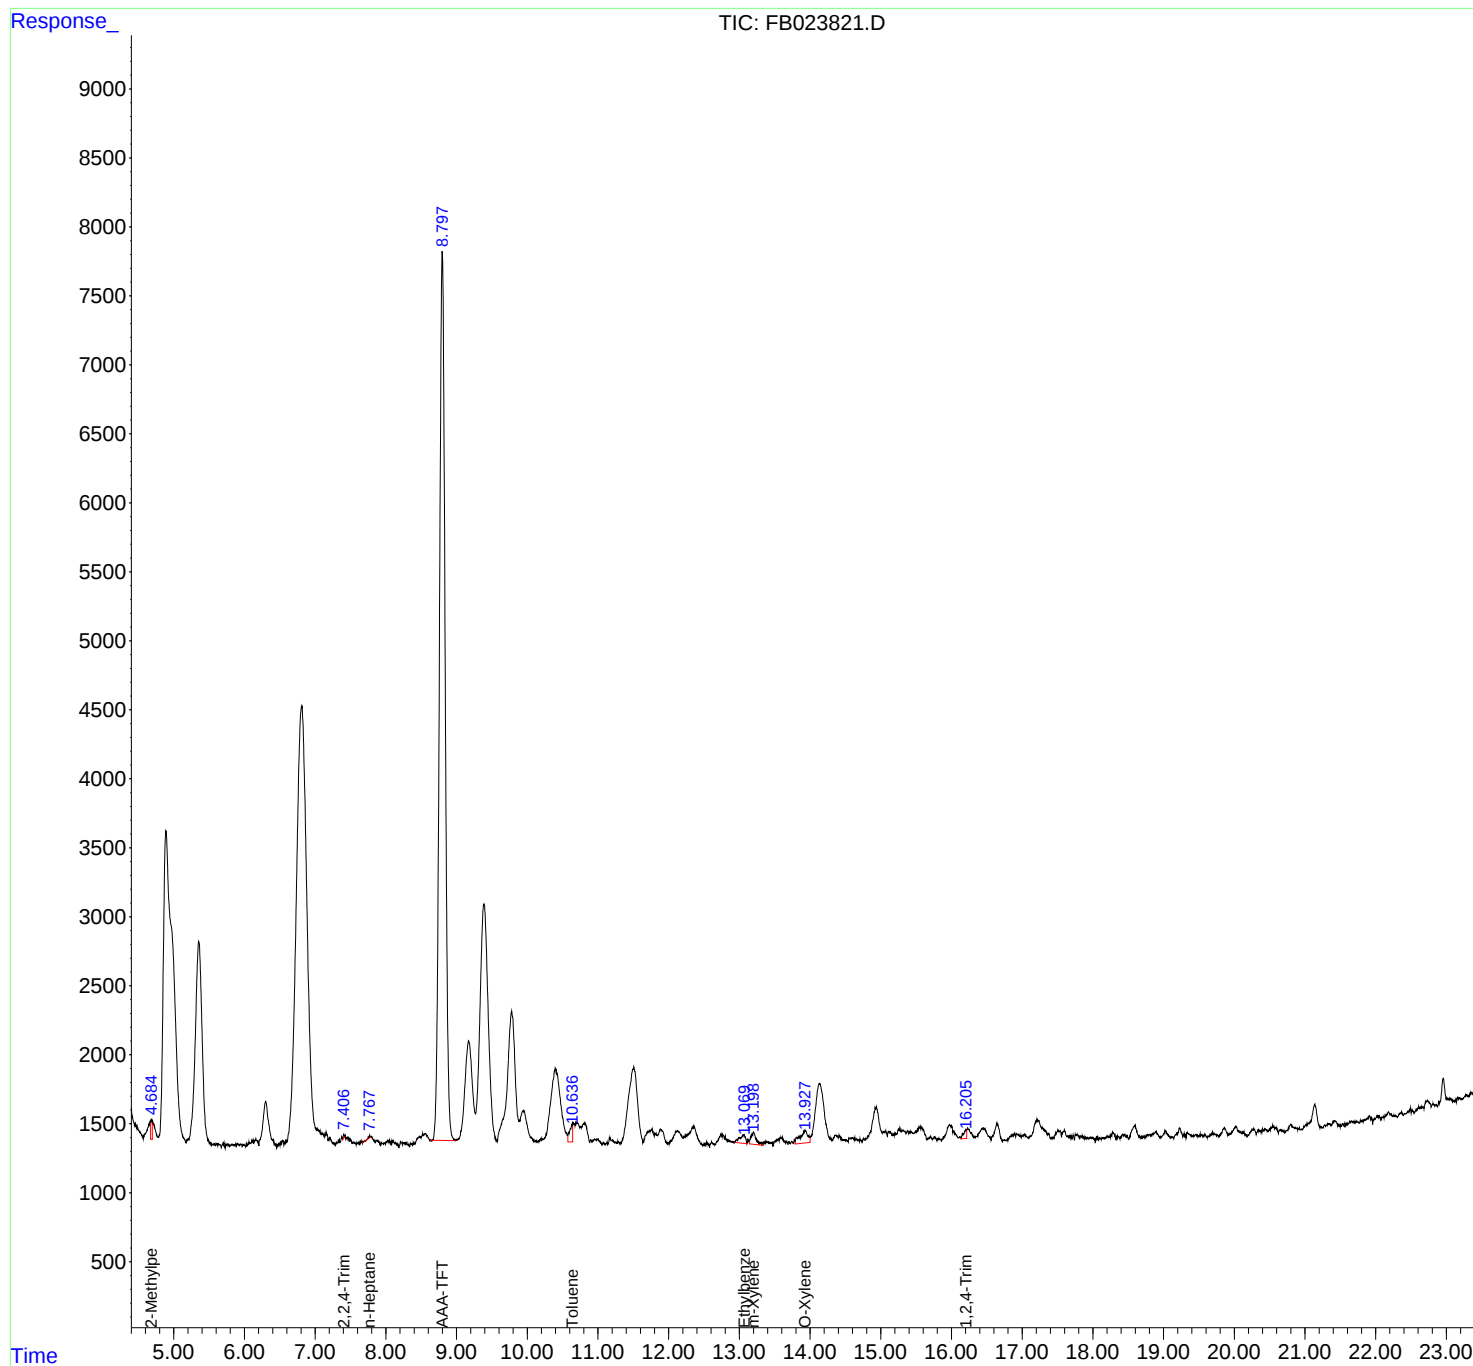


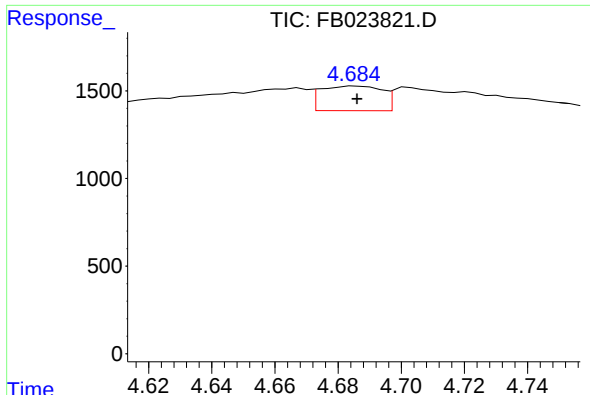

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 1889
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :

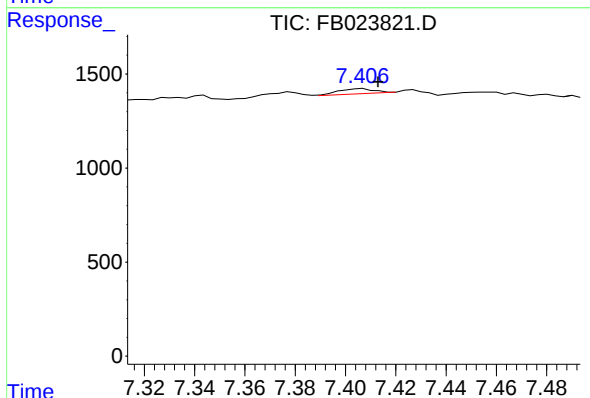


#2 2,2,4-Trimethylpentane

R.T.: 7.407 min
Delta R.T.: -0.006 min
Response: 247
Conc: 0.01 ng/ml

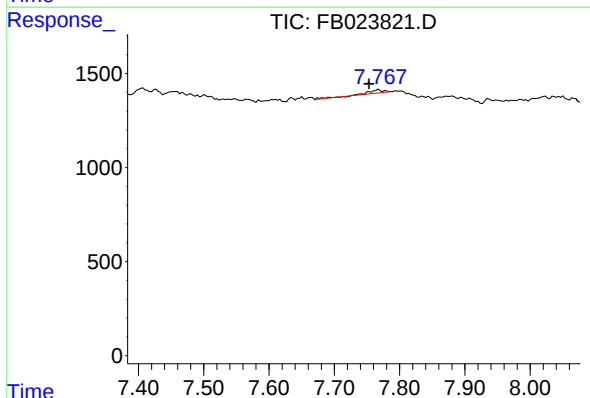


#3 n-Heptane

R.T.: 7.768 min
Delta R.T.: 0.015 min
Response: 238
Conc: 0.01 ng/ml

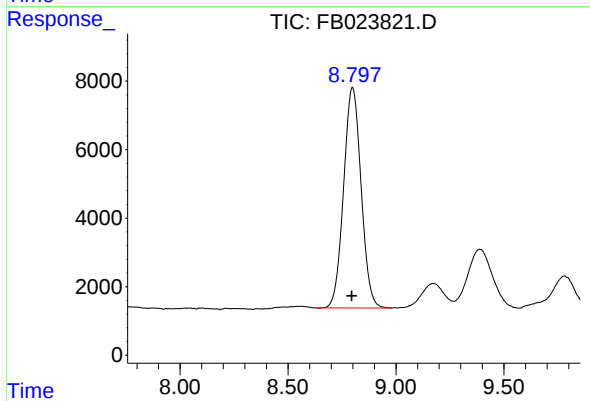

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.004 min
Response: 362623
Conc: 17.23 ng/ml

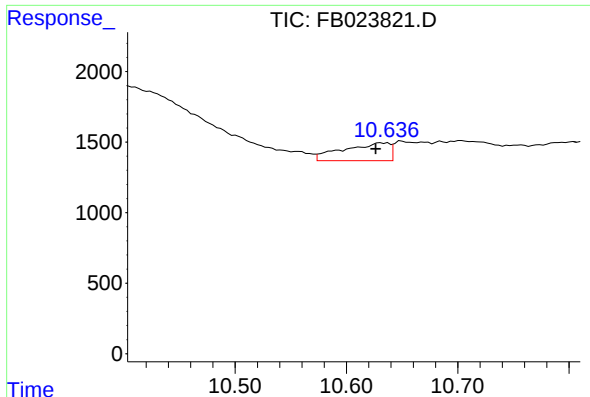

#6 Toluene


R.T.: 10.632 min
Delta R.T.: 0.006 min
Response: 3669
Conc: 0.09 ng/ml

Instrument :
FID_B
ClientSampleId :

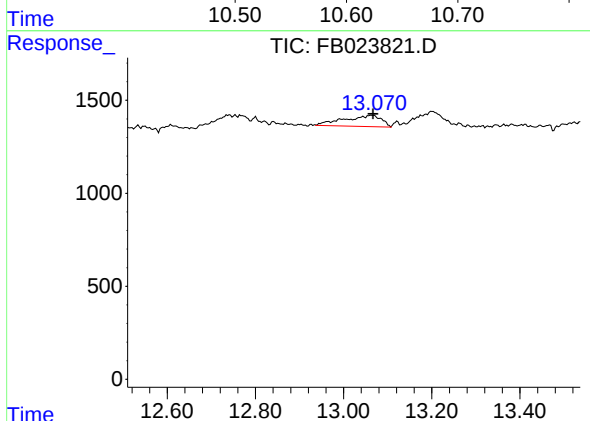


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.002 min
Response: 3523
Conc: 0.09 ng/ml

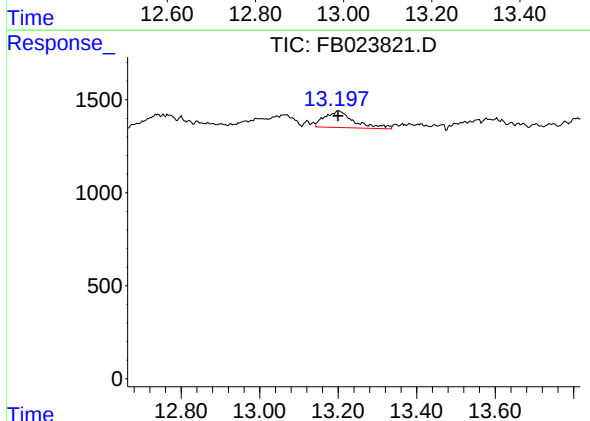


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.002 min
Response: 4575
Conc: 0.12 ng/ml

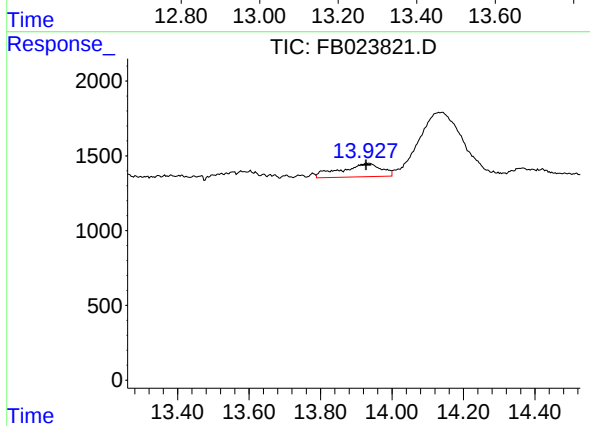

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 6981
Conc: 0.20 ng/ml

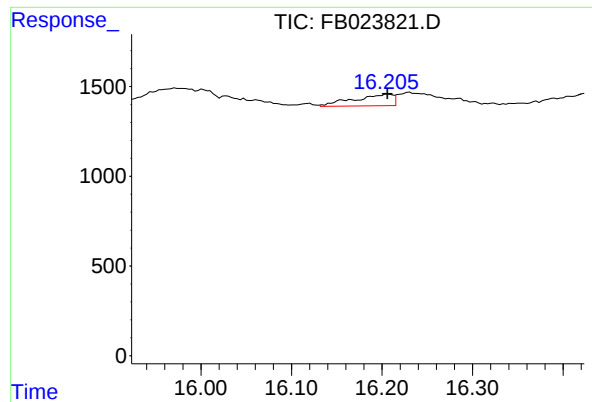

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.001 min
Response: 1877
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :