

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB030920\  
 Data File : FB023825.D  
 Signal(s) : FID2B.CH  
 Acq On : 10 Mar 2020 1:01  
 Operator : DD/AJ  
 Sample : L1852-18  
 Misc : 5.01g/5.00ml DI WATER  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Mar 10 13:48:24 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030520.M  
 Quant Title :  
 QLast Update : Thu Mar 05 11:03:12 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.798  | 306925   | 14.580 ng/ml |
| Target Compounds            |        |          |              |
| 1) t 2-Methylpentane        | 4.672  | 4807     | 0.156 ng/ml  |
| 6) t Toluene                | 10.637 | 750      | 0.018 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB030920\  
Data File : FB023825.D  
Signal(s) : FID2B.CH  
Acq On : 10 Mar 2020 1:01  
Operator : DD/AJ  
Sample : L1852-18  
Misc : 5.01g/5.00ml DI WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Mar 10 13:48:24 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB030520.M  
Quant Title :  
QLast Update : Thu Mar 05 11:03:12 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

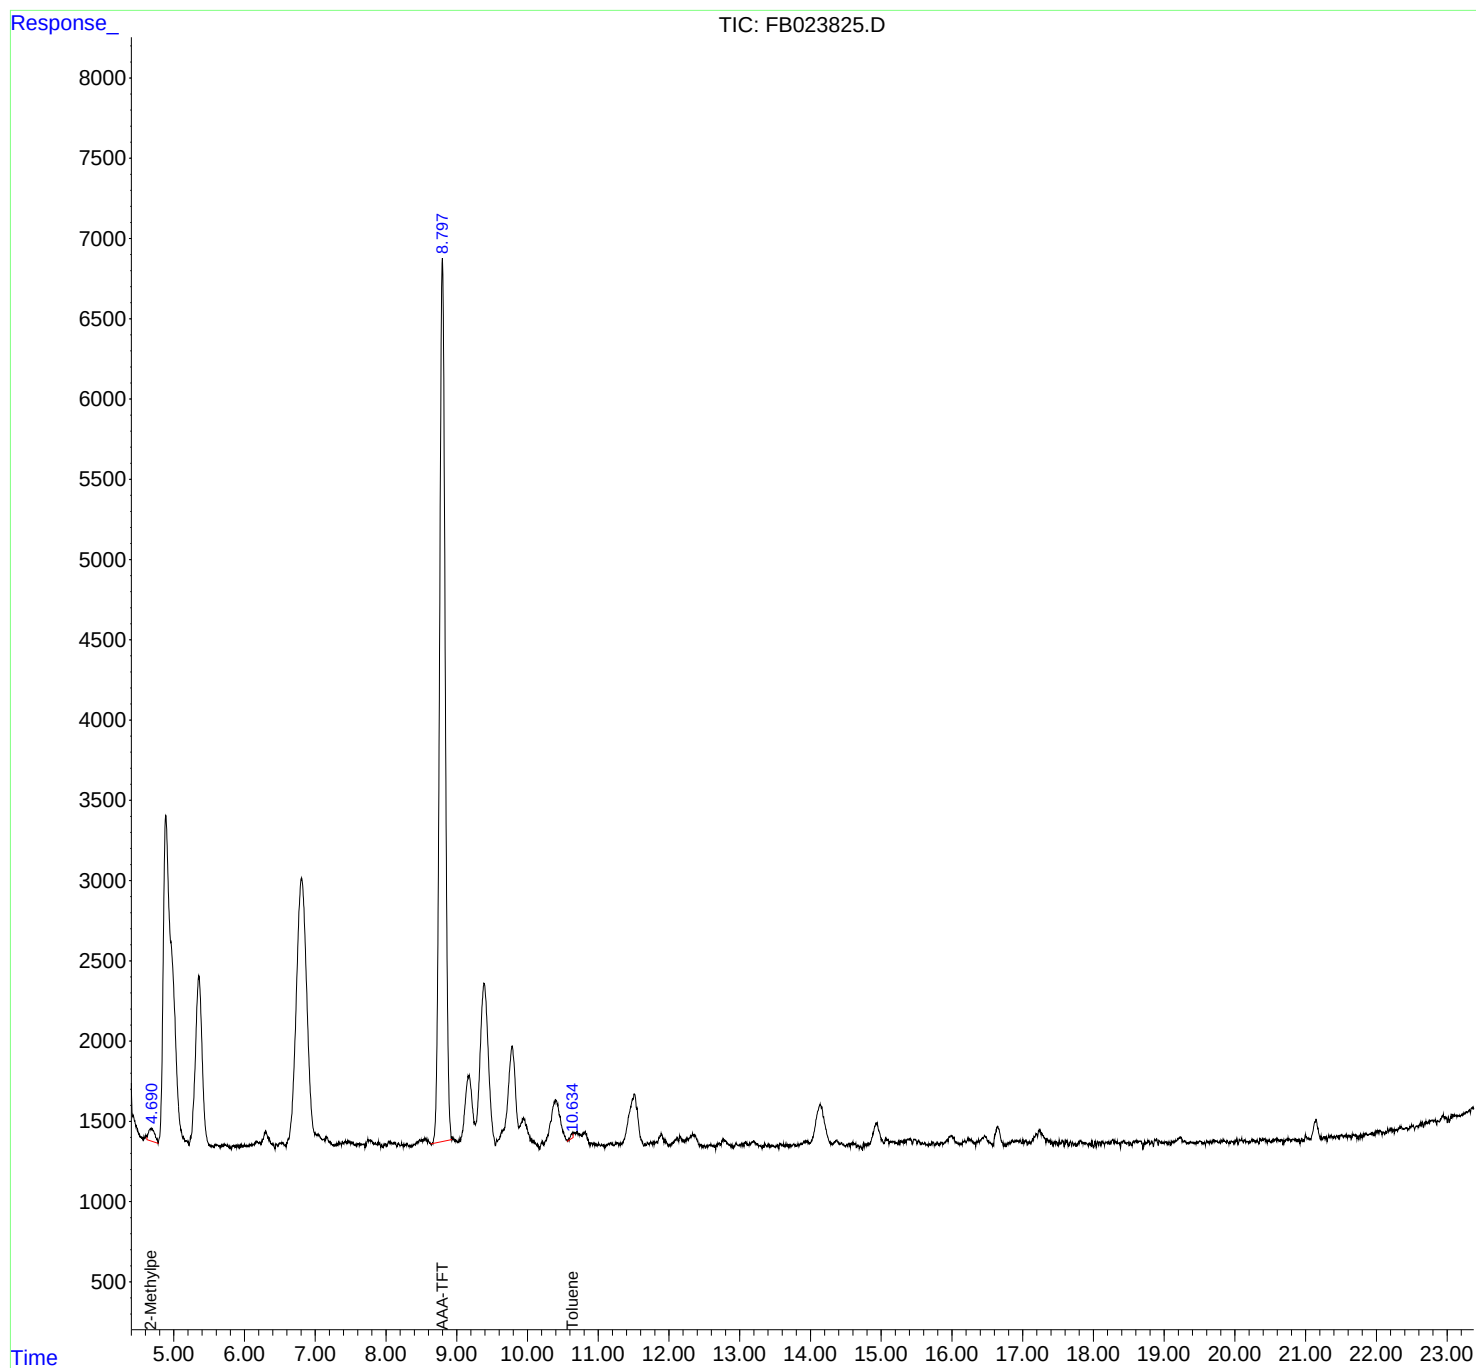


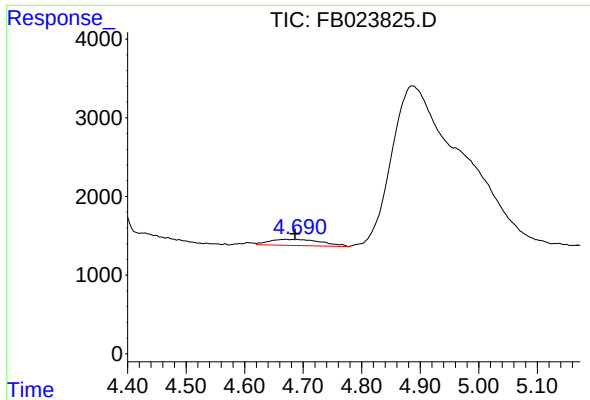

#1 2-Methylpentane


R.T.: 4.672 min  
Delta R.T.: -0.014 min  
Response: 4807  
Conc: 0.16 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

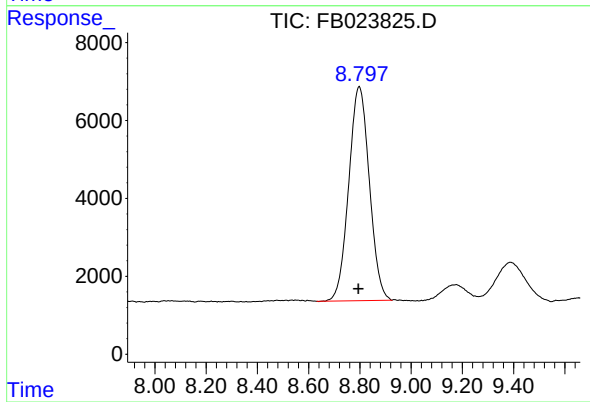

#5 AAA-TFT

R.T.: 8.798 min  
Delta R.T.: 0.003 min  
Response: 306925  
Conc: 14.58 ng/ml

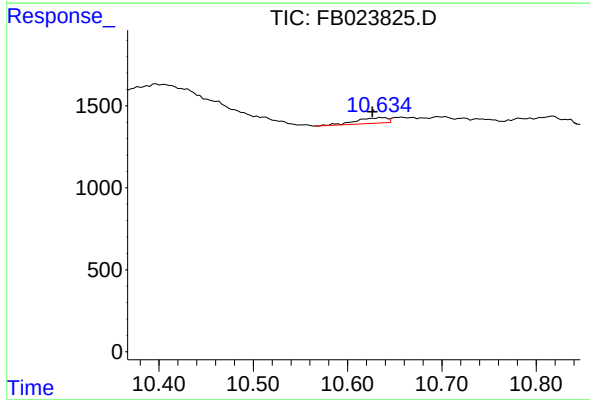

#6 Toluene

R.T.: 10.637 min  
Delta R.T.: 0.011 min  
Response: 750  
Conc: 0.02 ng/ml