

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
 Data File : FB023826.D
 Signal(s) : FID2B.CH
 Acq On : 10 Mar 2020 8:32
 Operator : DD/AJ
 Sample : L1852-21
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 10 13:48:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.791	342652	16.277 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	279	0.009 ng/ml
2) t	2,2,4-Trimethylpentane	7.379	1666	0.049 ng/ml
3) t	n-Heptane	7.767	1944	0.059 ng/ml
6) t	Toluene	10.625	21866	0.536 ng/ml
7) t	Ethylbenzene	13.055	23576	0.617 ng/ml
8) t	m-Xylene	13.194	37072	1.007 ng/ml
9) t	O-Xylene	13.925	26424	0.743 ng/ml
10) t	1,2,4-Trimethylbenzene	16.205	51840	1.711 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030920\
Data File : FB023826.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2020 8:32
Operator : DD/AJ
Sample : L1852-21
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 10 13:48:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

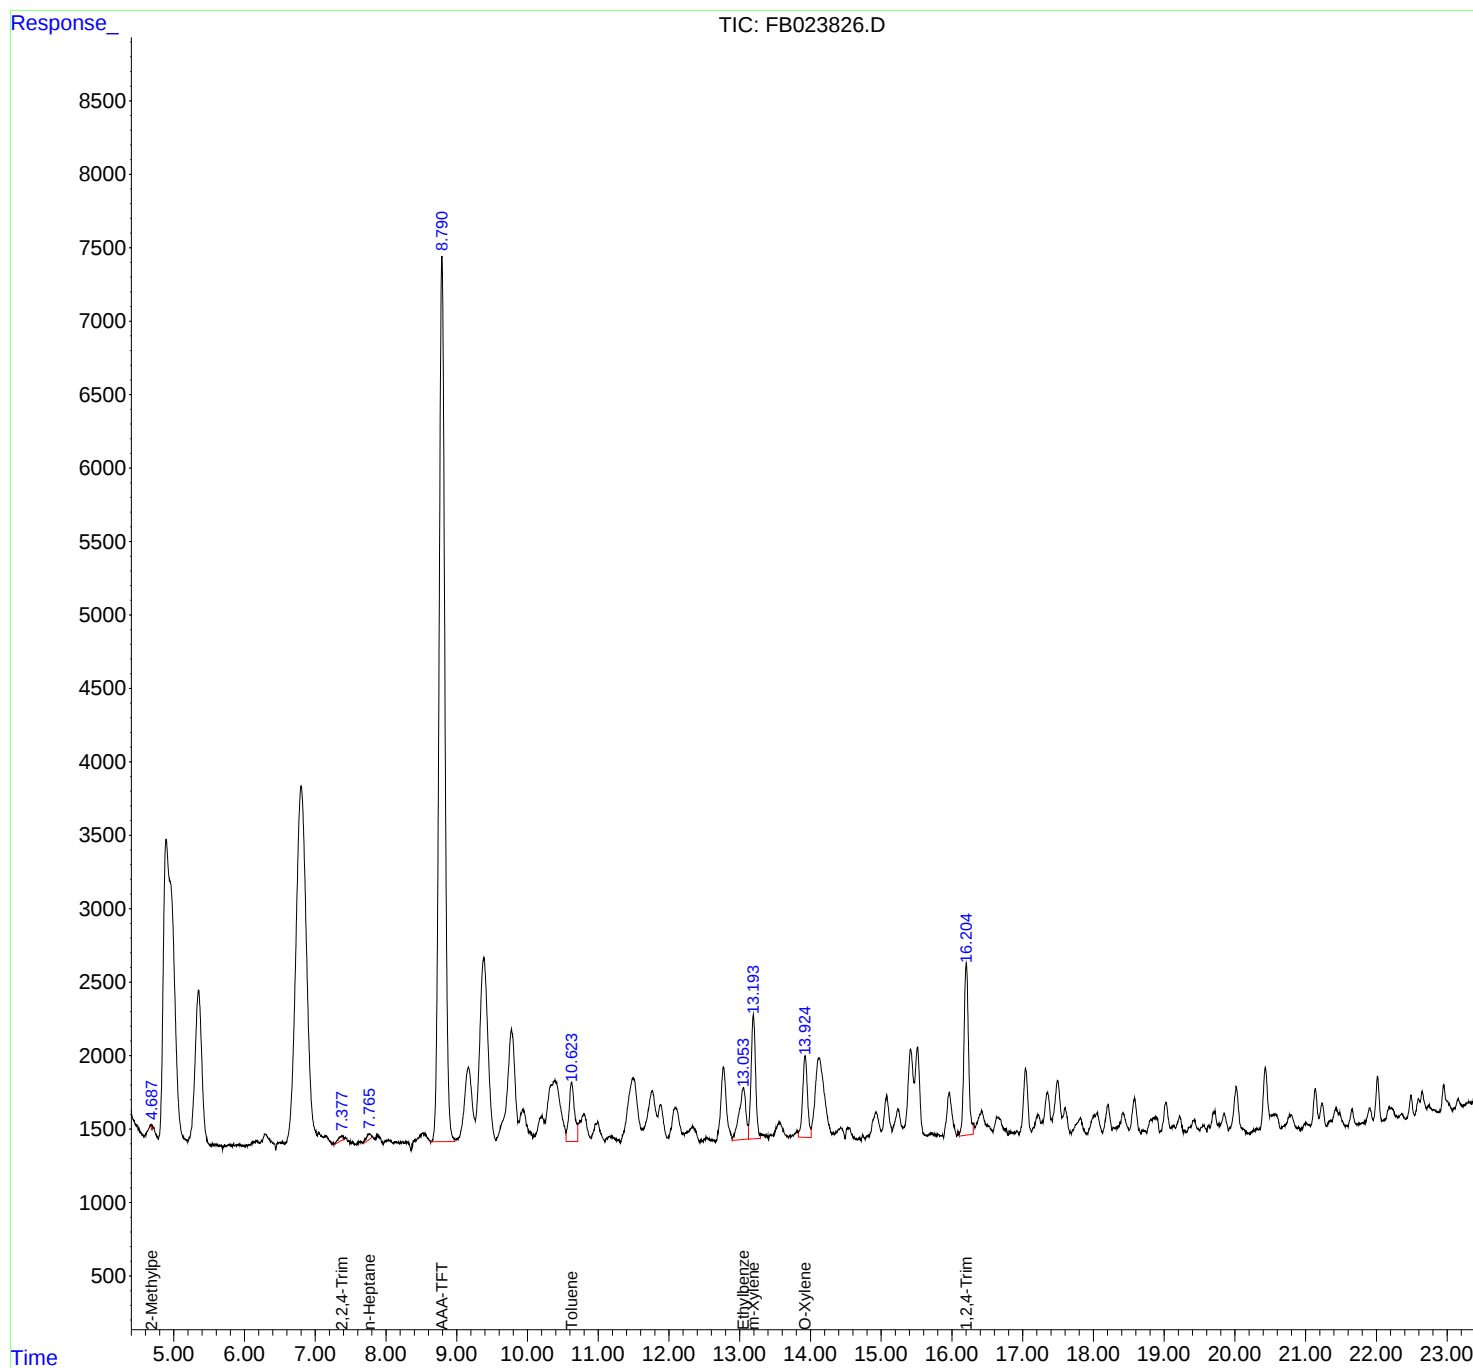


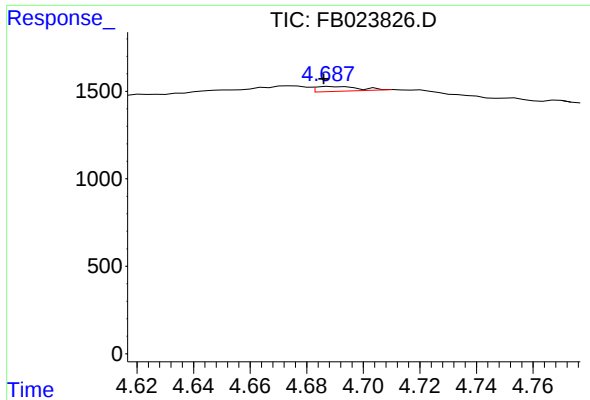

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.003 min
Response: 279
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :

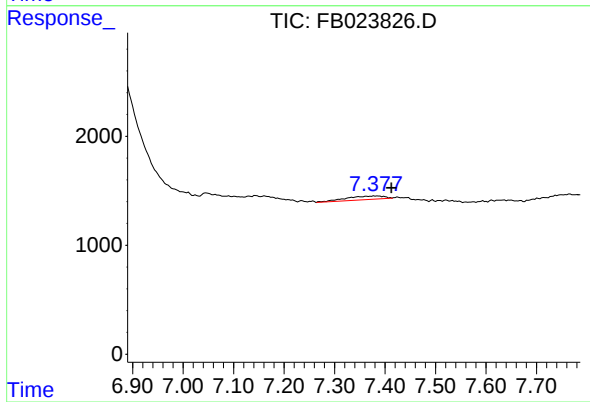


#2 2,2,4-Trimethylpentane

R.T.: 7.379 min
Delta R.T.: -0.034 min
Response: 1666
Conc: 0.05 ng/ml

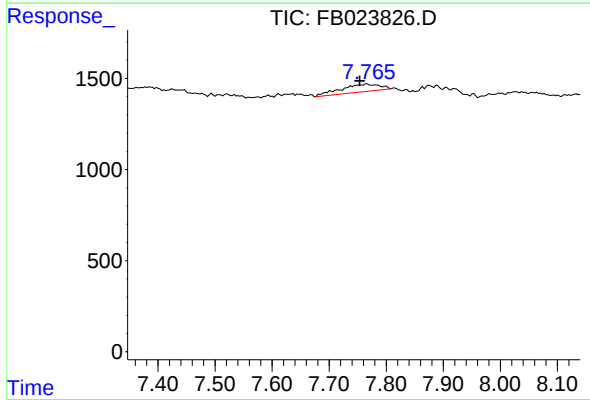


#3 n-Heptane

R.T.: 7.767 min
Delta R.T.: 0.013 min
Response: 1944
Conc: 0.06 ng/ml

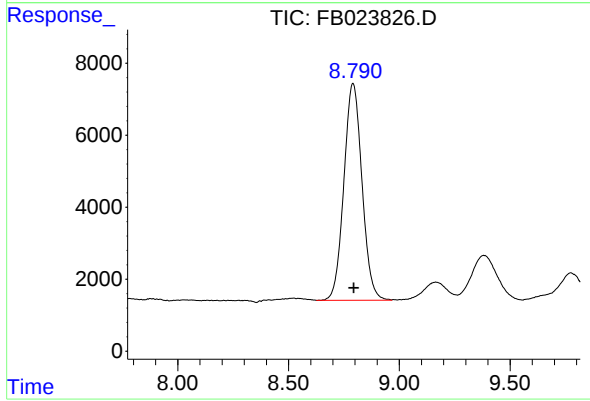

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.003 min
Response: 342652
Conc: 16.28 ng/ml

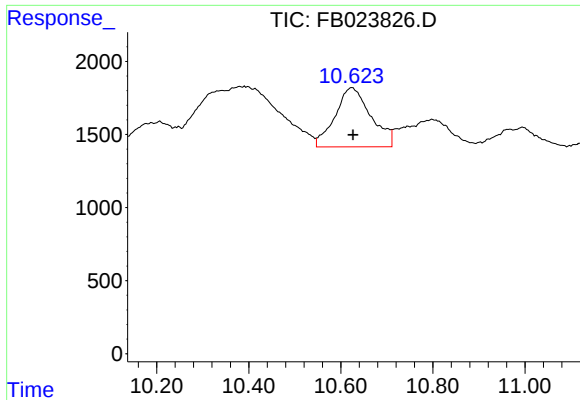

#6 Toluene


R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 21866
Conc: 0.54 ng/ml

Instrument :
FID_B
ClientSampleId :

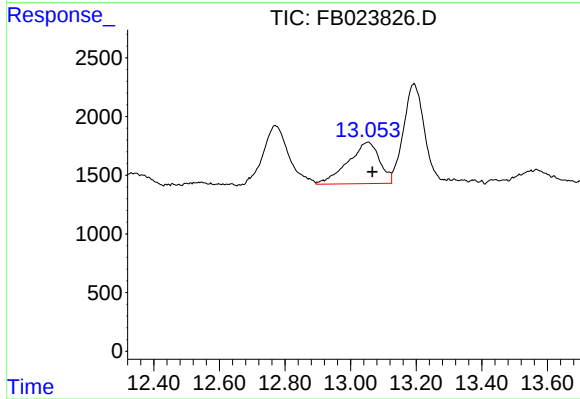


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.012 min
Response: 23576
Conc: 0.62 ng/ml

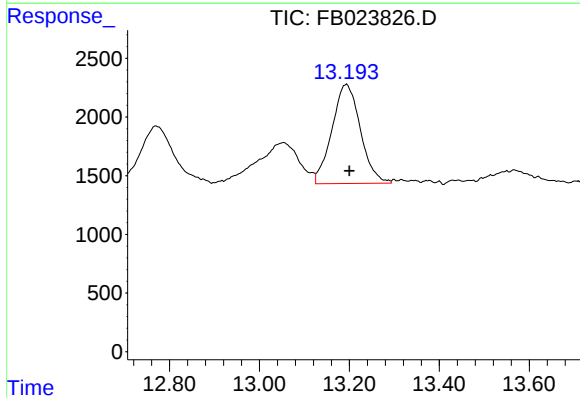


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: -0.006 min
Response: 37072
Conc: 1.01 ng/ml

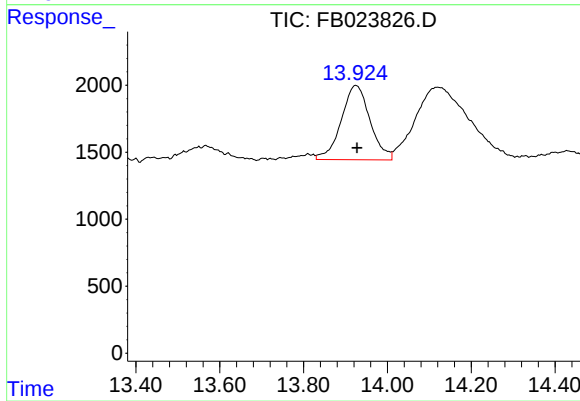

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.002 min
Response: 26424
Conc: 0.74 ng/ml

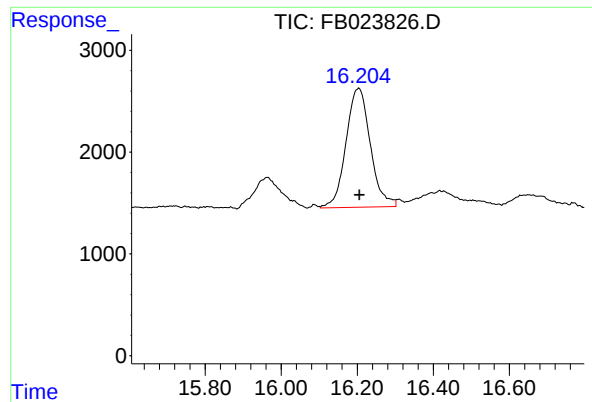

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.001 min
Response: 51840
Conc: 1.71 ng/ml

Instrument :
FID_B
ClientSampleId :