

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030921\
 Data File : FB025514.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2021 9:40
 Operator : DD/AJ
 Sample : BSF0309S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0309S1

Integration File: Calibration.e
 Quant Time: Mar 10 00:09:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	504236	19.879 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	953450	27.052 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1068943	28.788 ng/ml
3) t n-Heptane	7.758	343694	9.494 ng/ml
4) t Benzene	7.892	432672	9.366 ng/ml
6) t Toluene	10.630	1252967	28.025 ng/ml
7) t Ethylbenzene	13.070	389932	9.661 ng/ml
8) t m-Xylene	13.203	779209	19.370 ng/ml
9) t O-Xylene	13.931	749328	19.358 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	664862	19.806 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030921\
Data File : FB025514.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2021 9:40
Operator : DD/AJ
Sample : BSF0309S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0309S1

Integration File: Calibration.e
Quant Time: Mar 10 00:09:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

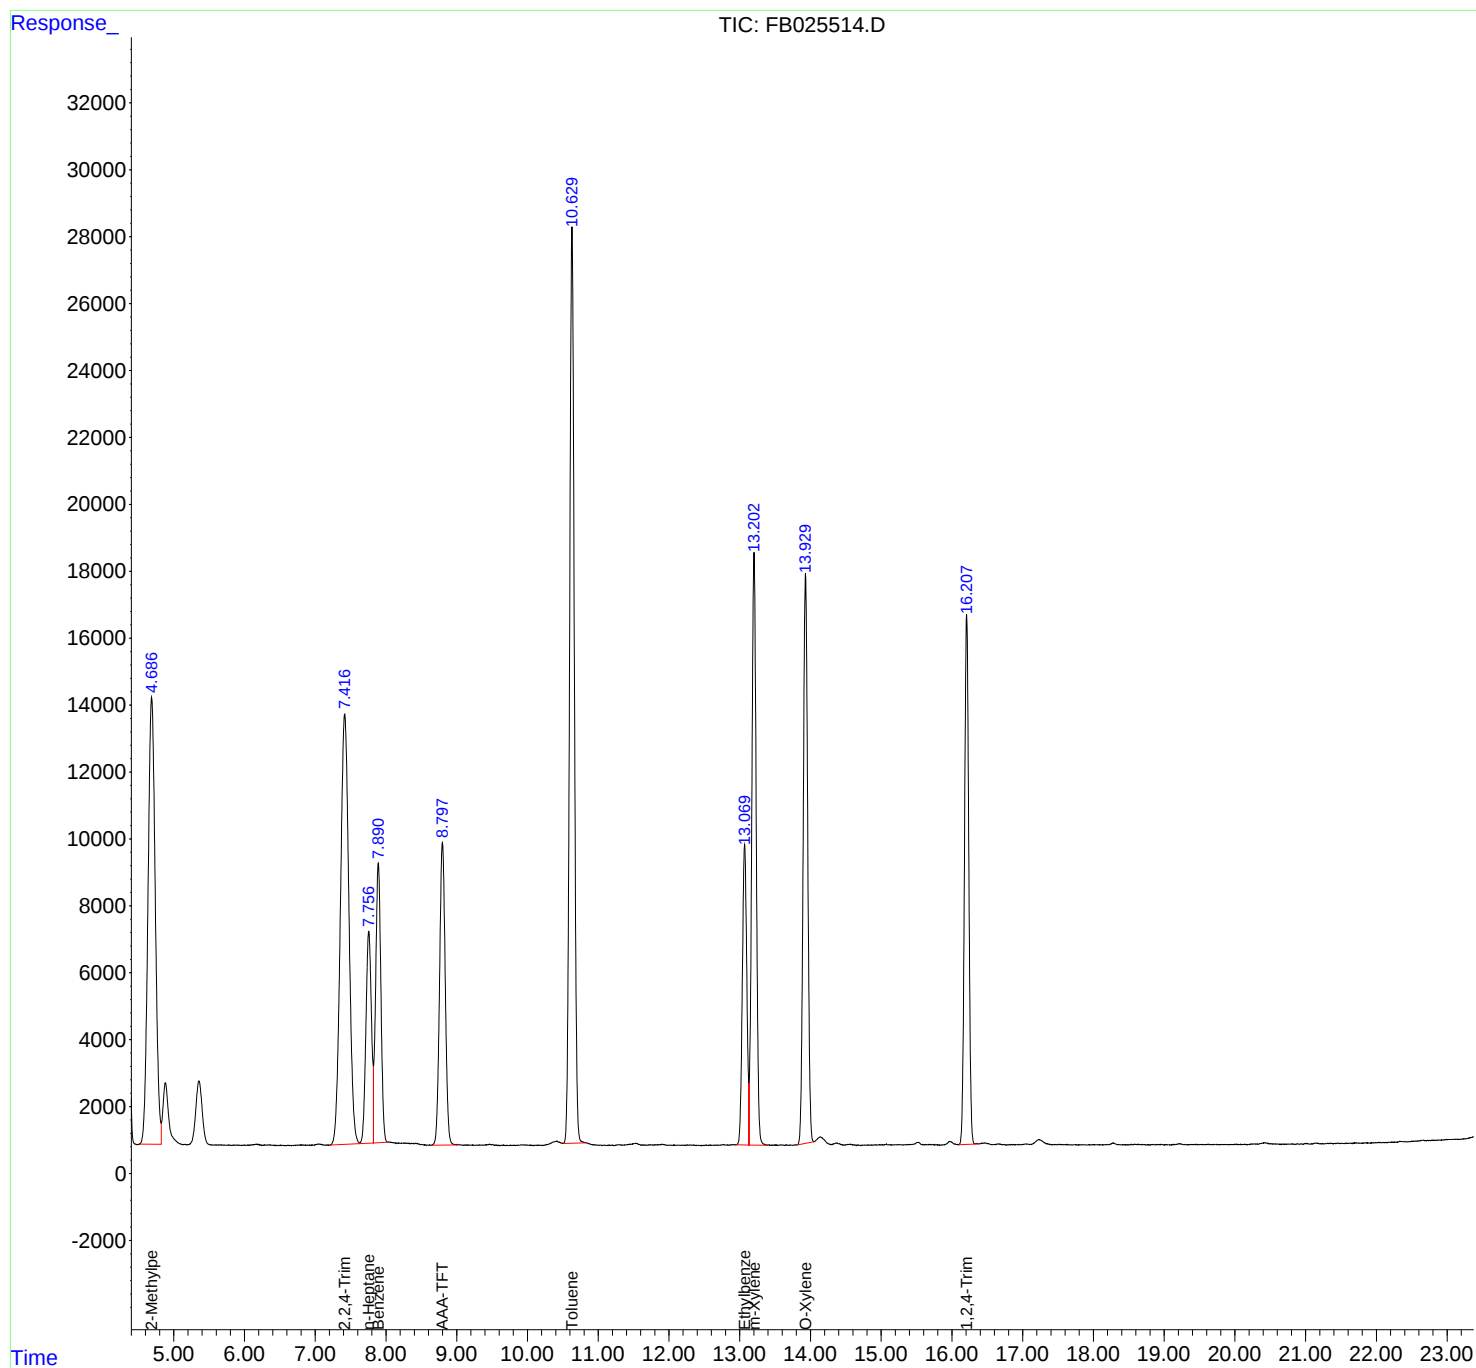


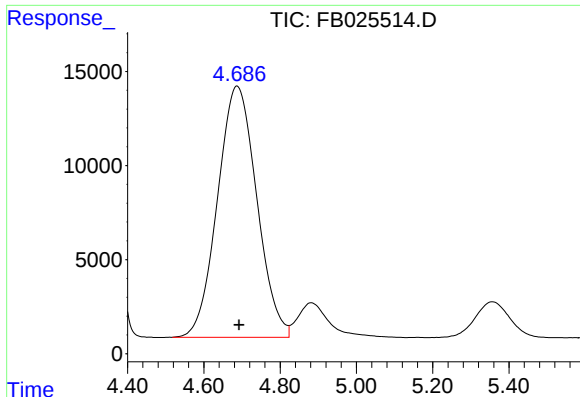

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.005 min
Response: 953450
Conc: 27.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0309S1

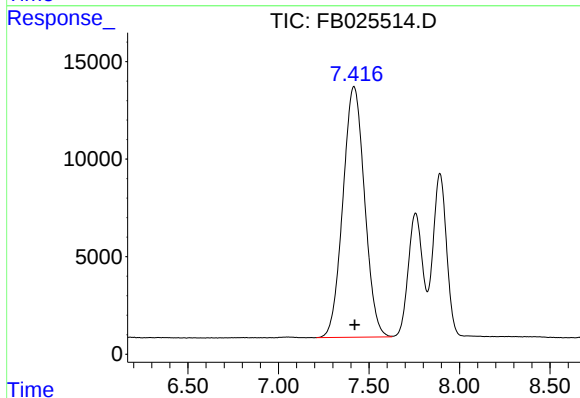


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.005 min
Response: 1068943
Conc: 28.79 ng/ml

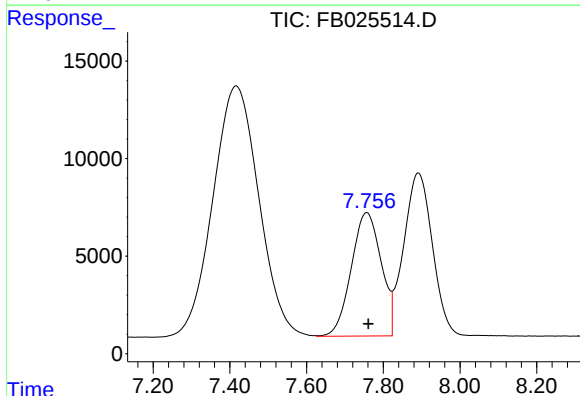


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.004 min
Response: 343694
Conc: 9.49 ng/ml

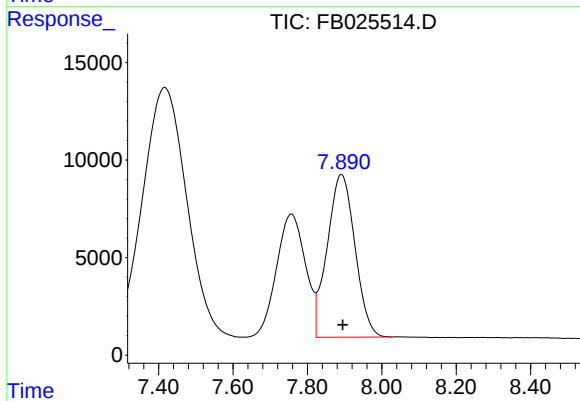

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.004 min
Response: 432672
Conc: 9.37 ng/ml

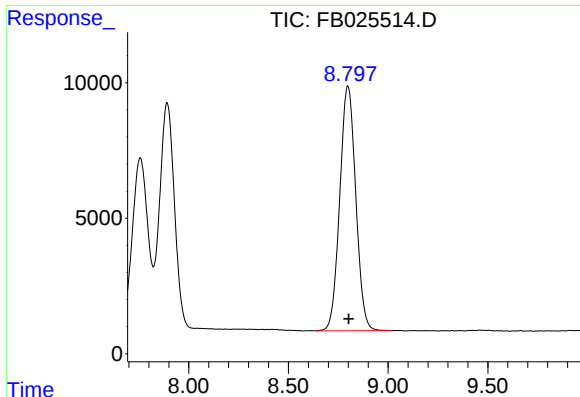

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.004 min
Response: 504236
Conc: 19.88 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0309S1

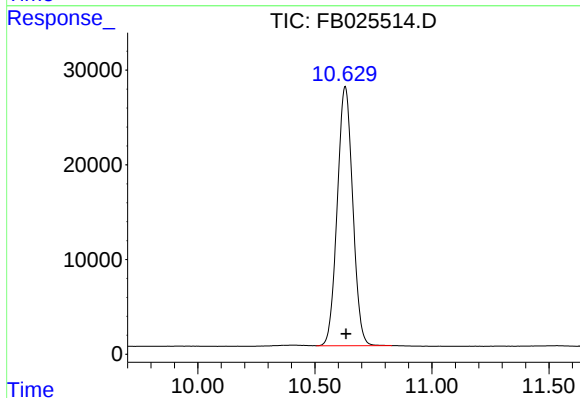


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.004 min
Response: 1252967
Conc: 28.02 ng/ml

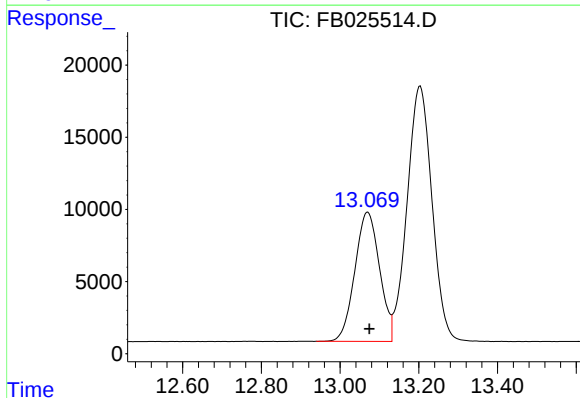


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.004 min
Response: 389932
Conc: 9.66 ng/ml

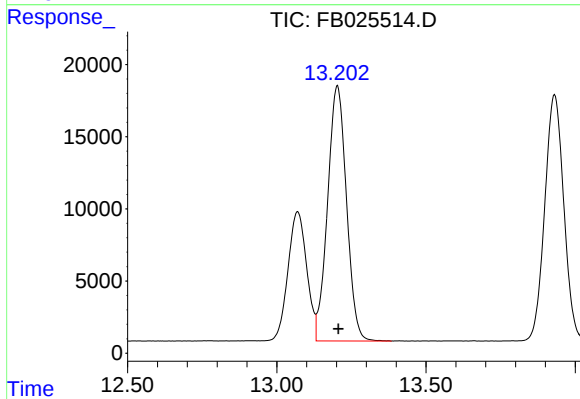

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.003 min
Response: 779209
Conc: 19.37 ng/ml

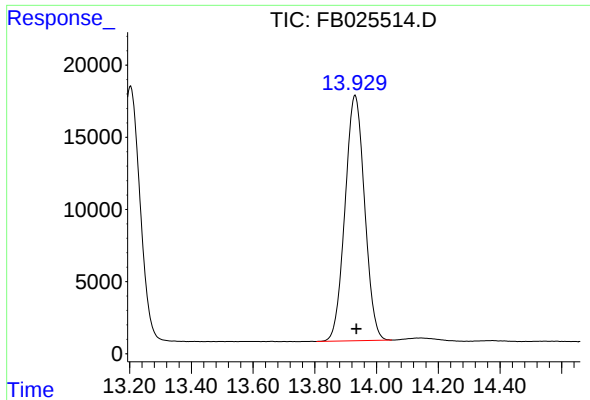

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.003 min
Response: 749328
Conc: 19.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0309S1

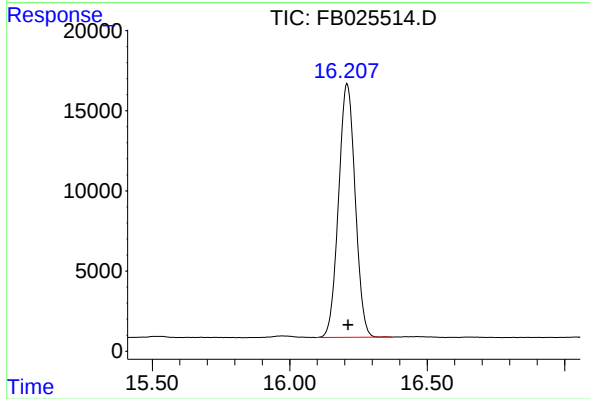

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.003 min
Response: 664862
Conc: 19.81 ng/ml