

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030921\
 Data File : FB025519.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2021 12:11
 Operator : DD/AJ
 Sample : M1603-01MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 31-NORTHMS

Integration File: Calibration.e
 Quant Time: Mar 10 00:10:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	558683	22.026 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	997983	28.316 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1089205	29.333 ng/ml
3) t n-Heptane	7.760	332053	9.172 ng/ml
4) t Benzene	7.895	448644	9.712 ng/ml
6) t Toluene	10.633	1304523	29.178 ng/ml
7) t Ethylbenzene	13.073	407930	10.107 ng/ml
8) t m-Xylene	13.206	800269	19.893 ng/ml
9) t O-Xylene	13.934	778352	20.108 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	656380	19.554 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030921\
Data File : FB025519.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2021 12:11
Operator : DD/AJ
Sample : M1603-01MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
31-NORTHMS

Integration File: Calibration.e
Quant Time: Mar 10 00:10:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

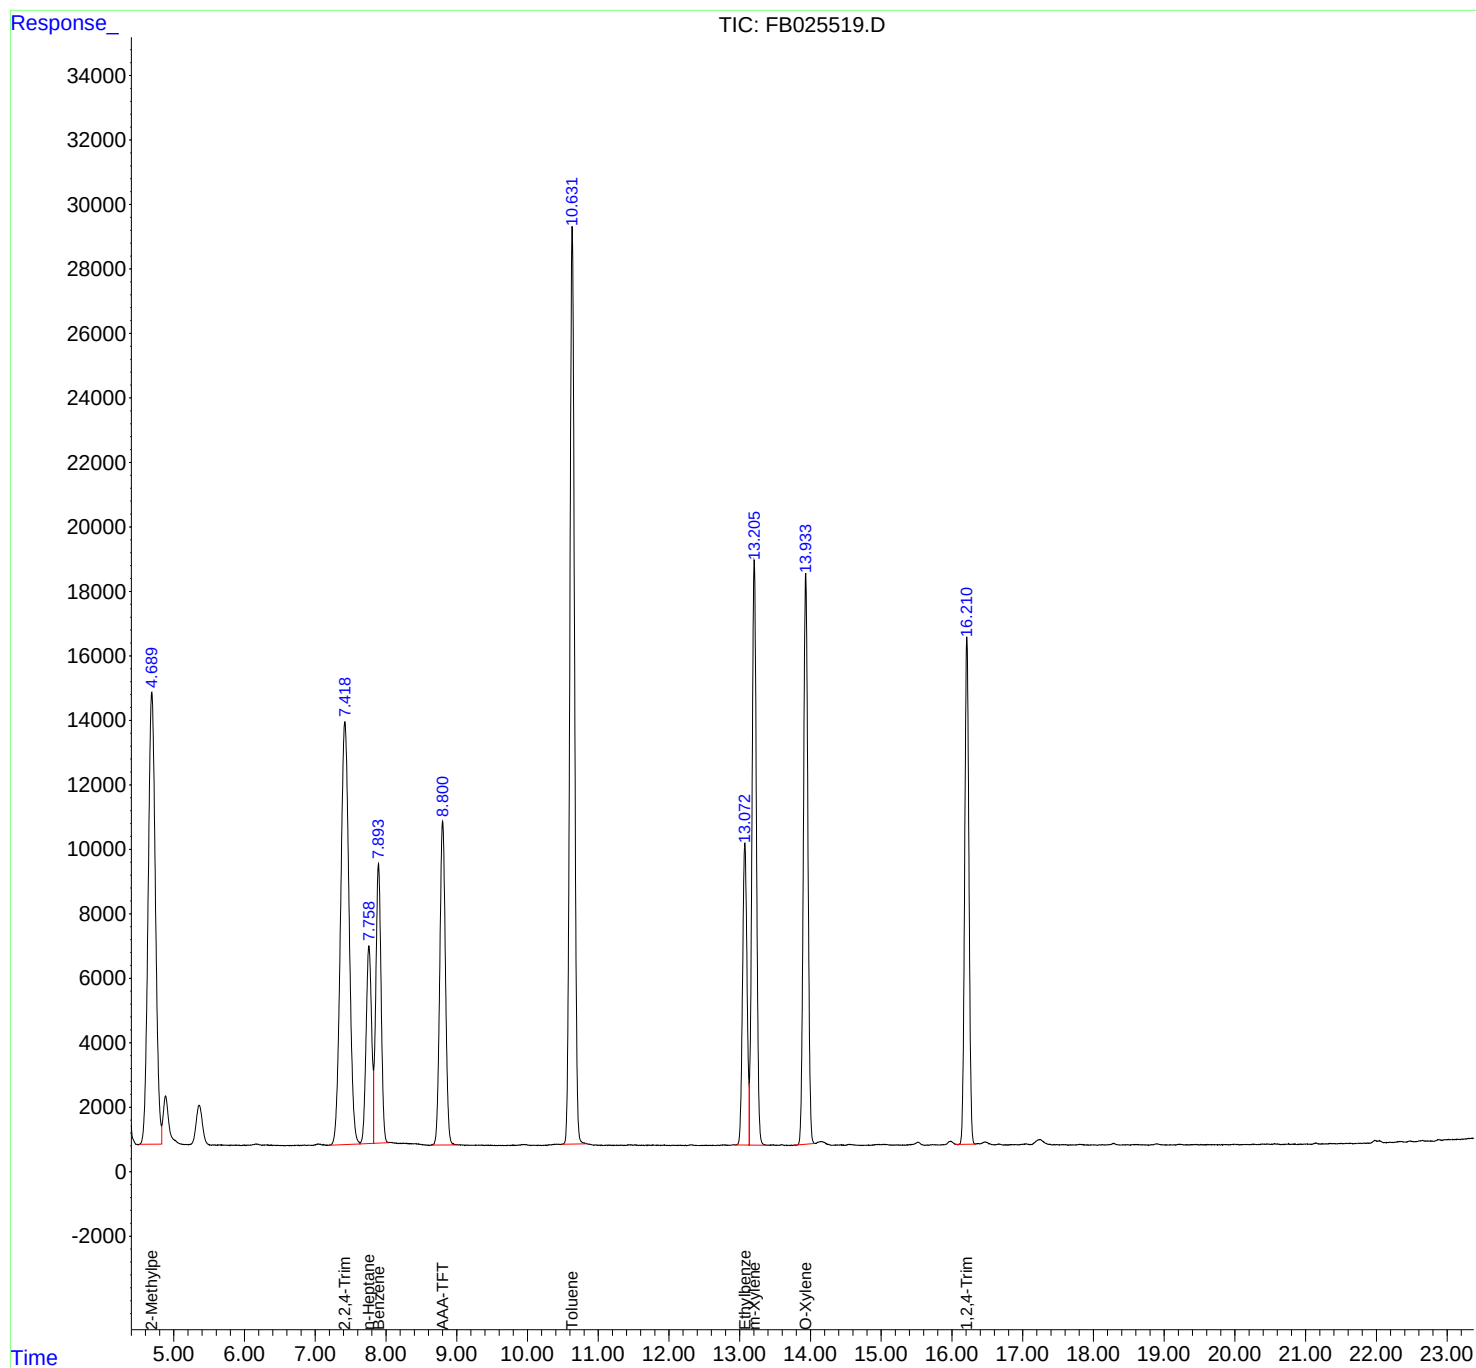


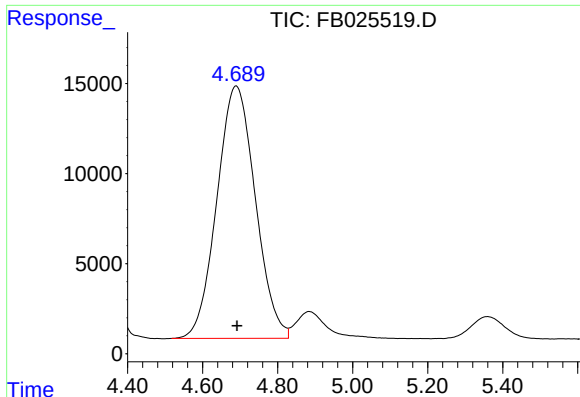

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: -0.002 min
Response: 997983
Conc: 28.32 ng/ml

Instrument :
FID_B
ClientSampleId :
31-NORTHMS

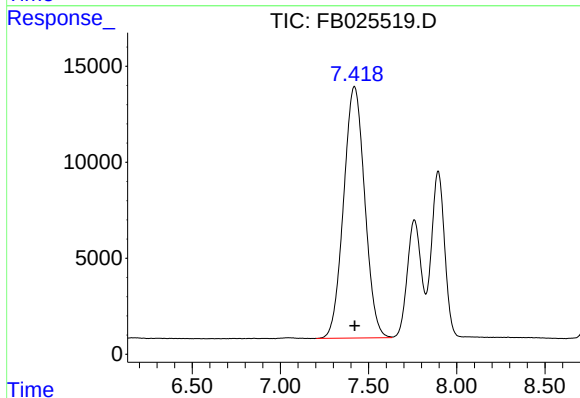


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.002 min
Response: 1089205
Conc: 29.33 ng/ml

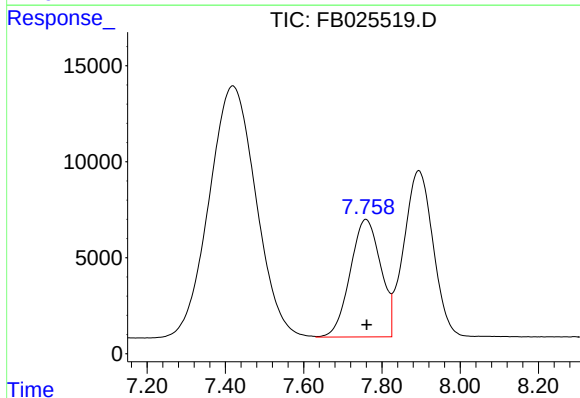


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: -0.002 min
Response: 332053
Conc: 9.17 ng/ml

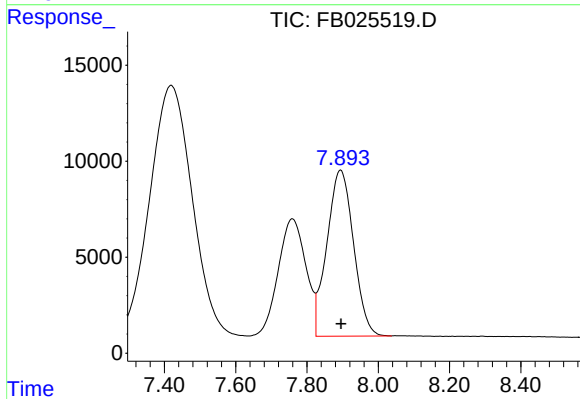

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 448644
Conc: 9.71 ng/ml

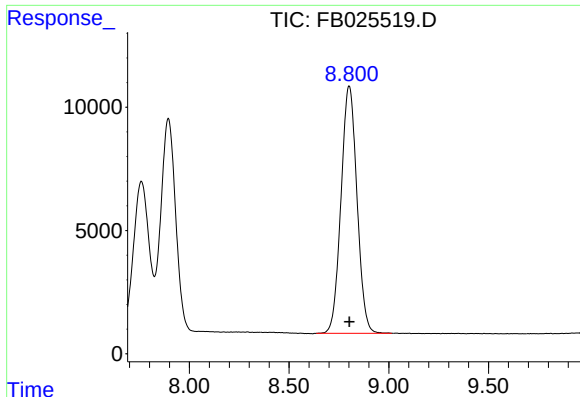

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 558683
Conc: 22.03 ng/ml

Instrument :
FID_B
ClientSampleId :
31-NORTHMS

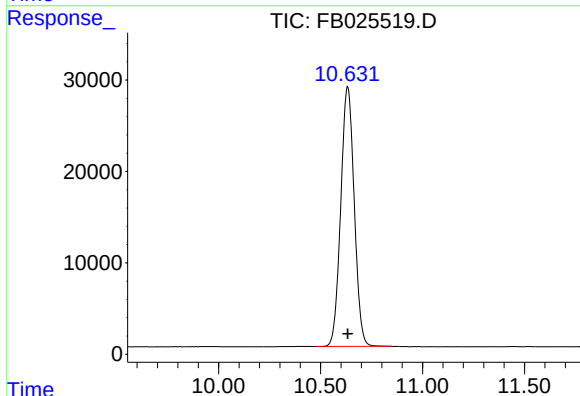


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.000 min
Response: 1304523
Conc: 29.18 ng/ml

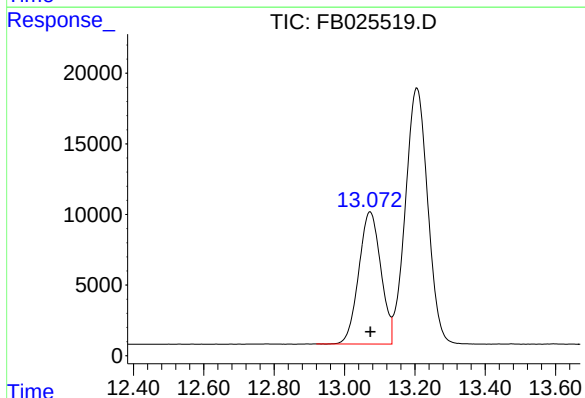


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.000 min
Response: 407930
Conc: 10.11 ng/ml

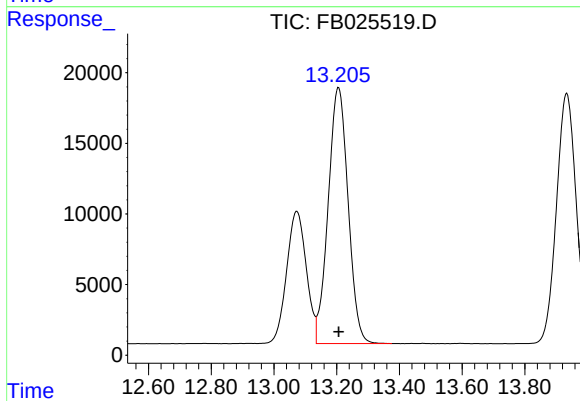

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 800269
Conc: 19.89 ng/ml

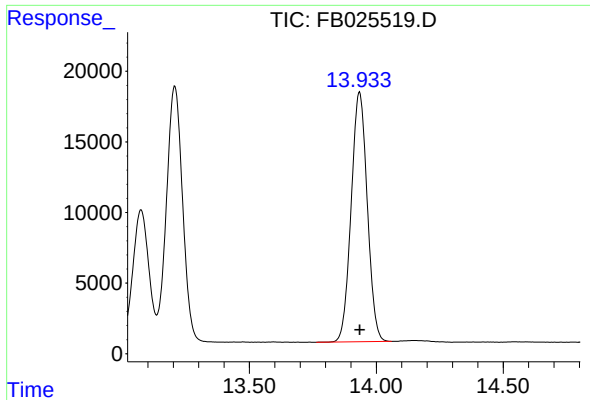

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 778352
Conc: 20.11 ng/ml

Instrument :
FID_B
ClientSampleId :
31-NORTHMS

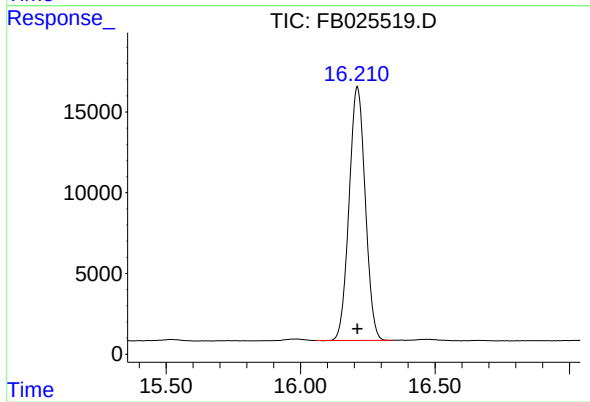

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.000 min
Response: 656380
Conc: 19.55 ng/ml