

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026656.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 12:51
 Operator : AJ/MA
 Sample : N1645-01
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:00:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	188914	18.003 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	15220	0.804 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	30145	1.454 ng/ml
3) t n-Heptane	7.740	9867	0.499 ng/ml
4) t Benzene	7.881	6037	0.262 ng/ml
6) t Toluene	10.619	33955	1.551 ng/ml
7) t Ethylbenzene	13.053	11731	0.584 ng/ml
8) t m-Xylene	13.194	22266	1.105 ng/ml
9) t O-Xylene	13.916	21136	1.059 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	22592	1.134 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026656.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 12:51
Operator : AJ/MA
Sample : N1645-01
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:00:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

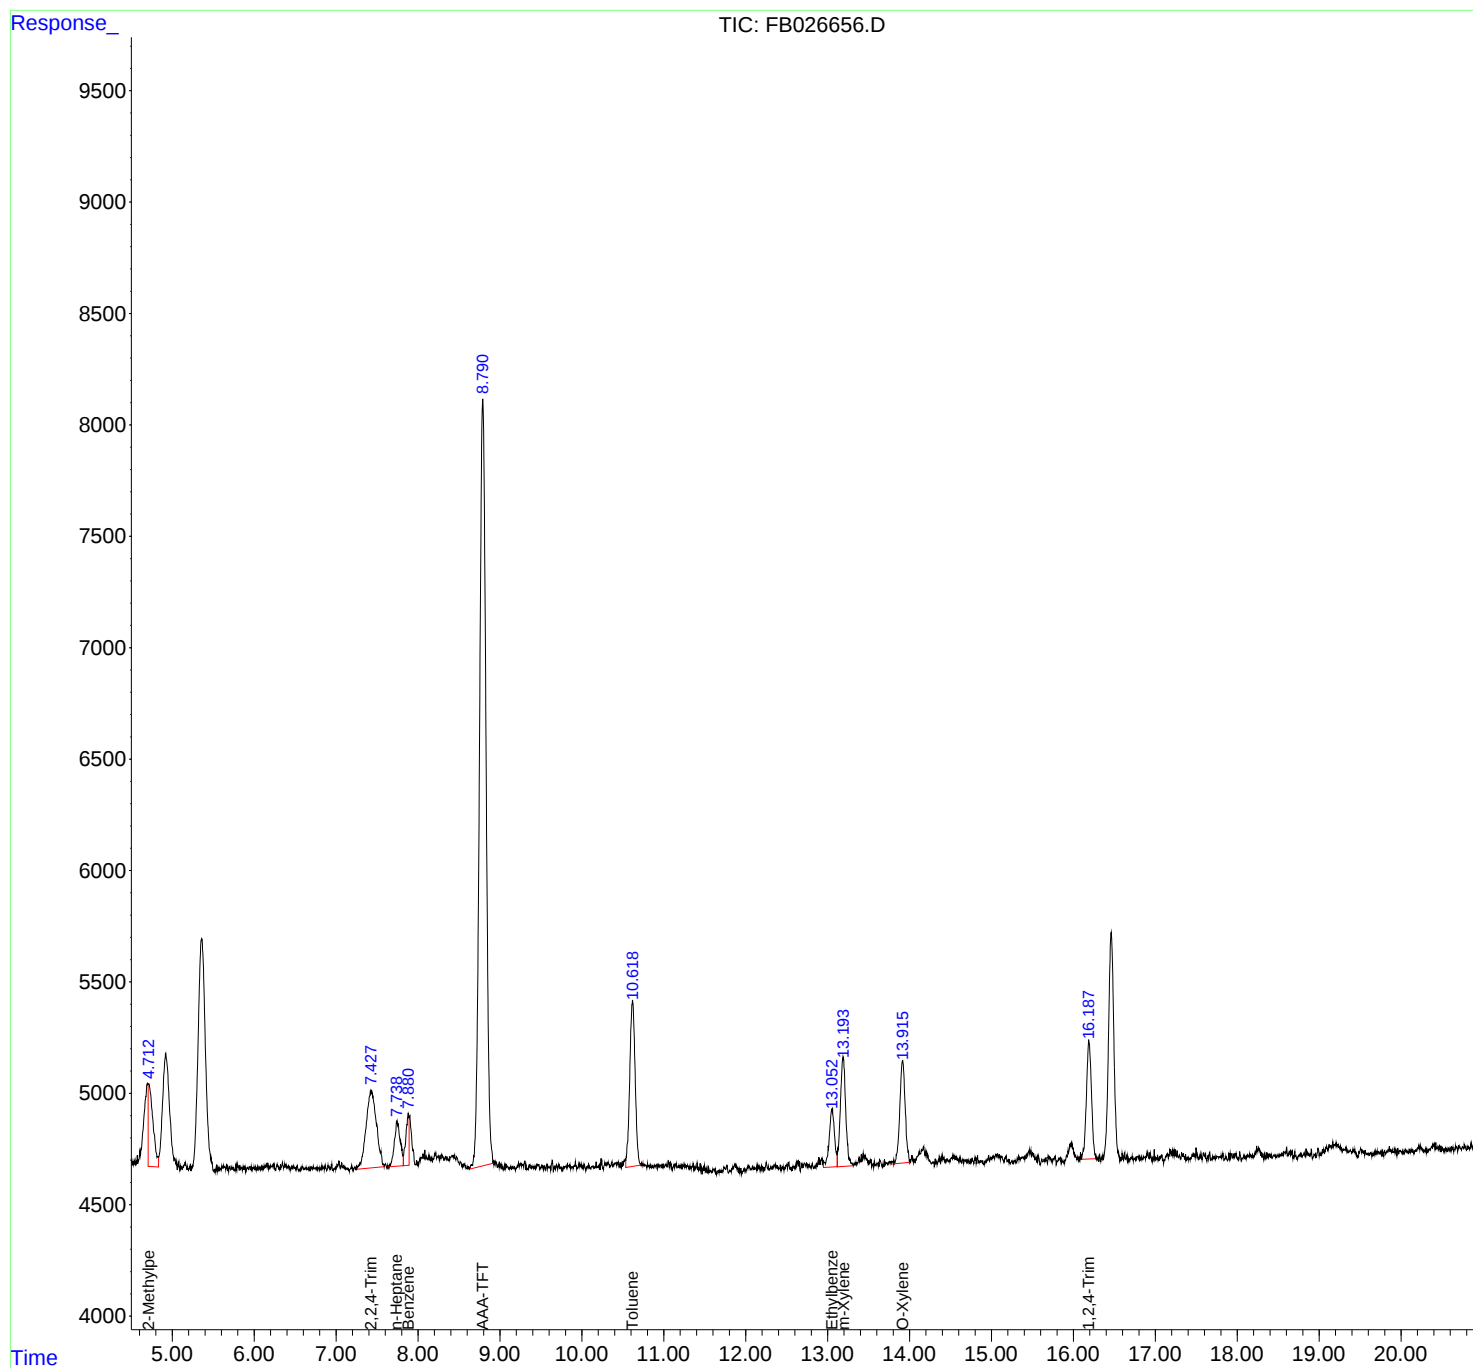

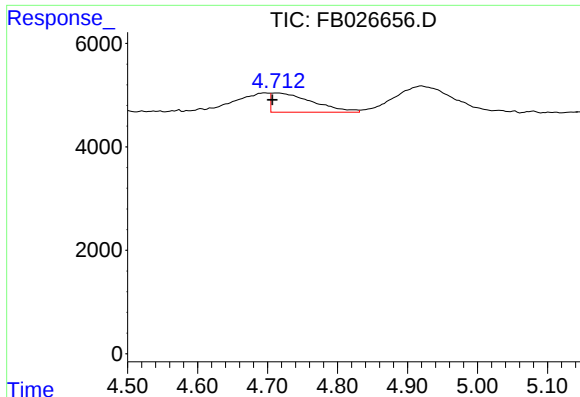


#1 2-Methylpentane

R.T.: 4.714 min
Delta R.T.: 0.007 min
Response: 15220
Conc: 0.80 ng/ml

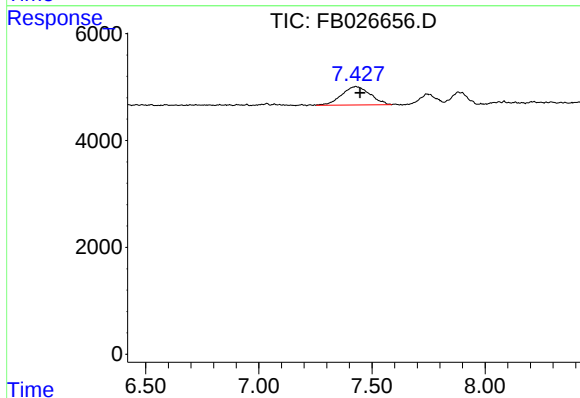


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.018 min
Response: 30145
Conc: 1.45 ng/ml

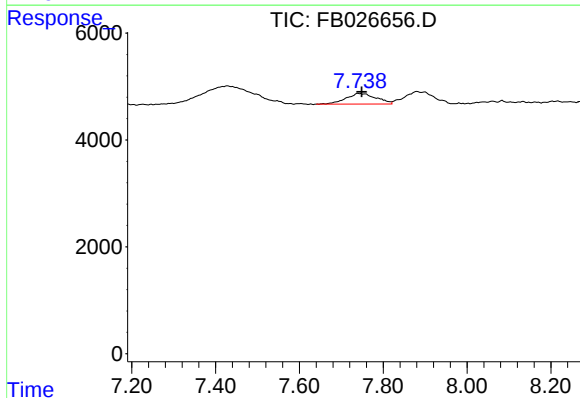


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.009 min
Response: 9867
Conc: 0.50 ng/ml

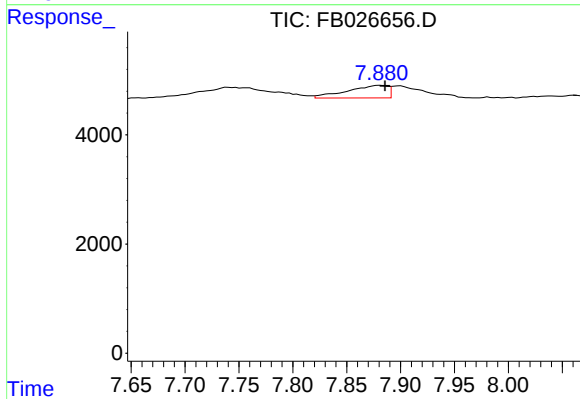


#4 Benzene

R.T.: 7.881 min
Delta R.T.: -0.005 min
Response: 6037
Conc: 0.26 ng/ml

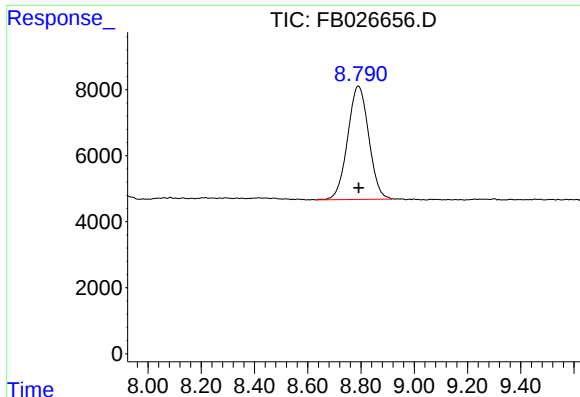


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 188914
Conc: 18.00 ng/ml

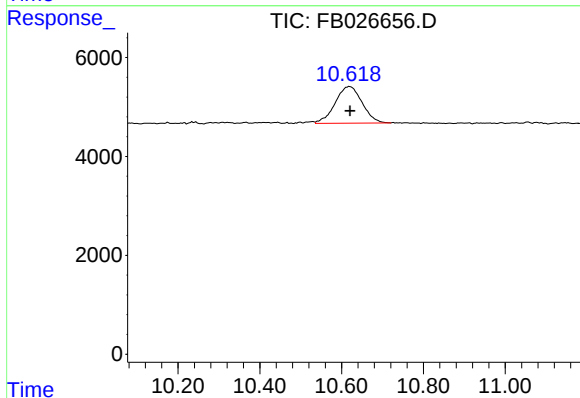


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 33955
Conc: 1.55 ng/ml

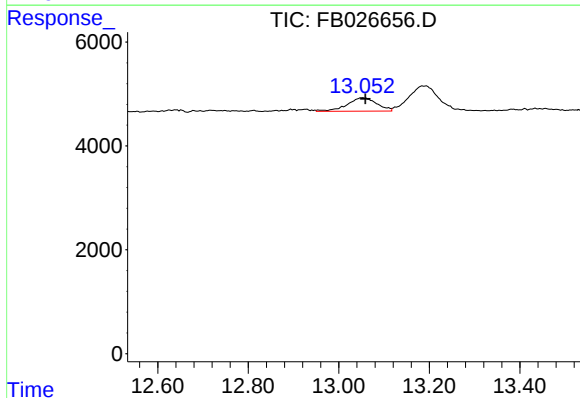


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 11731
Conc: 0.58 ng/ml

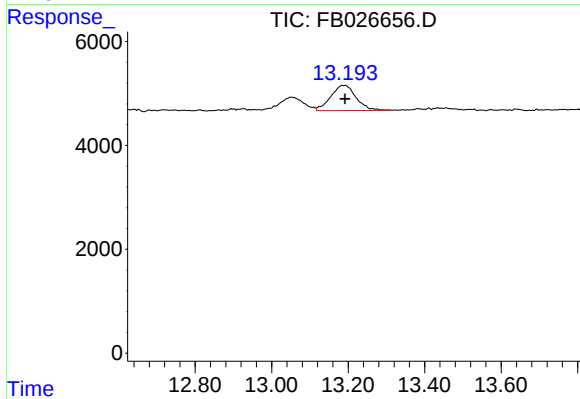


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.003 min
Response: 22266
Conc: 1.10 ng/ml

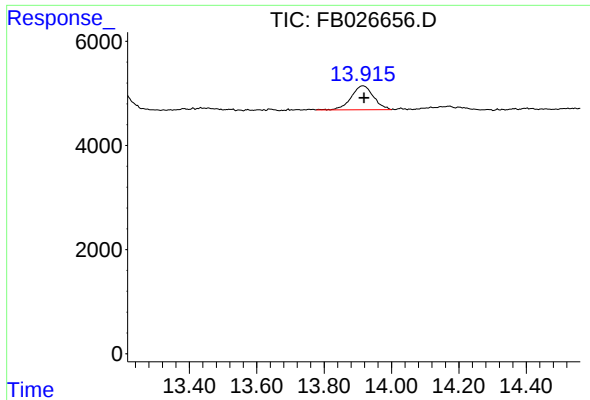

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 21136
Conc: 1.06 ng/ml

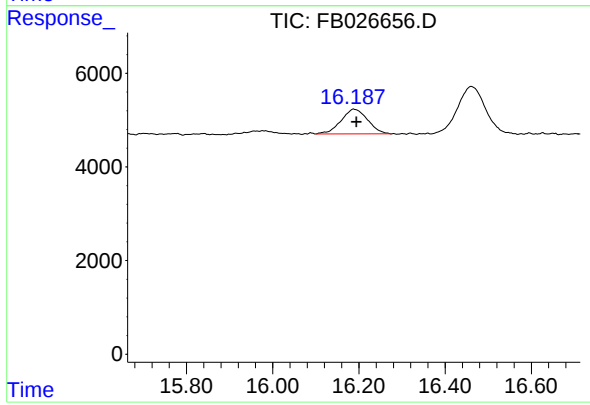

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.006 min
Response: 22592
Conc: 1.13 ng/ml