

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026658.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 14:13
 Operator : AJ/MA
 Sample : N1645-02
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:00:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	182401	17.382 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	127038	6.710 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	139019	6.707 ng/ml
3) t n-Heptane	7.752	45998	2.324 ng/ml
4) t Benzene	7.886	54128	2.346 ng/ml
6) t Toluene	10.619	151404	6.916 ng/ml
7) t Ethylbenzene	13.056	46152	2.296 ng/ml
8) t m-Xylene	13.189	91229	4.527 ng/ml
9) t O-Xylene	13.916	89936	4.508 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	92259	4.630 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026658.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 14:13
Operator : AJ/MA
Sample : N1645-02
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:00:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

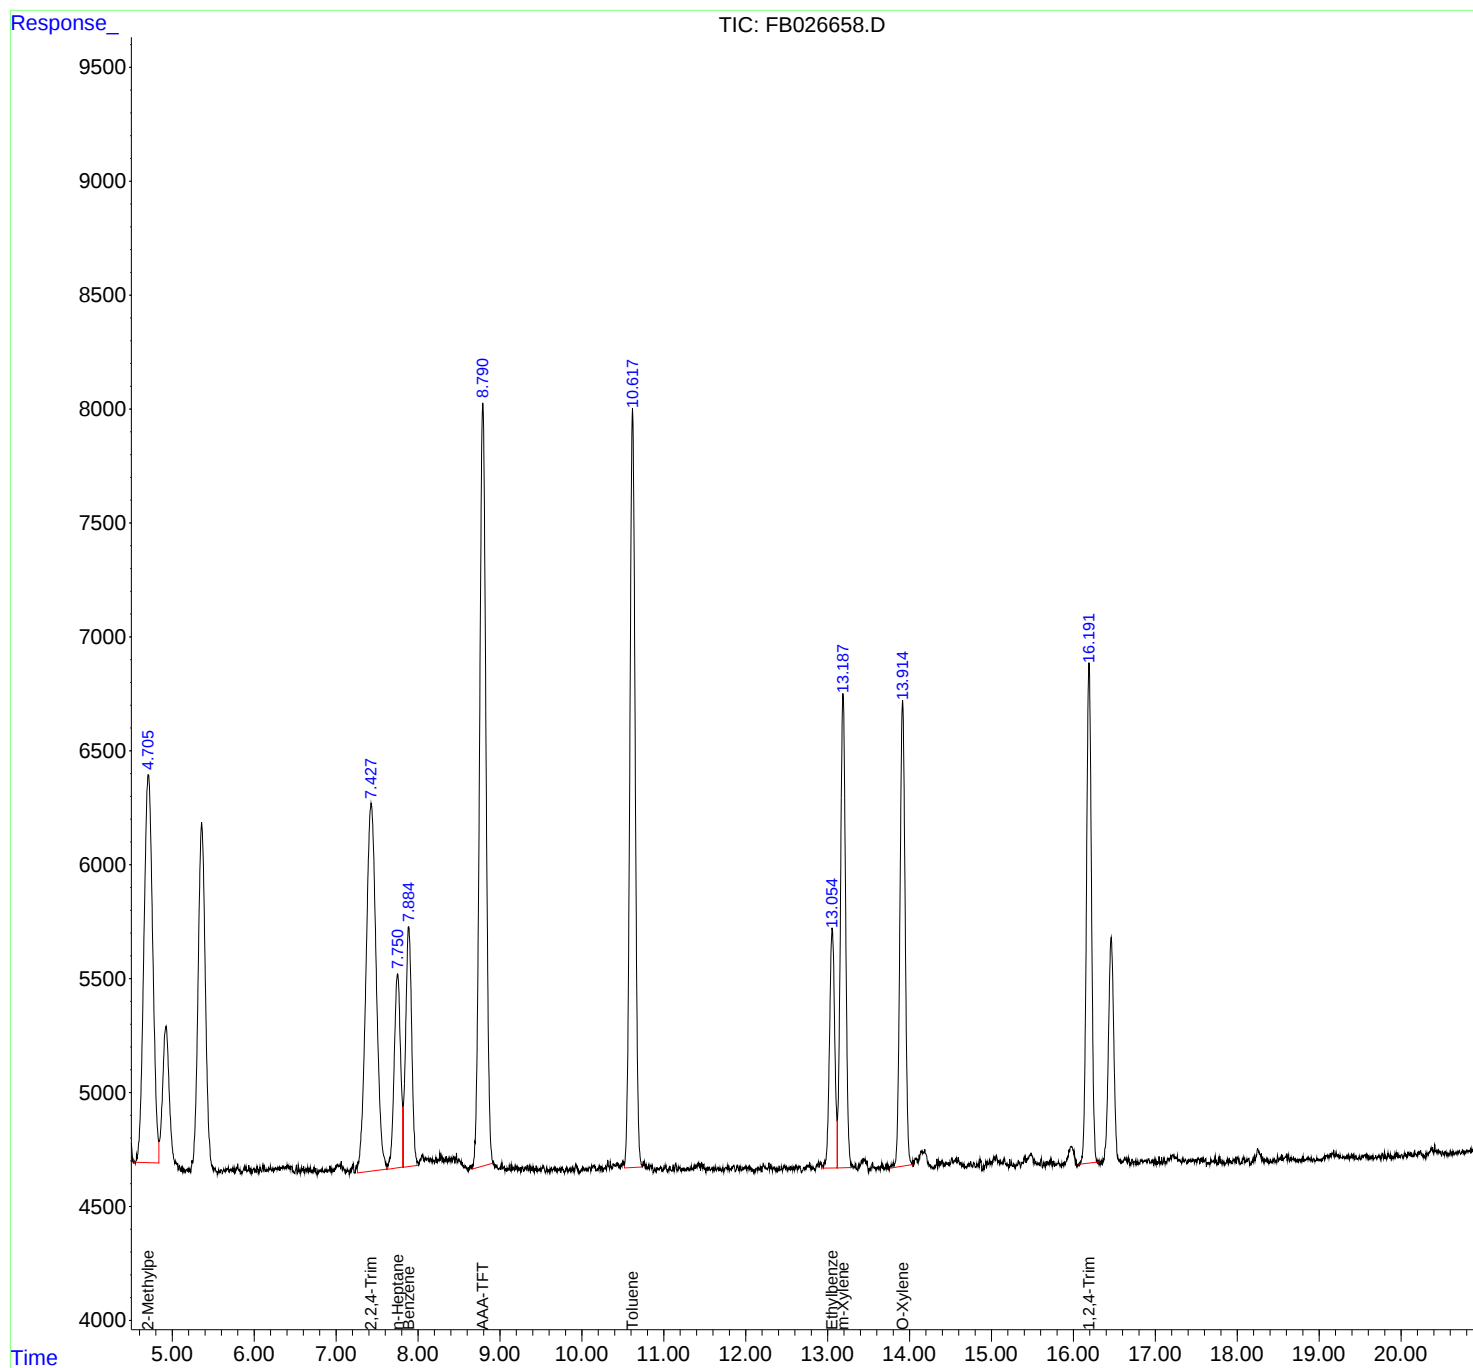

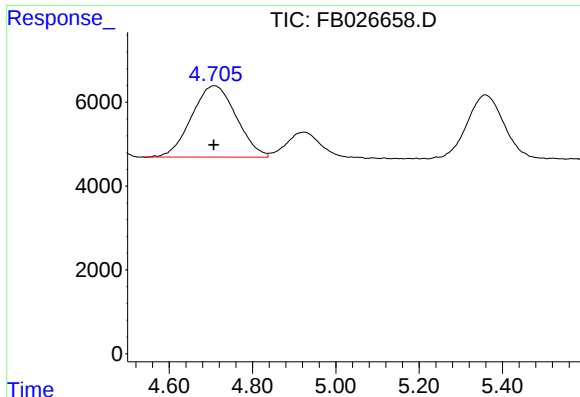


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.001 min
Response: 127038
Conc: 6.71 ng/ml

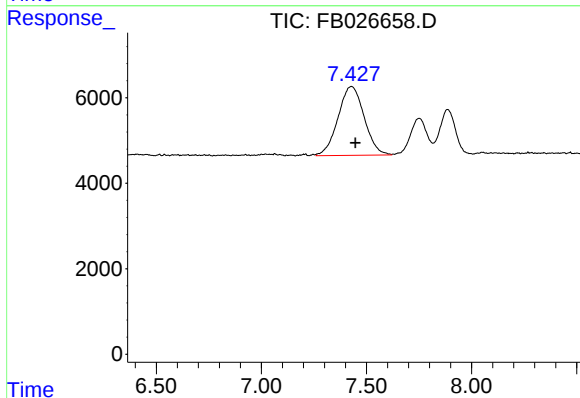


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.019 min
Response: 139019
Conc: 6.71 ng/ml

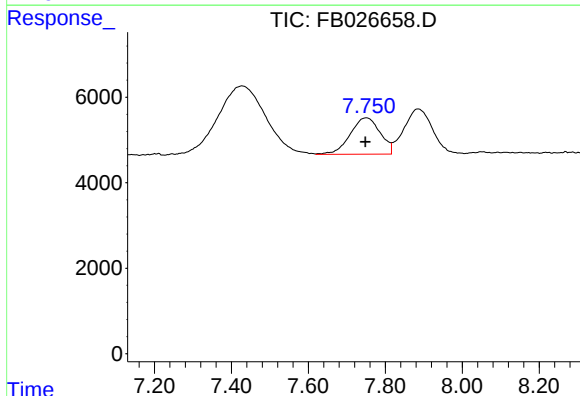


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.003 min
Response: 45998
Conc: 2.32 ng/ml

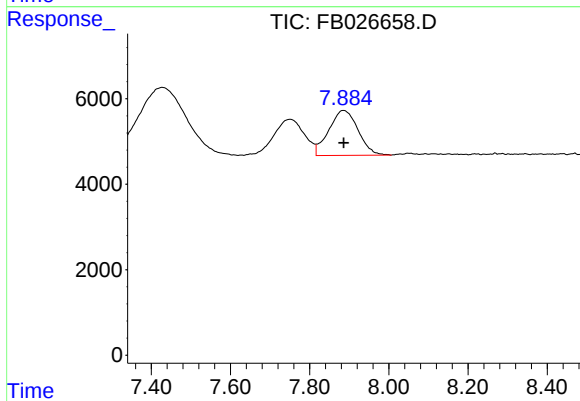


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 54128
Conc: 2.35 ng/ml

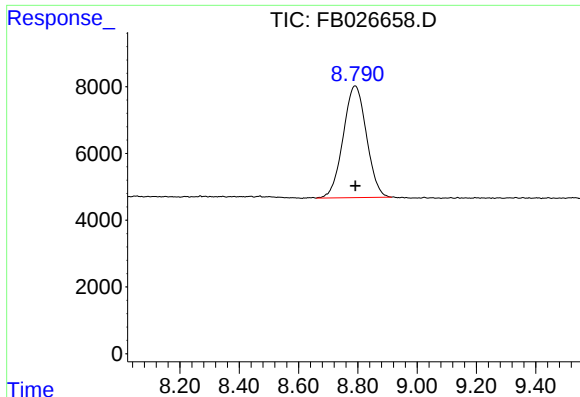


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 182401
Conc: 17.38 ng/ml

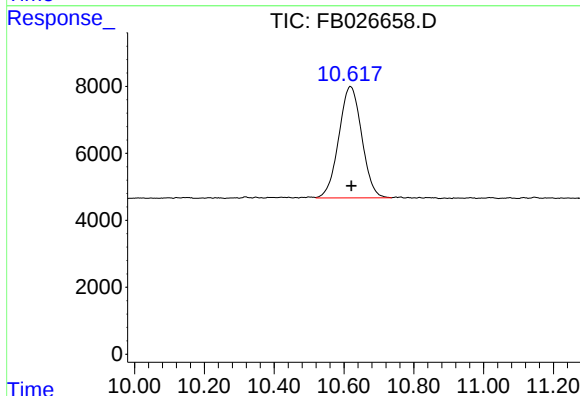


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 151404
Conc: 6.92 ng/ml

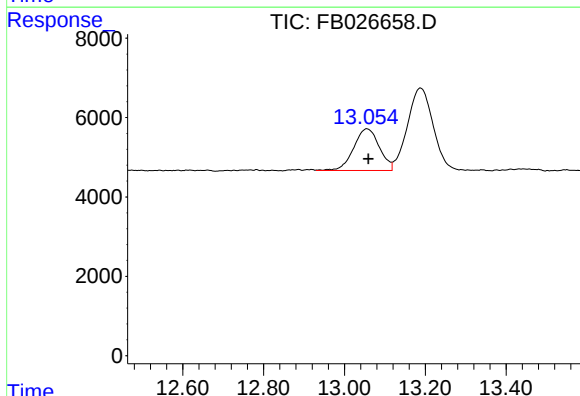


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 46152
Conc: 2.30 ng/ml

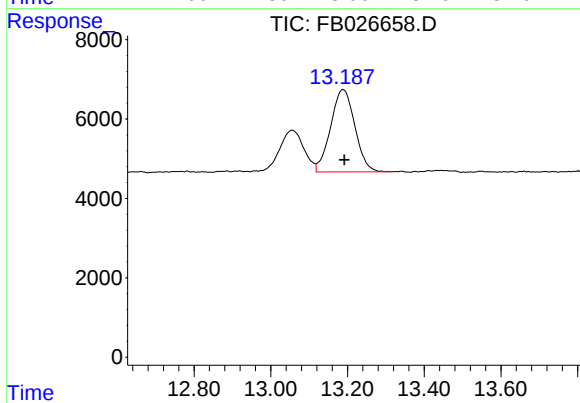


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.003 min
Response: 91229
Conc: 4.53 ng/ml

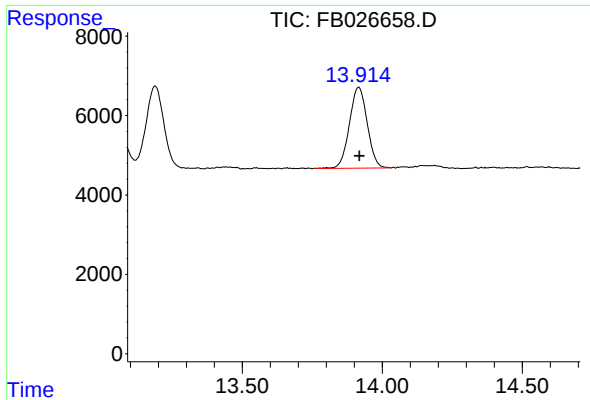

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 89936
Conc: 4.51 ng/ml

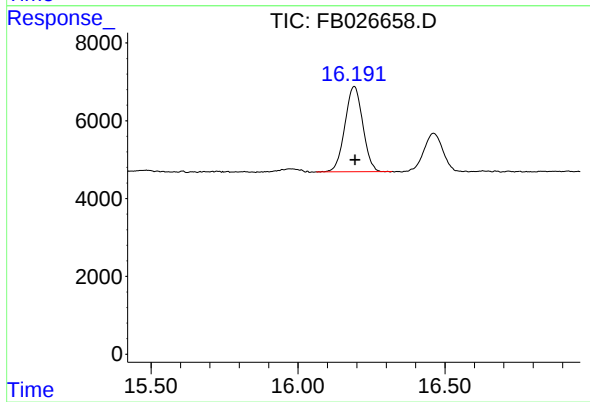

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.003 min
Response: 92259
Conc: 4.63 ng/ml