

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026659.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 14:54
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:00:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	231195	22.032 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	419470	22.155 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	446044	21.520 ng/ml
3) t n-Heptane	7.750	151297	7.644 ng/ml
4) t Benzene	7.886	179613	7.784 ng/ml
6) t Toluene	10.619	522023	23.845 ng/ml
7) t Ethylbenzene	13.056	158131	7.868 ng/ml
8) t m-Xylene	13.189	316685	15.714 ng/ml
9) t O-Xylene	13.916	314373	15.758 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	313424	15.731 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026659.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 14:54
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:00:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

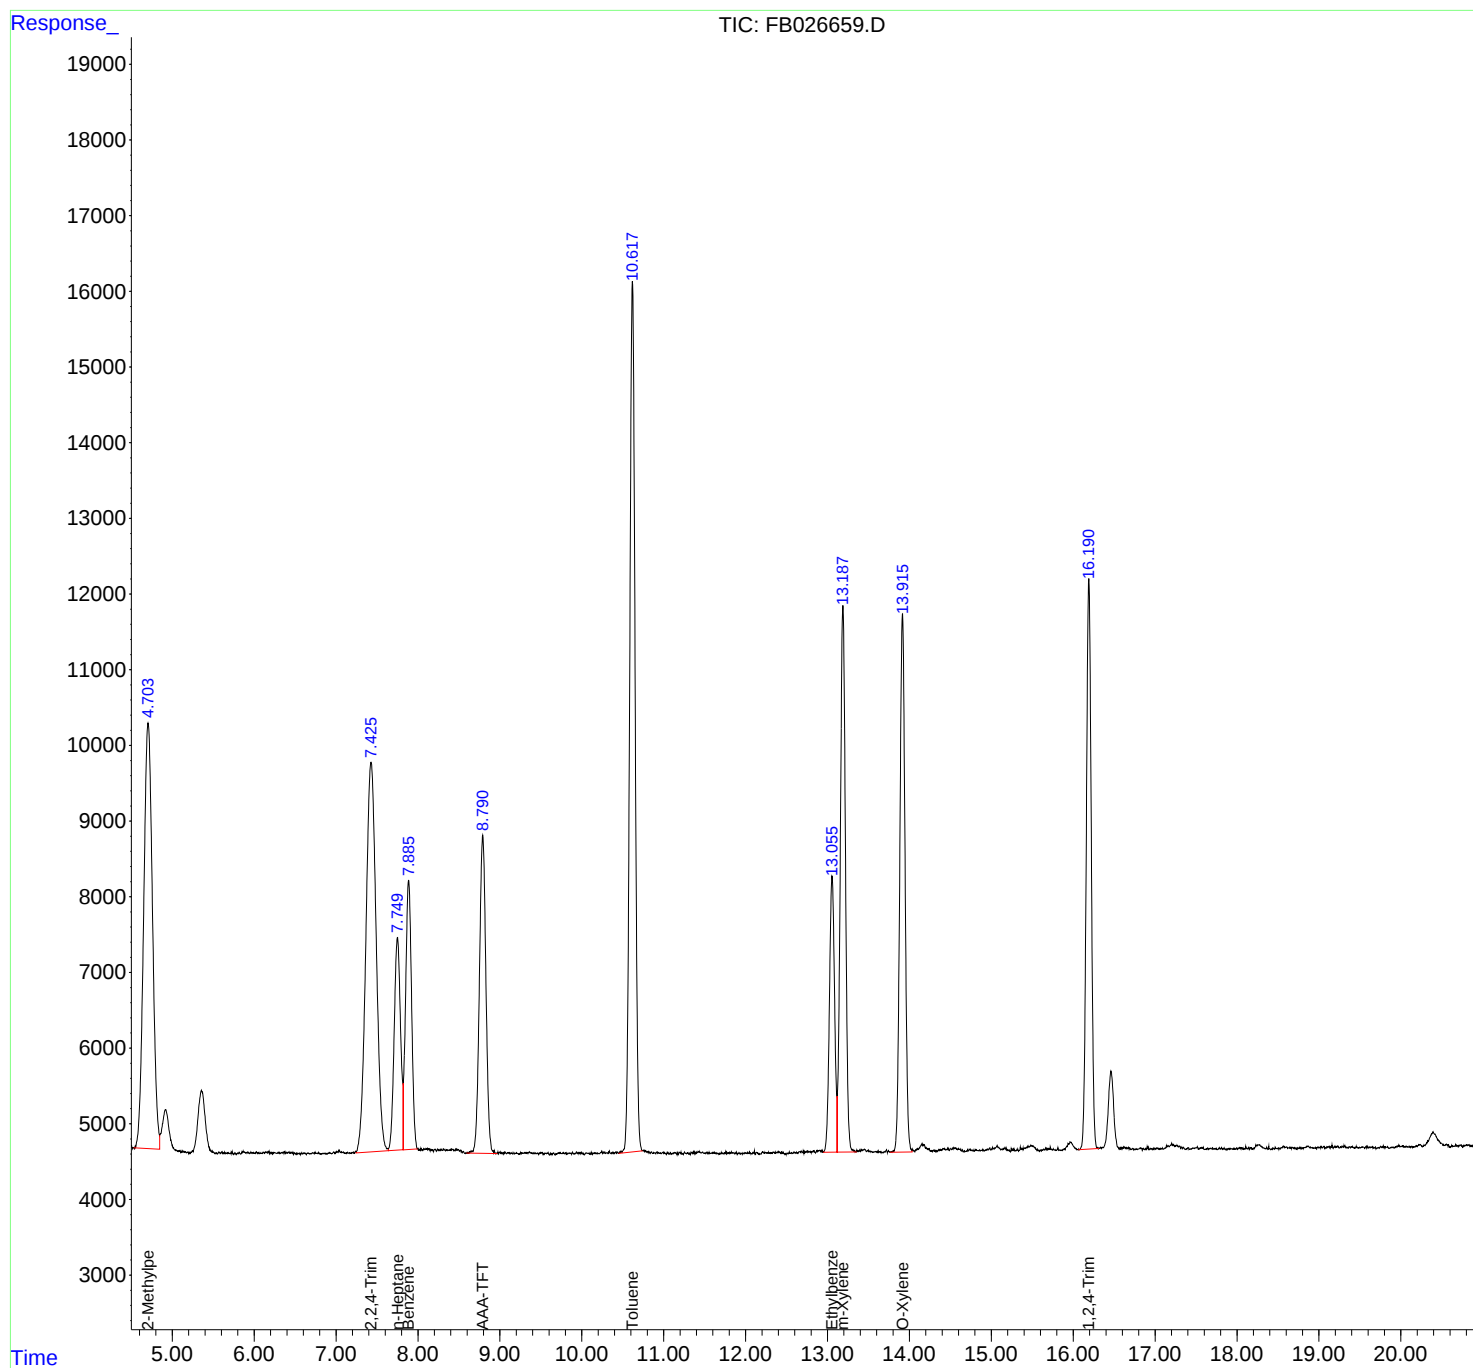

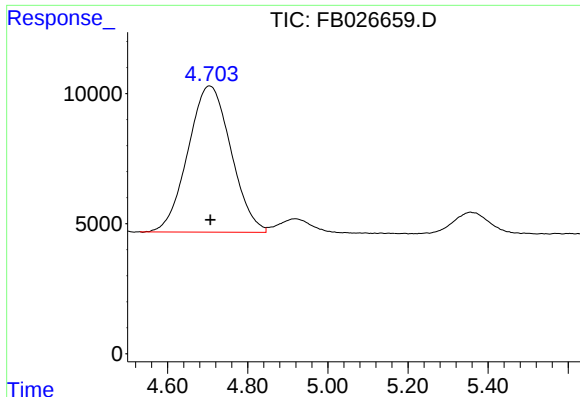


#1 2-Methylpentane

R.T.: 4.705 min
Delta R.T.: -0.002 min
Response: 419470
Conc: 22.15 ng/ml

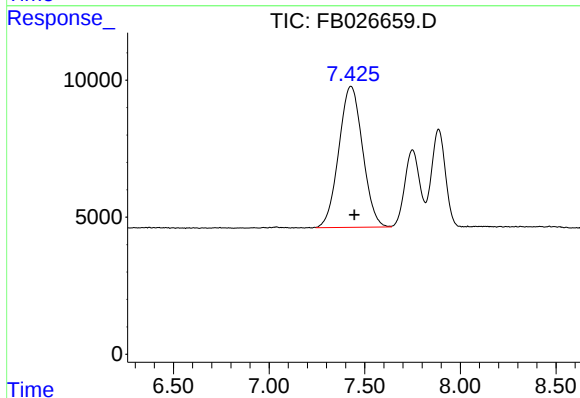


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.020 min
Response: 446044
Conc: 21.52 ng/ml

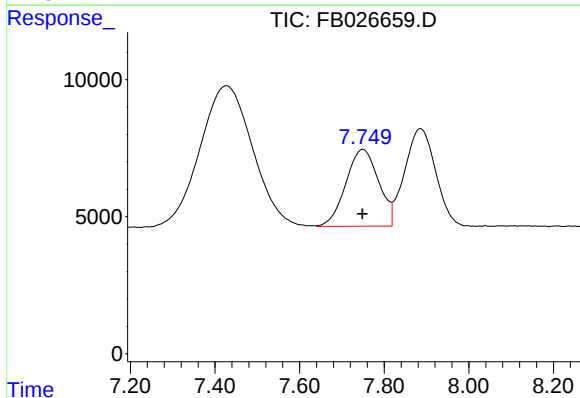


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 151297
Conc: 7.64 ng/ml

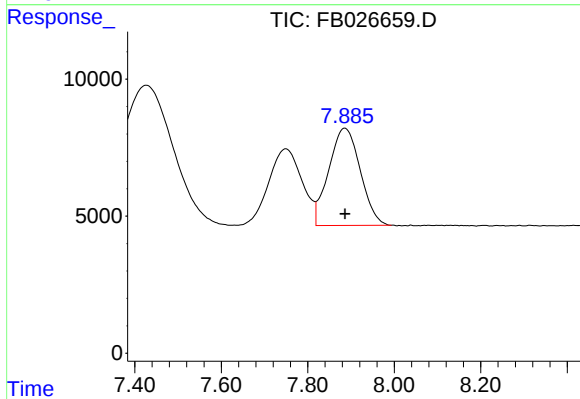


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 179613
Conc: 7.78 ng/ml

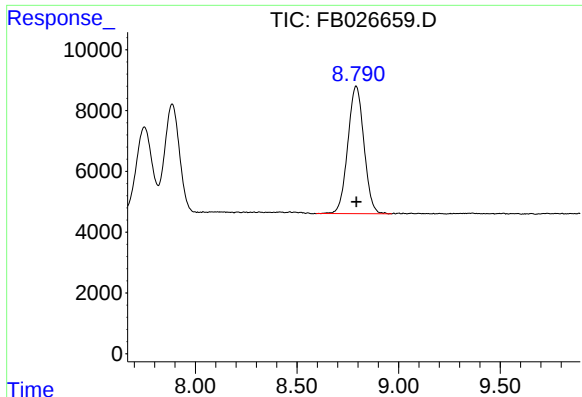


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 231195
Conc: 22.03 ng/ml

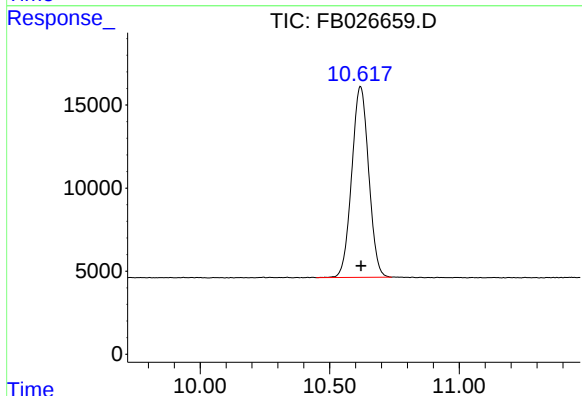


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 522023
Conc: 23.84 ng/ml

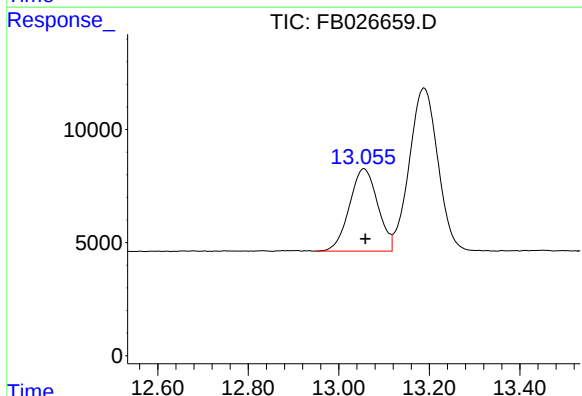


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 158131
Conc: 7.87 ng/ml

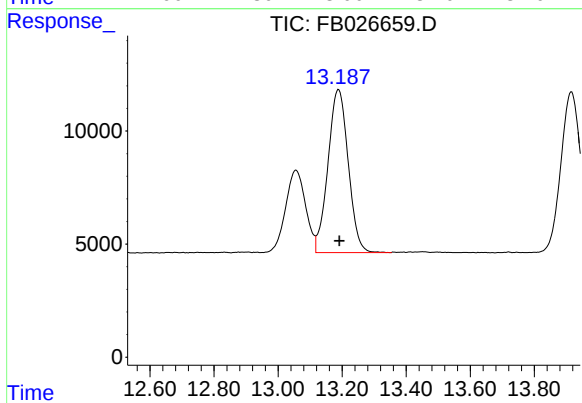


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.003 min
Response: 316685
Conc: 15.71 ng/ml

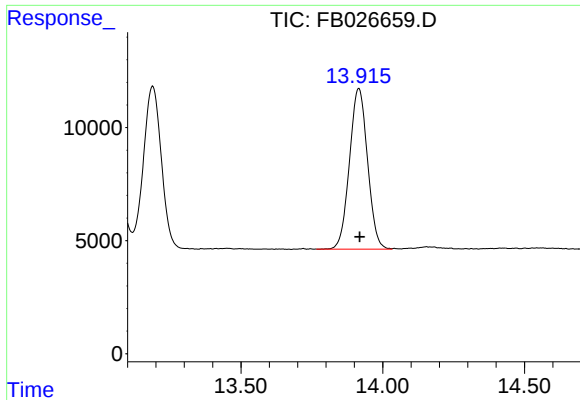

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 314373
Conc: 15.76 ng/ml

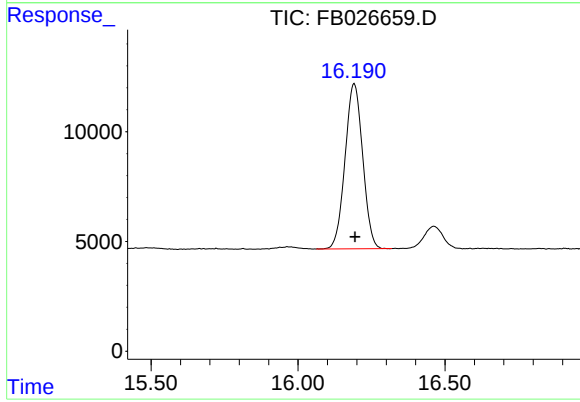

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.003 min
Response: 313424
Conc: 15.73 ng/ml