

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026665.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 18:51
 Operator : AJ/MA
 Sample : N1645-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:01:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.790	212918	20.291 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.705	128061	6.764 ng/ml
2) t	2,2,4-Trimethylpentane	7.433	143077	6.903 ng/ml
3) t	n-Heptane	7.750	46799	2.364 ng/ml
4) t	Benzene	7.883	53100	2.301 ng/ml
6) t	Toluene	10.618	149267	6.818 ng/ml
7) t	Ethylbenzene	13.056	45993	2.288 ng/ml
8) t	m-Xylene	13.187	92469	4.588 ng/ml
9) t	O-Xylene	13.915	92182	4.621 ng/ml
10) t	1,2,4-Trimethylbenzene	16.192	93440	4.690 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026665.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 18:51
Operator : AJ/MA
Sample : N1645-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:01:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

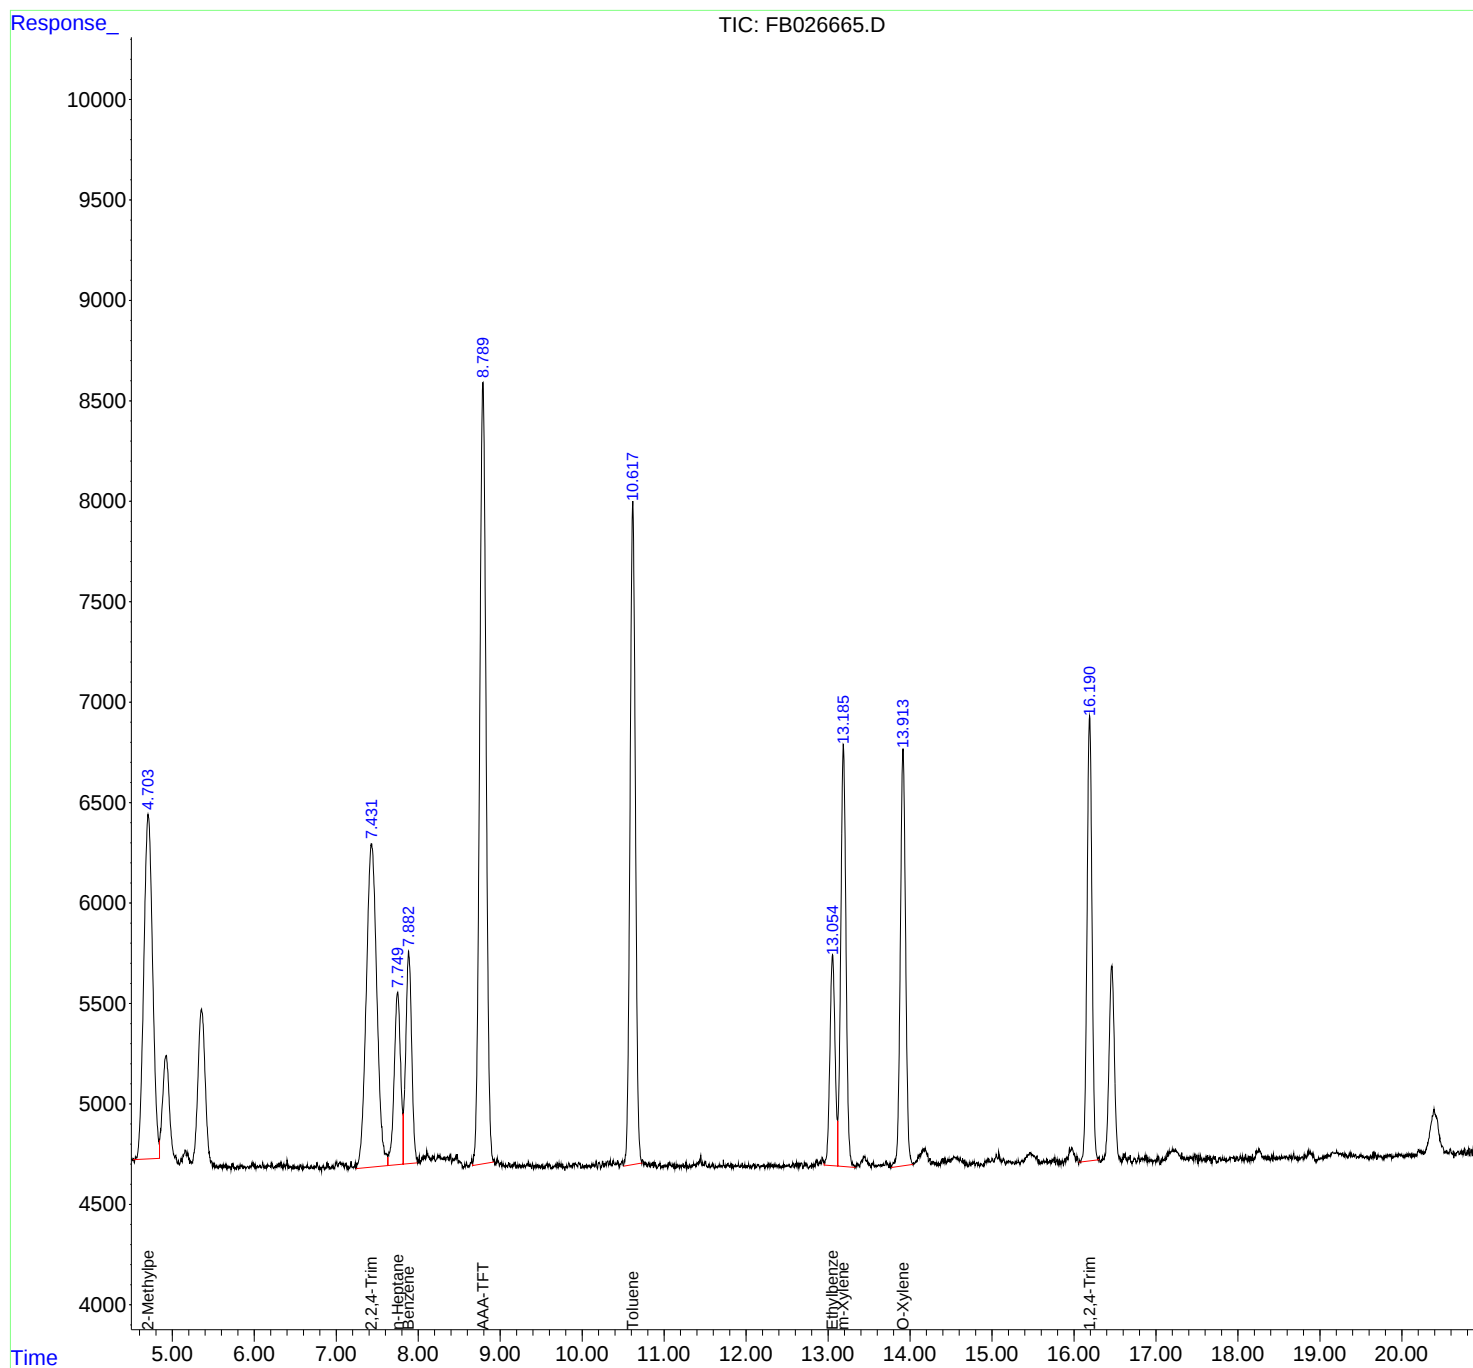

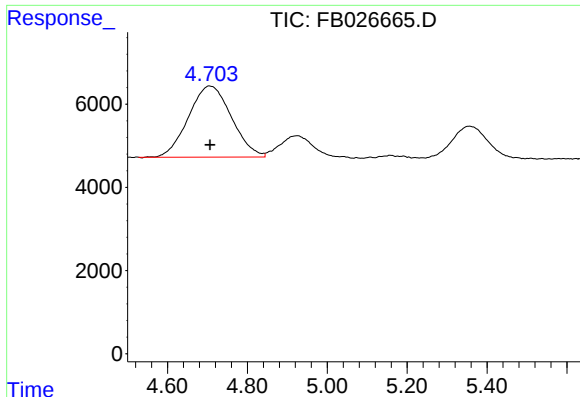


#1 2-Methylpentane

R.T.: 4.705 min
Delta R.T.: -0.002 min
Response: 128061
Conc: 6.76 ng/ml

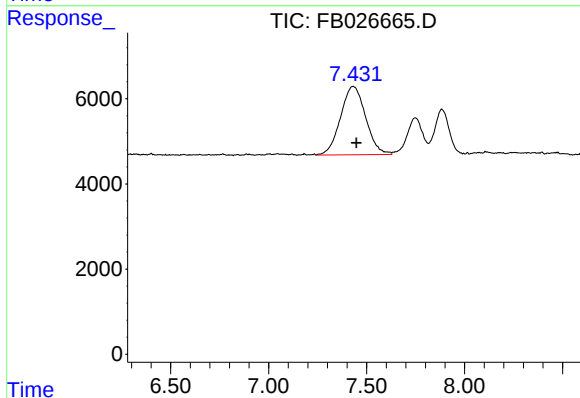


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.015 min
Response: 143077
Conc: 6.90 ng/ml

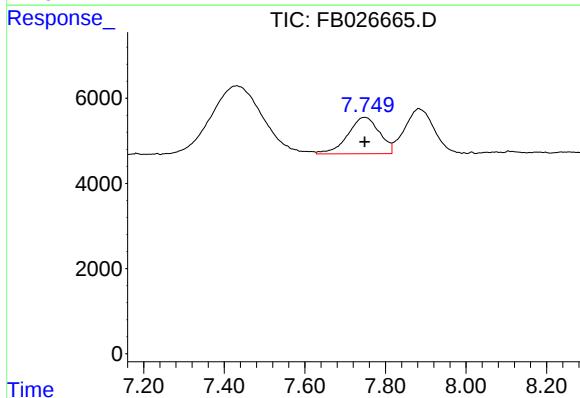


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.002 min
Response: 46799
Conc: 2.36 ng/ml

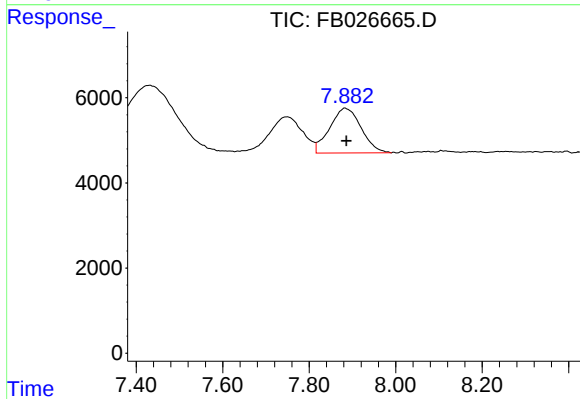


#4 Benzene

R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 53100
Conc: 2.30 ng/ml

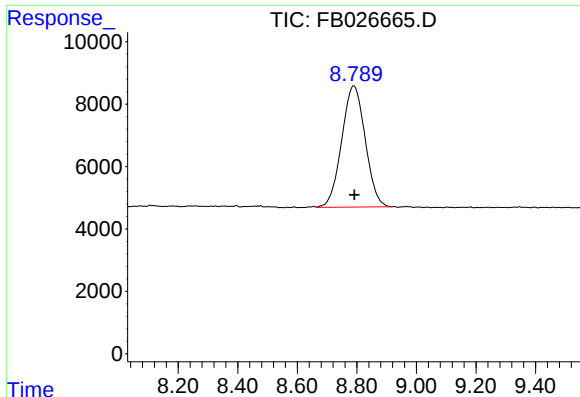


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 212918
Conc: 20.29 ng/ml

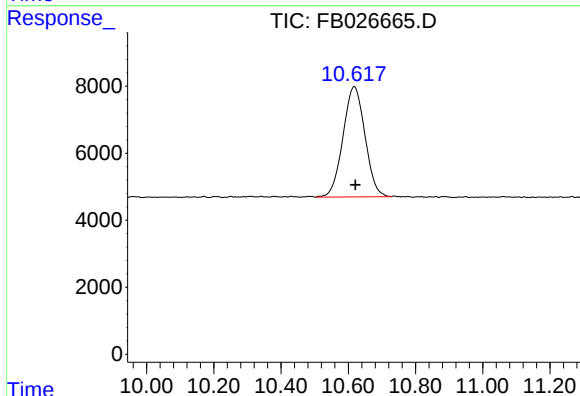


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 149267
Conc: 6.82 ng/ml

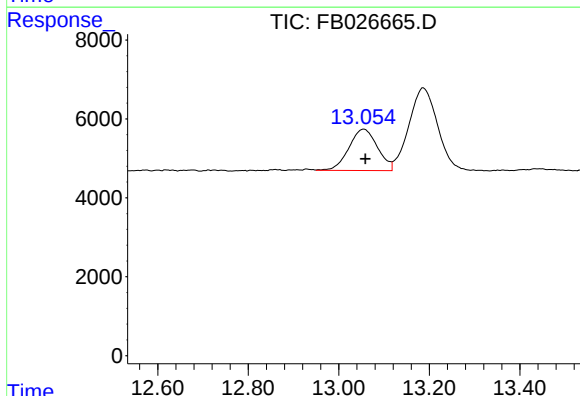


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 45993
Conc: 2.29 ng/ml

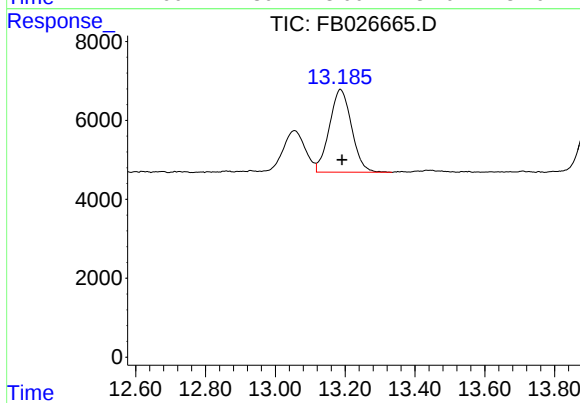


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 92469
Conc: 4.59 ng/ml

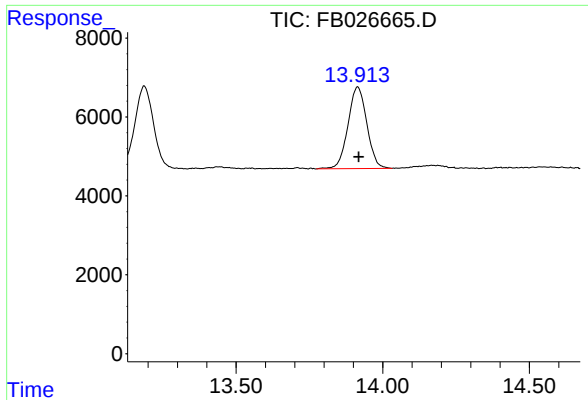

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.004 min
Response: 92182
Conc: 4.62 ng/ml

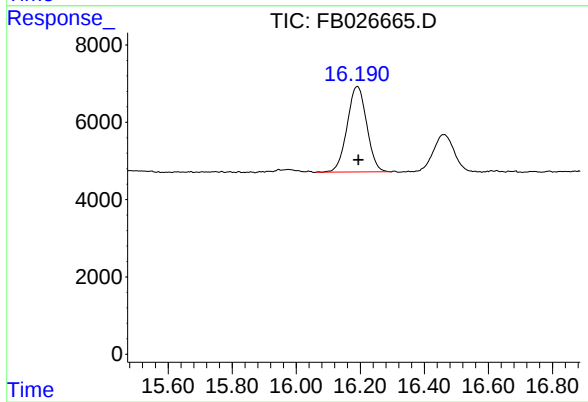

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.003 min
Response: 93440
Conc: 4.69 ng/ml