

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026655.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 12:13
 Operator : AJ/MA
 Sample : BSF0309S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:00:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	212376	20.239 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	560907	29.625 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	590267	28.478 ng/ml
3) t n-Heptane	7.750	198718	10.040 ng/ml
4) t Benzene	7.886	230766	10.001 ng/ml
6) t Toluene	10.619	647851	29.592 ng/ml
7) t Ethylbenzene	13.056	193254	9.616 ng/ml
8) t m-Xylene	13.188	387911	19.249 ng/ml
9) t O-Xylene	13.916	378980	18.996 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	375428	18.843 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026655.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 12:13
Operator : AJ/MA
Sample : BSF0309S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:00:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

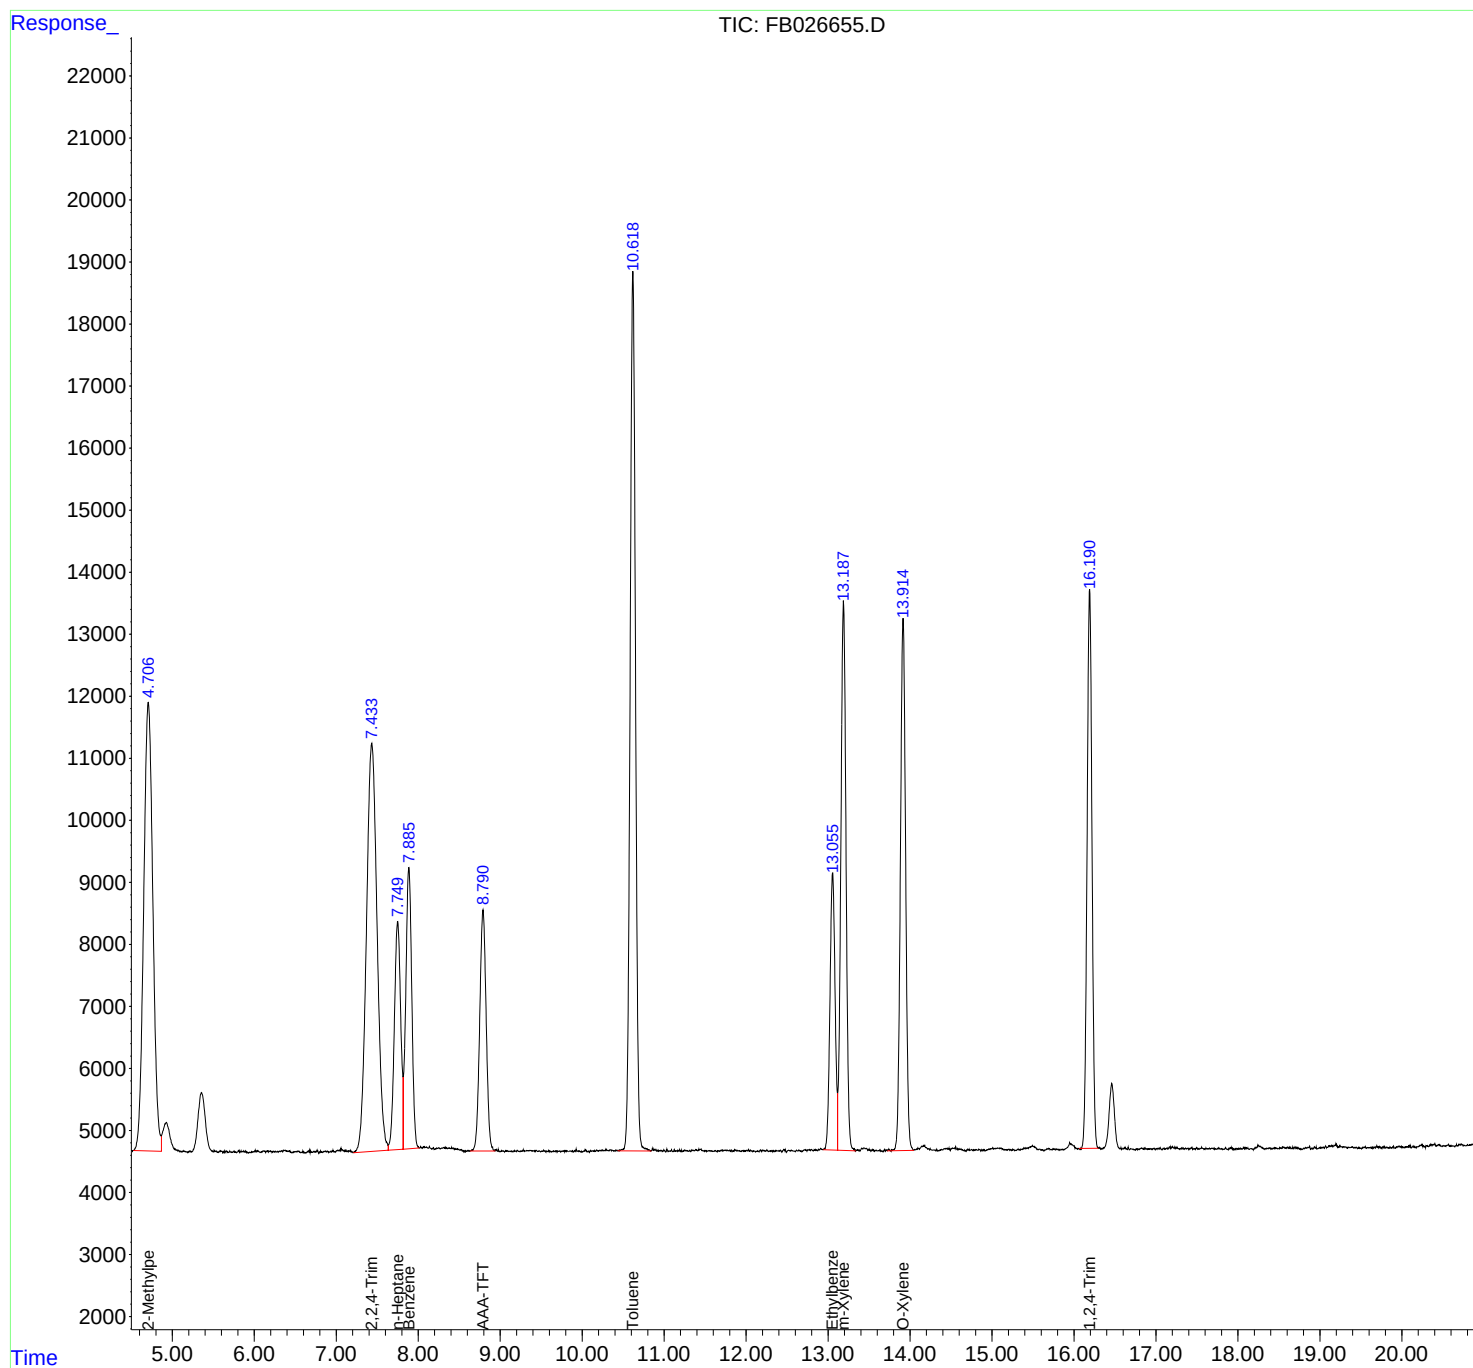

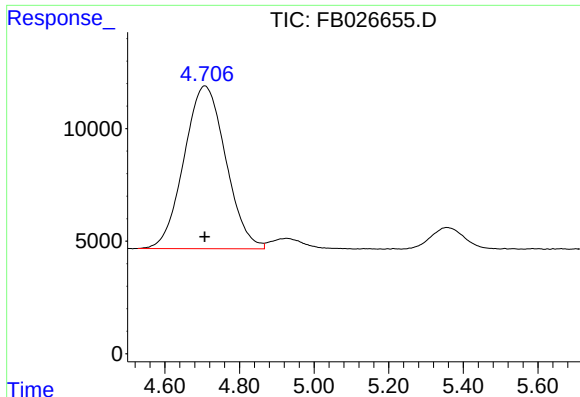


#1 2-Methylpentane

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 560907
Conc: 29.63 ng/ml

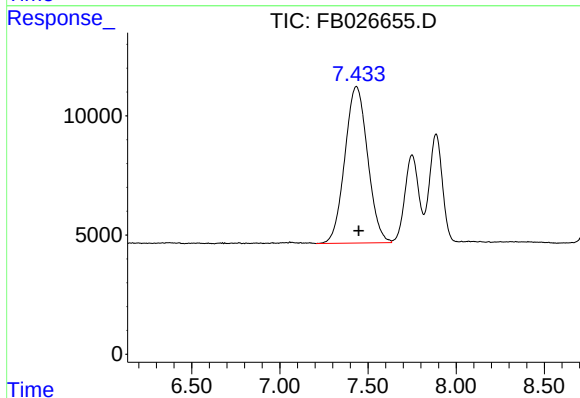


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.013 min
Response: 590267
Conc: 28.48 ng/ml

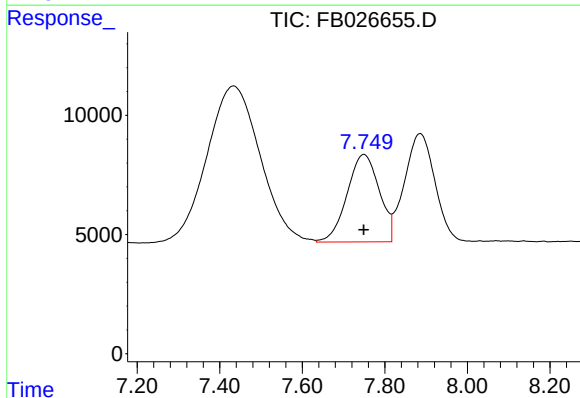


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 198718
Conc: 10.04 ng/ml

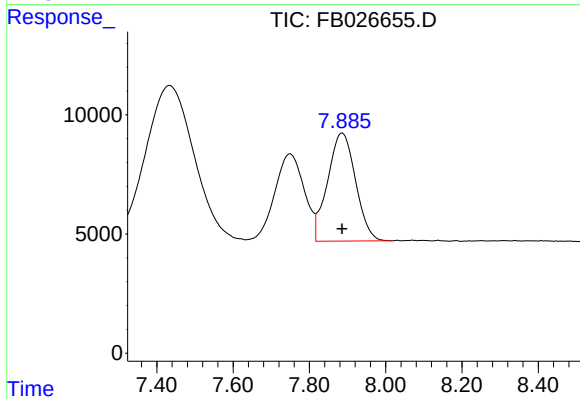


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 230766
Conc: 10.00 ng/ml

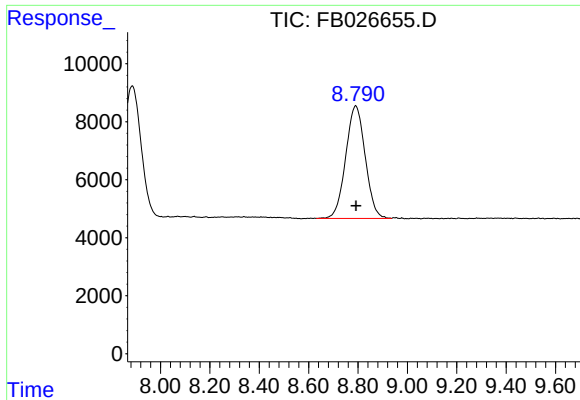


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 212376
Conc: 20.24 ng/ml

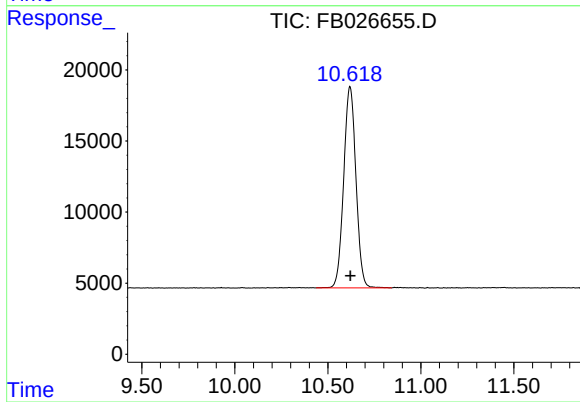


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 647851
Conc: 29.59 ng/ml

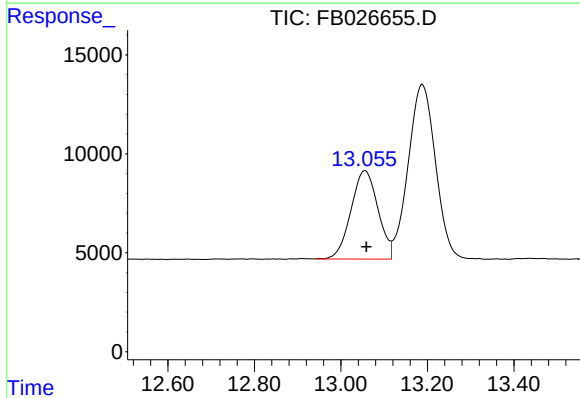


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 193254
Conc: 9.62 ng/ml

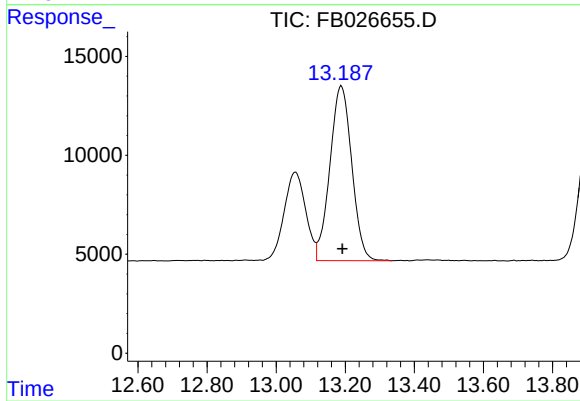

#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: -0.003 min
Response: 387911
Conc: 19.25 ng/ml

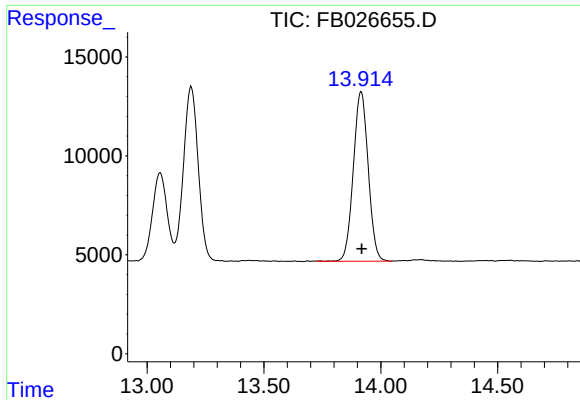


#9 O-Xylene

R.T.: 13.916 min

Delta R.T.: -0.003 min

Response: 378980

Conc: 19.00 ng/ml

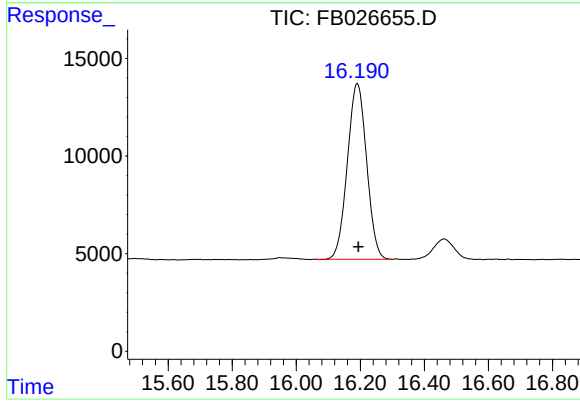

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min

Delta R.T.: -0.003 min

Response: 375428

Conc: 18.84 ng/ml