

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026656.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 12:51
 Operator : AJ/MA
 Sample : N1645-01
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:09:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.791	188914	18.003 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.696	23319	1.232 ng/mlm
2) t	2,2,4-Trimethylpentane	7.429	30145	1.454 ng/ml
3) t	n-Heptane	7.740	9867	0.499 ng/ml
4) t	Benzene	7.880	11417	0.495 ng/mlm
6) t	Toluene	10.619	33955	1.551 ng/ml
7) t	Ethylbenzene	13.053	11731	0.584 ng/ml
8) t	m-Xylene	13.194	22266	1.105 ng/ml
9) t	O-Xylene	13.916	21136	1.059 ng/ml
10) t	1,2,4-Trimethylbenzene	16.188	22592	1.134 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026656.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 12:51
Operator : AJ/MA
Sample : N1645-01
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:09:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

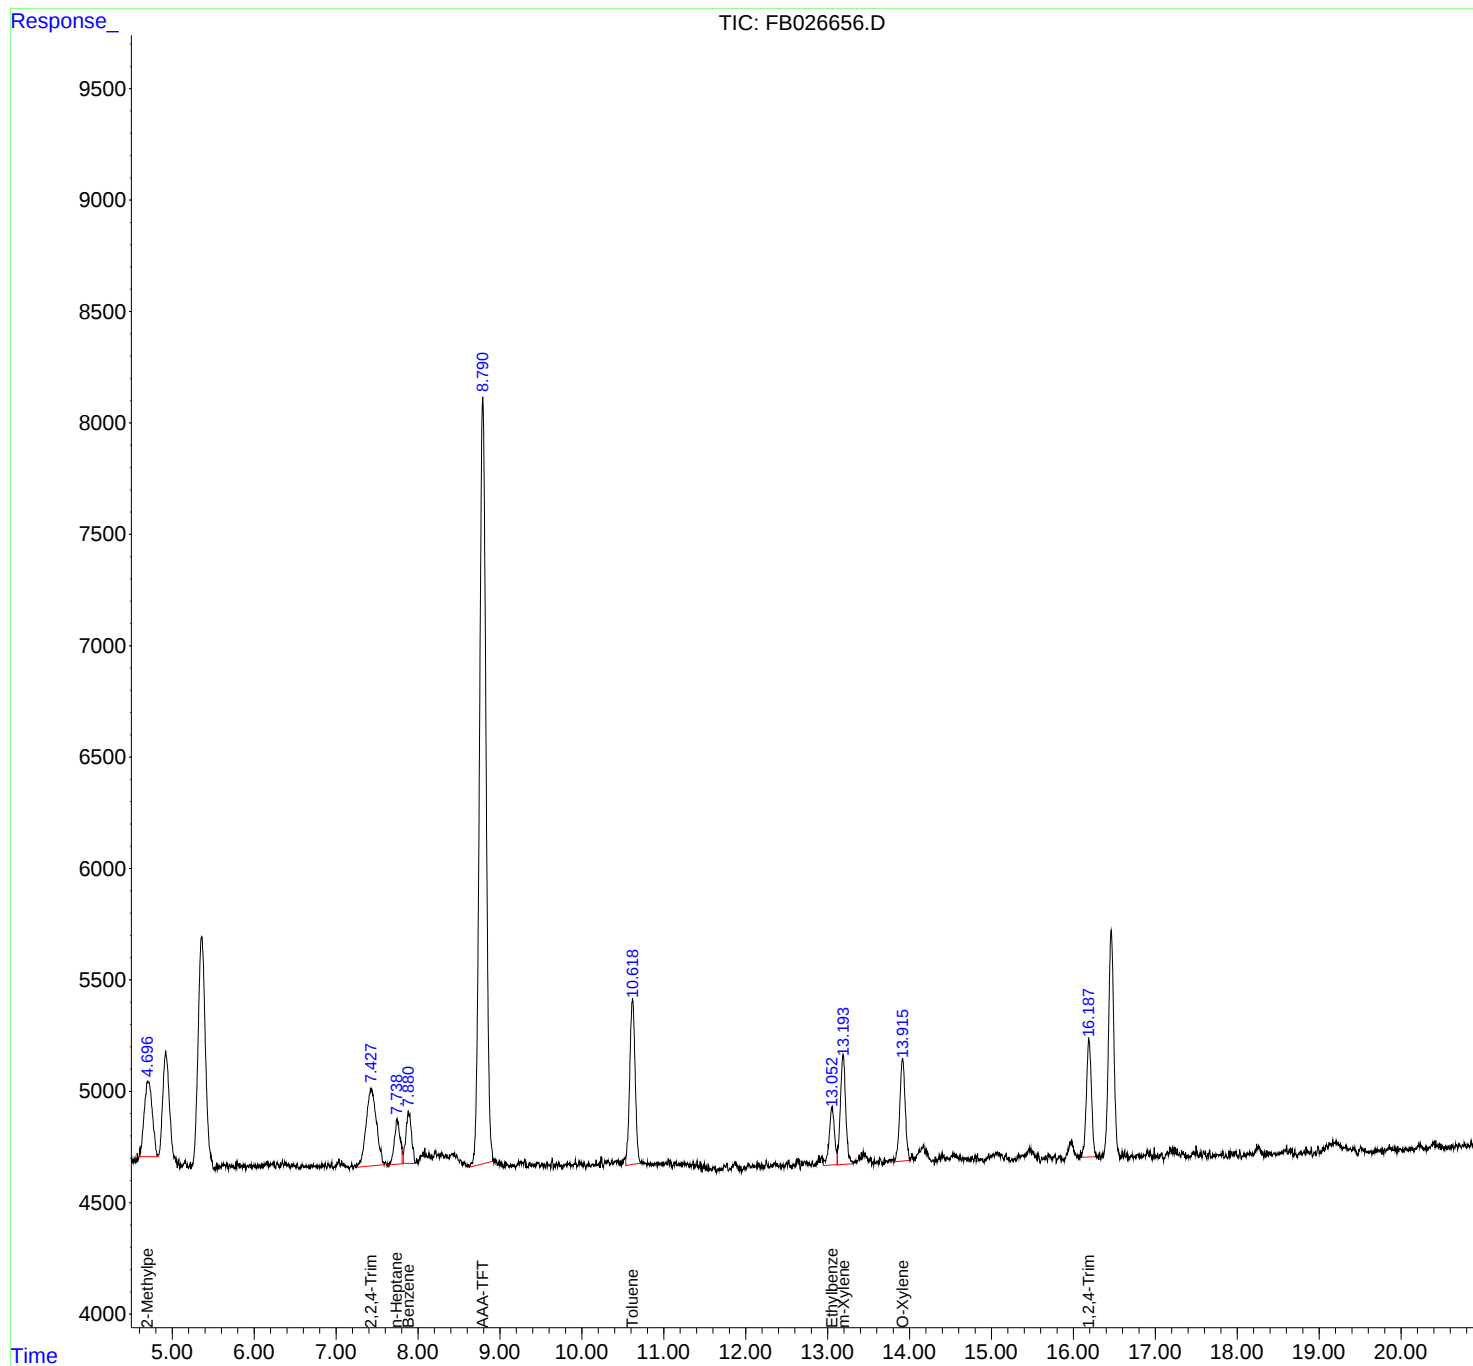

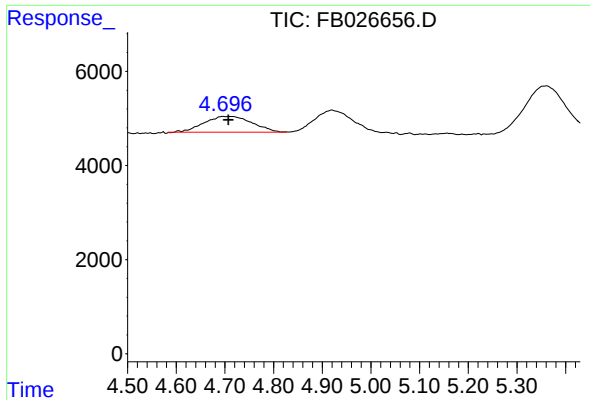


#1 2-Methylpentane

R.T.: 4.696 min
Delta R.T.: -0.011 min
Response: 23319
Conc: 1.23 ng/ml m

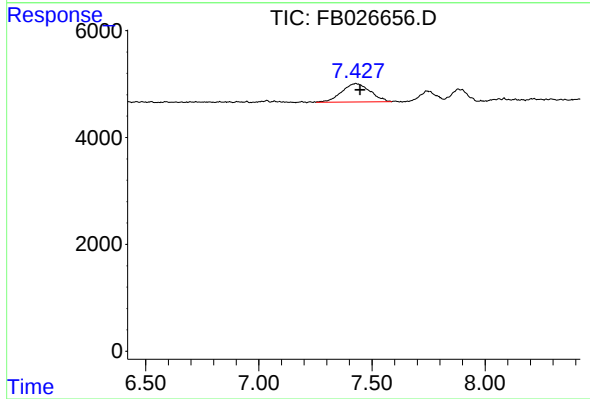


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.018 min
Response: 30145
Conc: 1.45 ng/ml

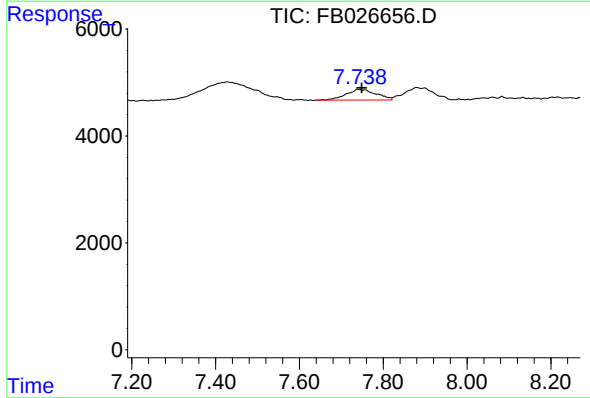


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.009 min
Response: 9867
Conc: 0.50 ng/ml

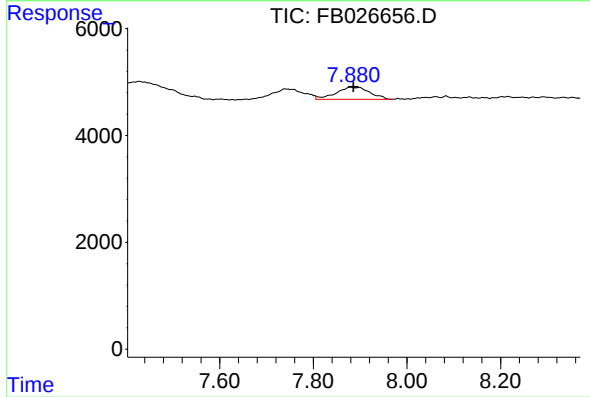


#4 Benzene

R.T.: 7.880 min
Delta R.T.: -0.006 min
Response: 11417
Conc: 0.49 ng/ml m

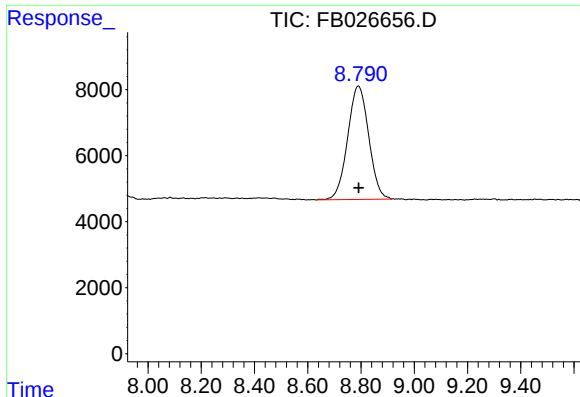


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 188914
Conc: 18.00 ng/ml

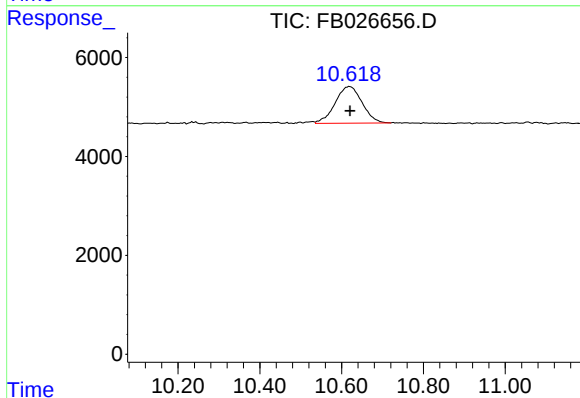


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 33955
Conc: 1.55 ng/ml

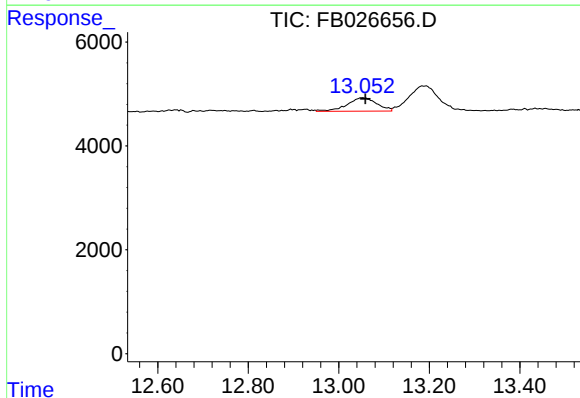


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 11731
Conc: 0.58 ng/ml

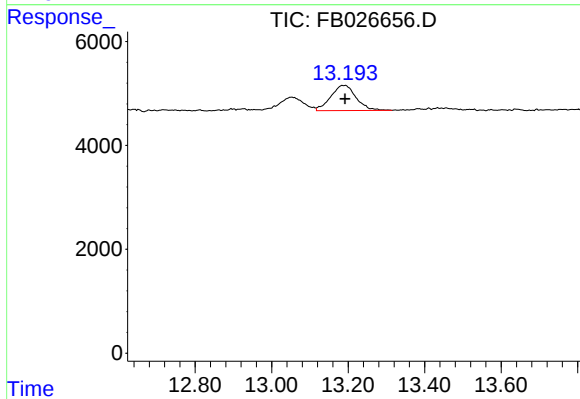


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.003 min
Response: 22266
Conc: 1.10 ng/ml

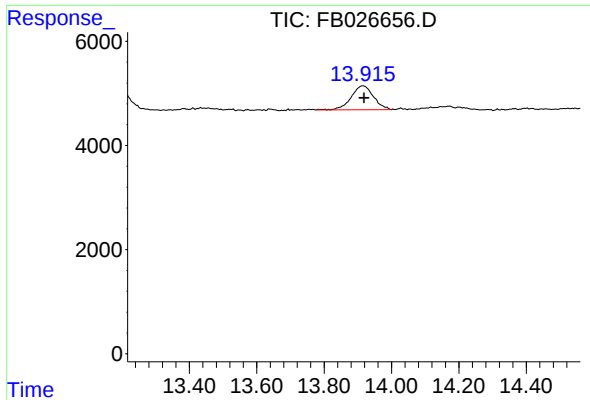

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 21136
Conc: 1.06 ng/ml

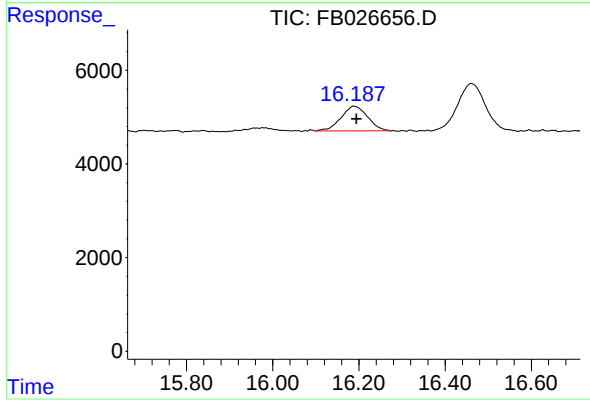

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.006 min
Response: 22592
Conc: 1.13 ng/ml