

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026657.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 13:35
 Operator : AJ/MA
 Sample : N1645-01
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:00:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.791	155575	14.826 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.712	89041	4.703 ng/ml
2) t	2,2,4-Trimethylpentane	7.434	101761	4.910 ng/ml
3) t	n-Heptane	7.754	27670	1.398 ng/ml
4) t	Benzene	7.881	35252	1.528 ng/ml
6) t	Toluene	10.620	102894	4.700 ng/ml
7) t	Ethylbenzene	13.055	34158	1.700 ng/ml
8) t	m-Xylene	13.186	69237	3.436 ng/ml
9) t	O-Xylene	13.916	69792	3.498 ng/ml
10) t	1,2,4-Trimethylbenzene	16.192	75733	3.801 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026657.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 13:35
Operator : AJ/MA
Sample : N1645-01
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:00:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

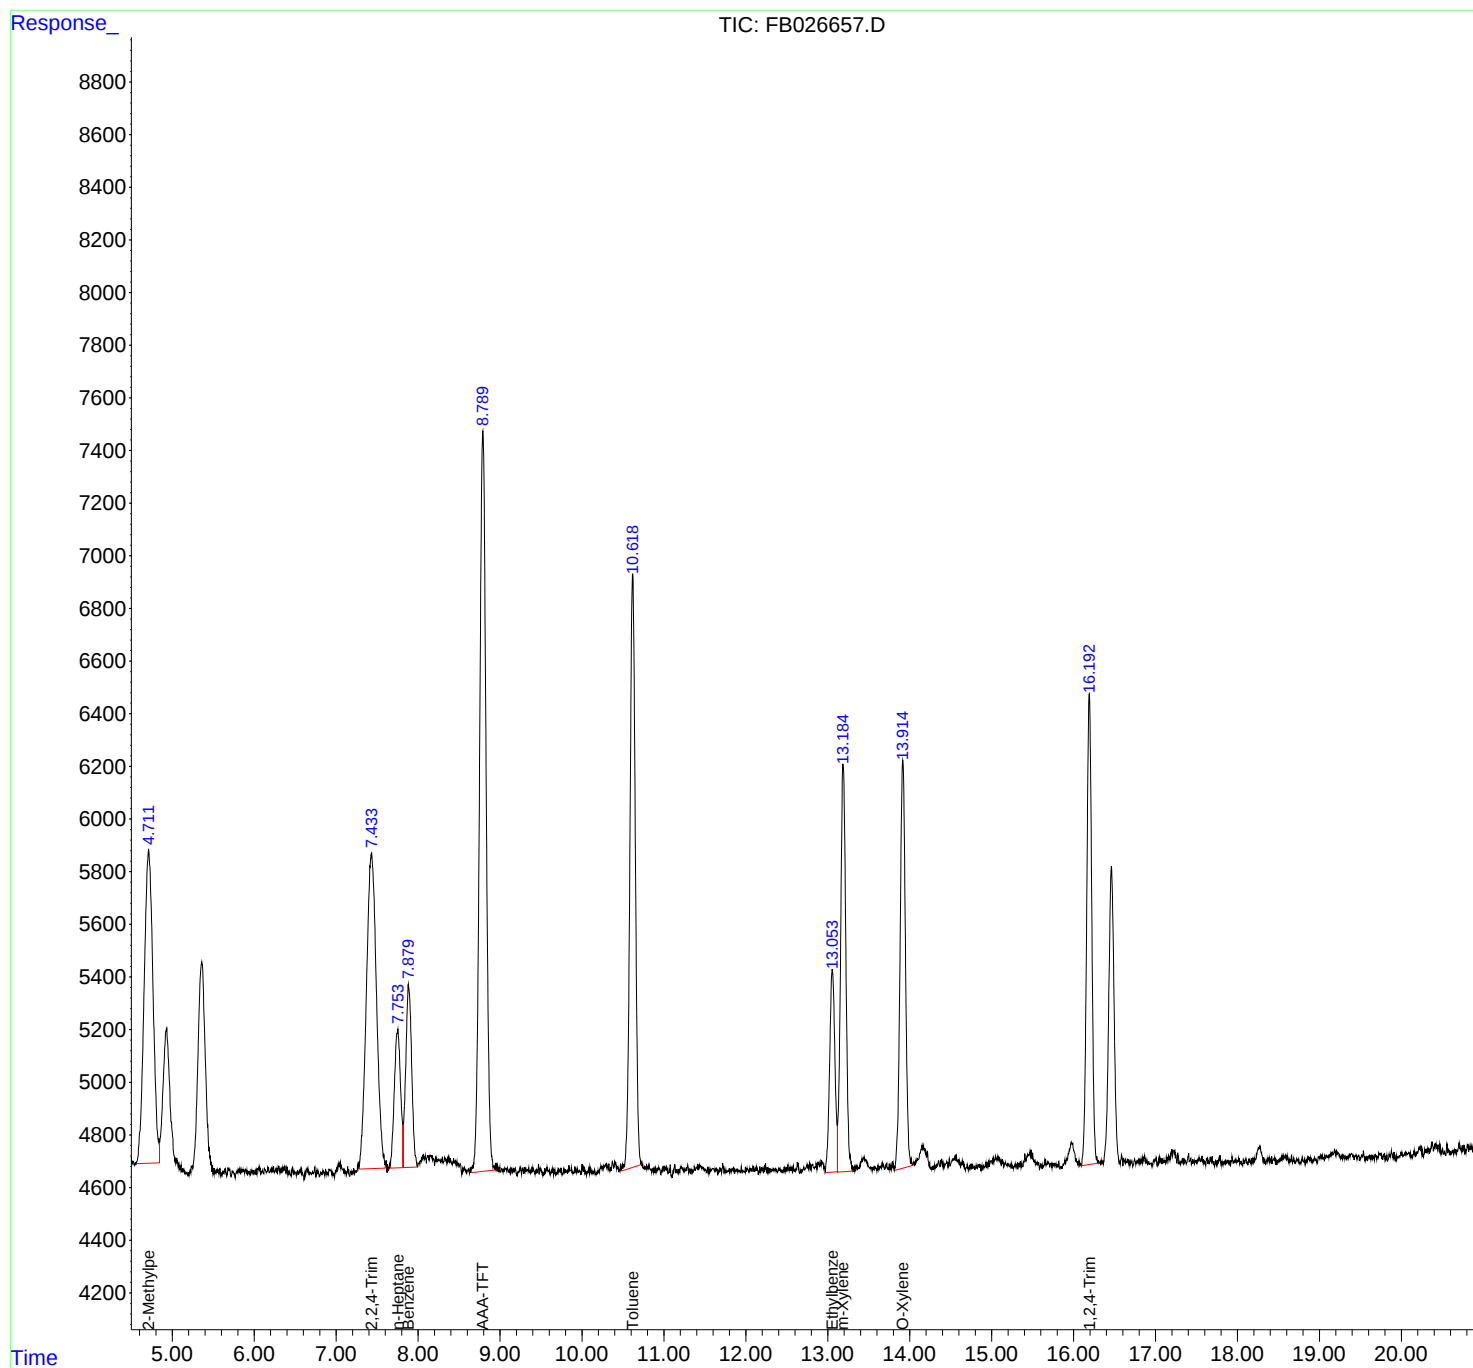

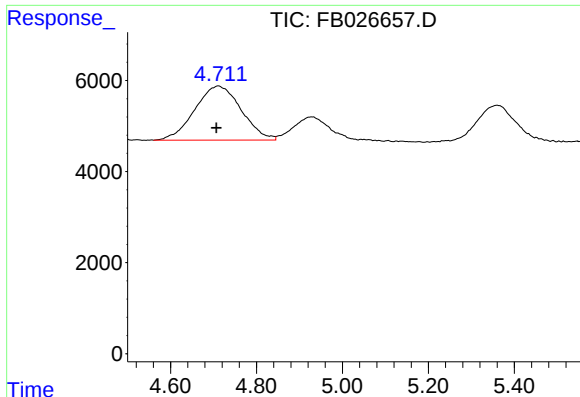


#1 2-Methylpentane

R.T.: 4.712 min
Delta R.T.: 0.005 min
Response: 89041
Conc: 4.70 ng/ml

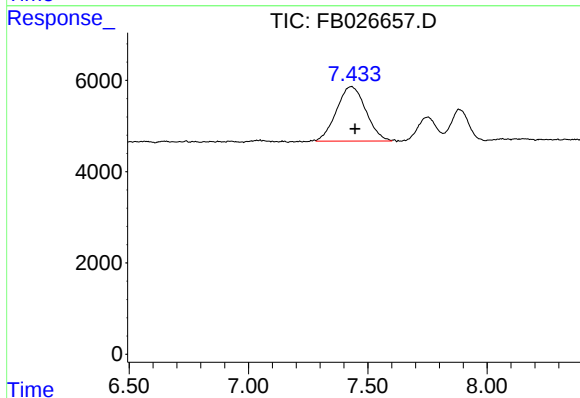


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.013 min
Response: 101761
Conc: 4.91 ng/ml

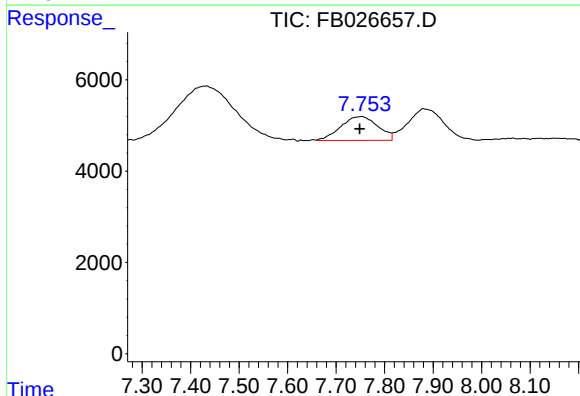


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.005 min
Response: 27670
Conc: 1.40 ng/ml

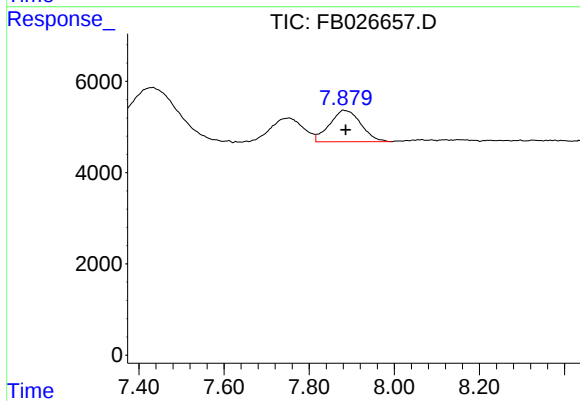


#4 Benzene

R.T.: 7.881 min
Delta R.T.: -0.005 min
Response: 35252
Conc: 1.53 ng/ml

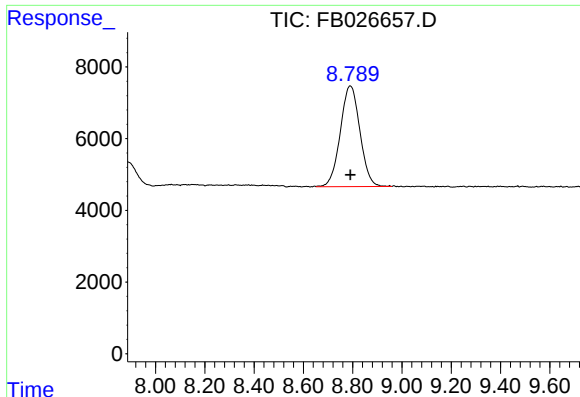


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.001 min
Response: 155575
Conc: 14.83 ng/ml

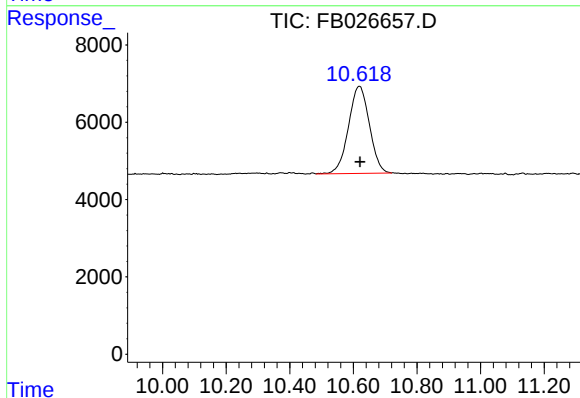


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.001 min
Response: 102894
Conc: 4.70 ng/ml

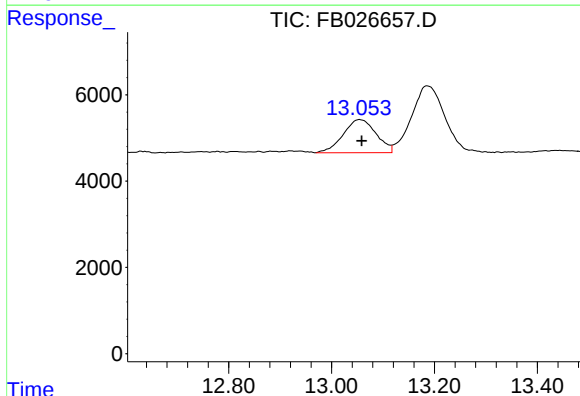


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 34158
Conc: 1.70 ng/ml

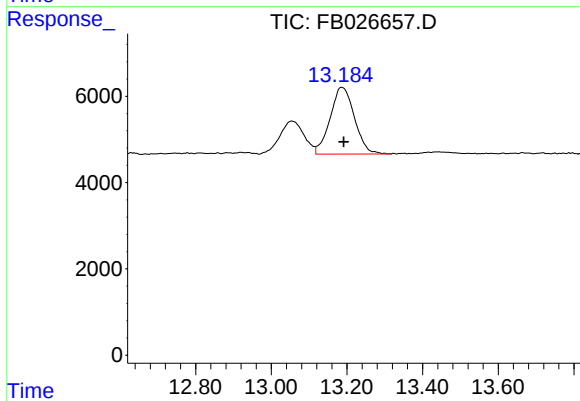


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: -0.006 min
Response: 69237
Conc: 3.44 ng/ml

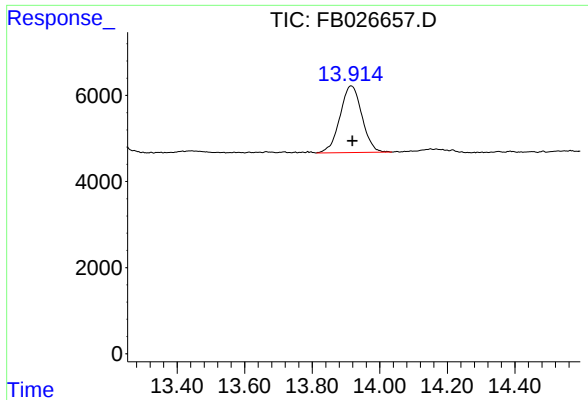

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 69792
Conc: 3.50 ng/ml

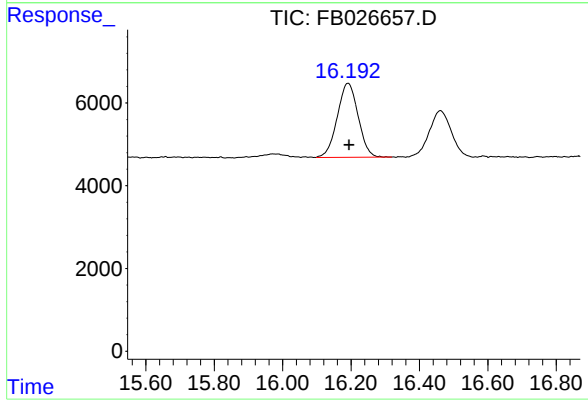

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.002 min
Response: 75733
Conc: 3.80 ng/ml