

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026661.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 16:17
 Operator : AJ/MA
 Sample : BSF0309W1
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:00:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	203748	19.417 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	545897	28.832 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	581460	28.053 ng/ml
3) t n-Heptane	7.750	195181	9.861 ng/ml
4) t Benzene	7.886	227349	9.853 ng/ml
6) t Toluene	10.619	641555	29.304 ng/ml
7) t Ethylbenzene	13.056	194906	9.698 ng/ml
8) t m-Xylene	13.188	383981	19.054 ng/ml
9) t O-Xylene	13.916	375611	18.828 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	368875	18.514 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026661.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 16:17
Operator : AJ/MA
Sample : BSF0309W1
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:00:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

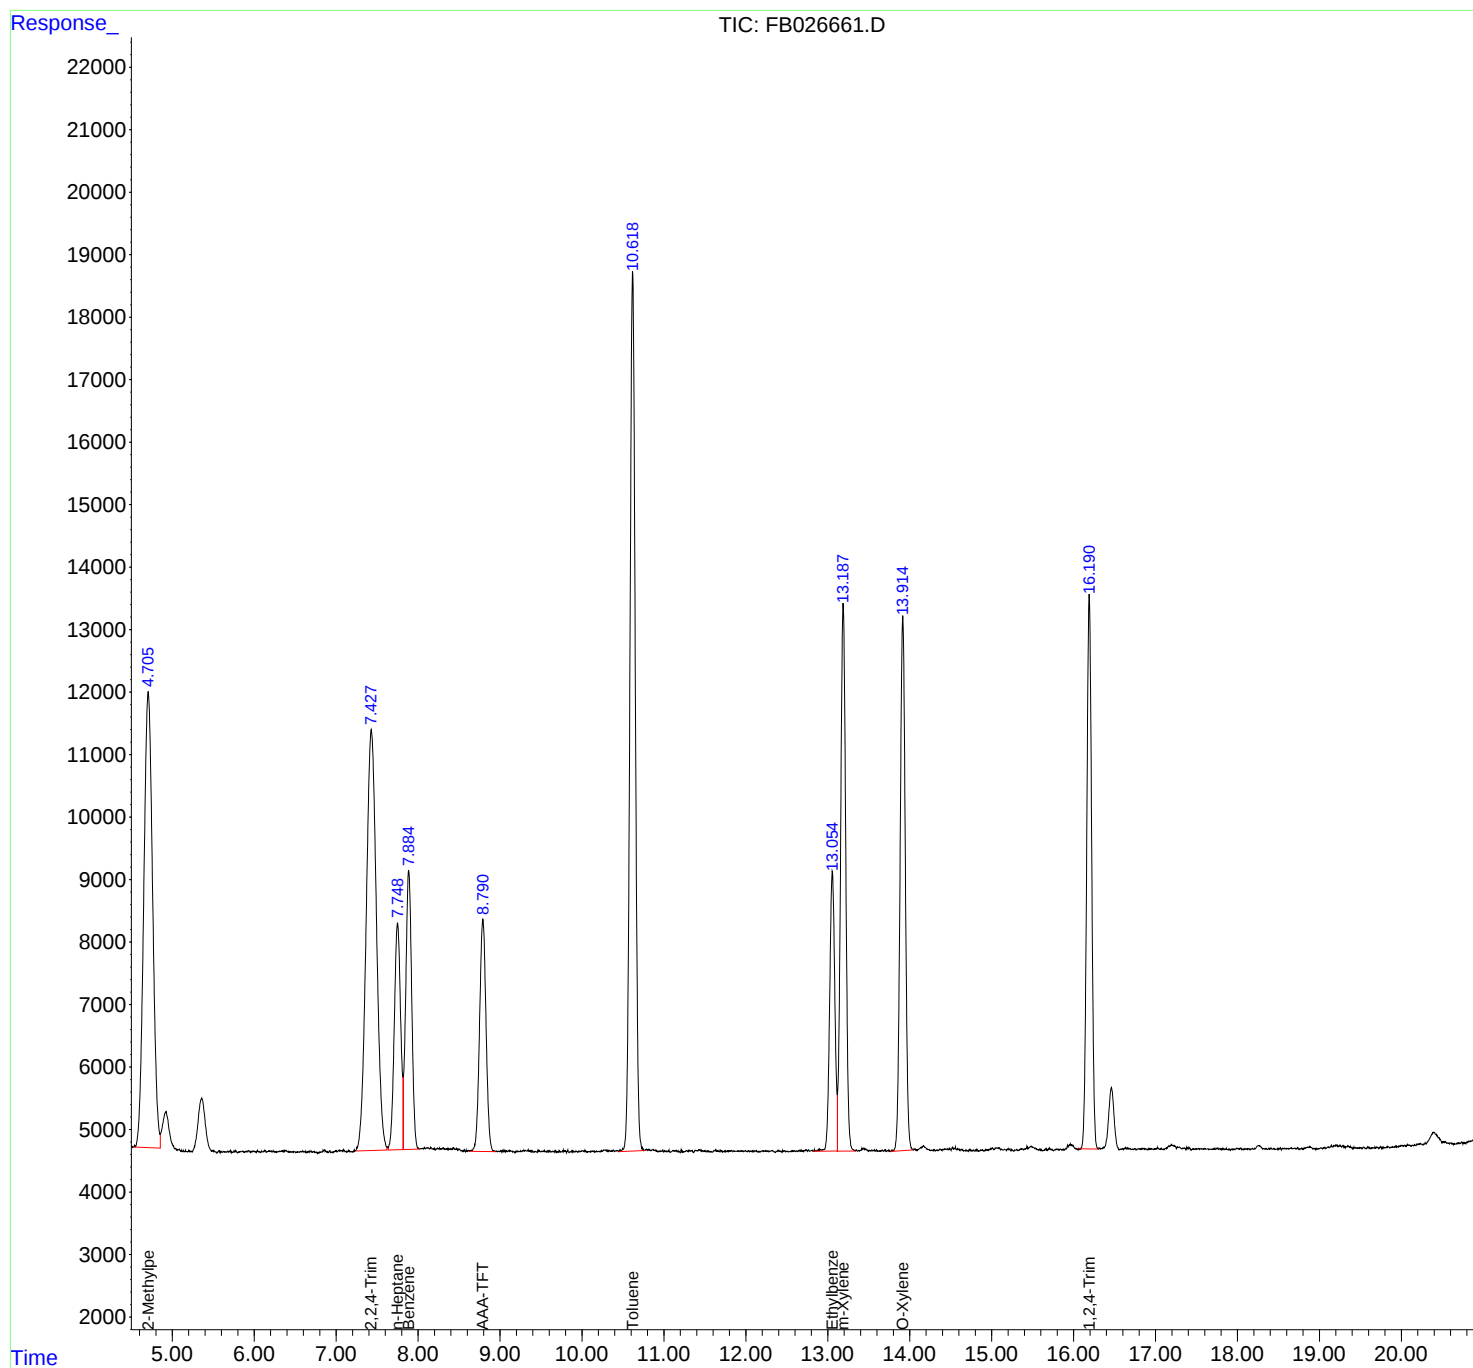

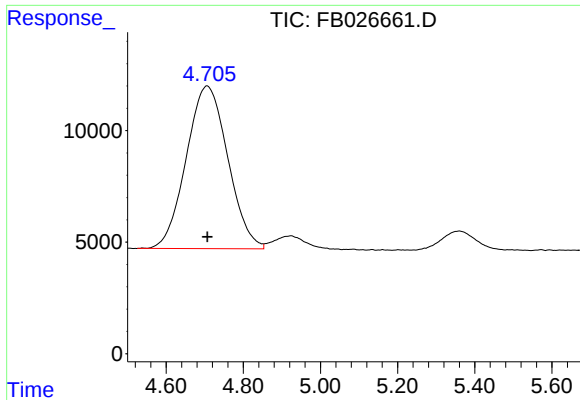


#1 2-Methylpentane

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 545897
Conc: 28.83 ng/ml

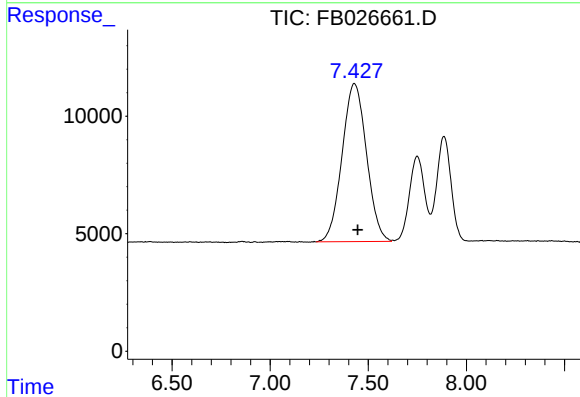


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.018 min
Response: 581460
Conc: 28.05 ng/ml

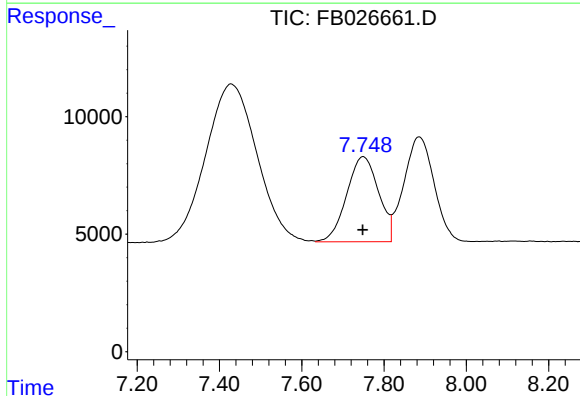


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 195181
Conc: 9.86 ng/ml

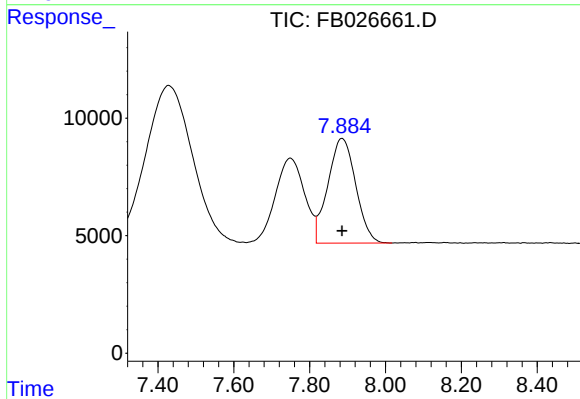


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 227349
Conc: 9.85 ng/ml

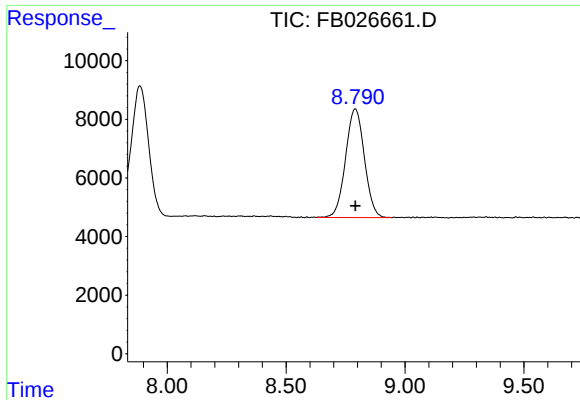


#5 AAA-TFT

R.T.: 8.791 min
 Delta R.T.: 0.000 min
 Response: 203748
 Conc: 19.42 ng/ml

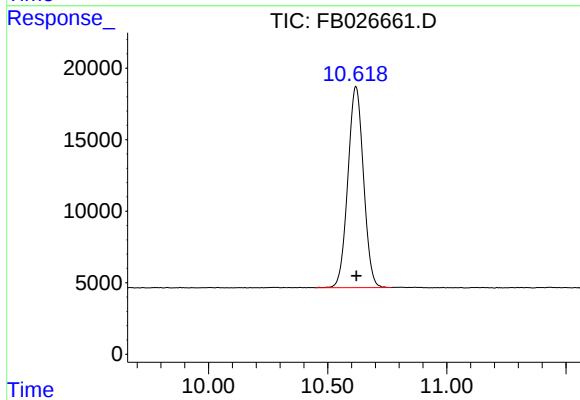


#6 Toluene

R.T.: 10.619 min
 Delta R.T.: -0.002 min
 Response: 641555
 Conc: 29.30 ng/ml

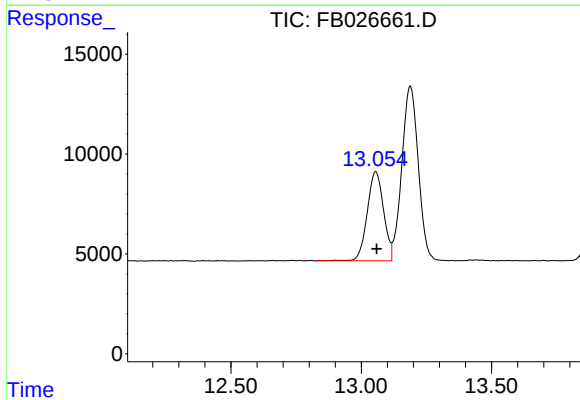


#7 Ethylbenzene

R.T.: 13.056 min
 Delta R.T.: -0.003 min
 Response: 194906
 Conc: 9.70 ng/ml

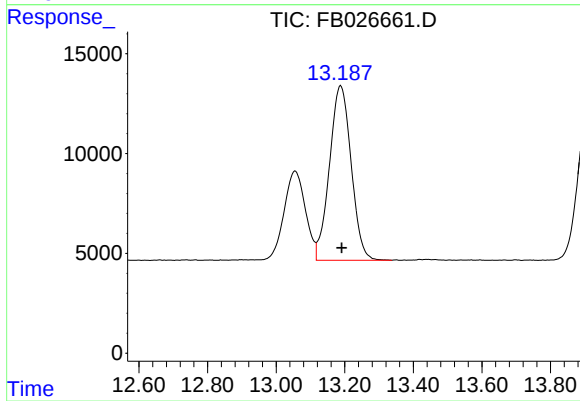


#8 m-Xylene

R.T.: 13.188 min
 Delta R.T.: -0.003 min
 Response: 383981
 Conc: 19.05 ng/ml

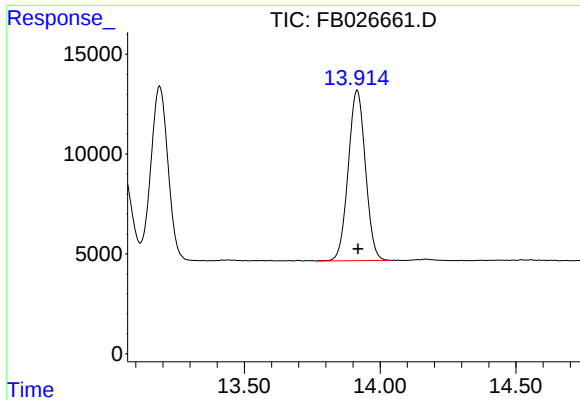

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 375611
Conc: 18.83 ng/ml

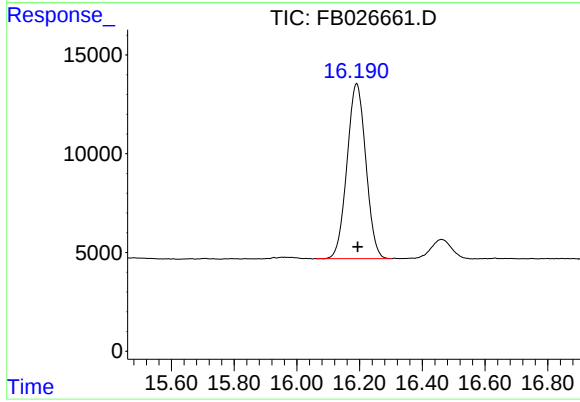

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.003 min
Response: 368875
Conc: 18.51 ng/ml