

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
 Data File : FB026663.D
 Signal(s) : FID2B.CH
 Acq On : 9 Mar 2022 17:34
 Operator : AJ/MA
 Sample : N1645-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 10 01:01:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.792	166702	15.886 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.720	24754	1.307 ng/ml
2) t	2,2,4-Trimethylpentane	7.435	24790	1.196 ng/mlm
3) t	n-Heptane	7.751	8452	0.427 ng/ml
4) t	Benzene	7.883	10296	0.446 ng/ml
6) t	Toluene	10.623	29100	1.329 ng/ml
7) t	Ethylbenzene	13.055	8356	0.416 ng/ml
8) t	m-Xylene	13.189	17956	0.891 ng/ml
9) t	O-Xylene	13.919	18626	0.934 ng/ml
10) t	1,2,4-Trimethylbenzene	16.191	18916	0.949 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030922\
Data File : FB026663.D
Signal(s) : FID2B.CH
Acq On : 9 Mar 2022 17:34
Operator : AJ/MA
Sample : N1645-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 10 01:01:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

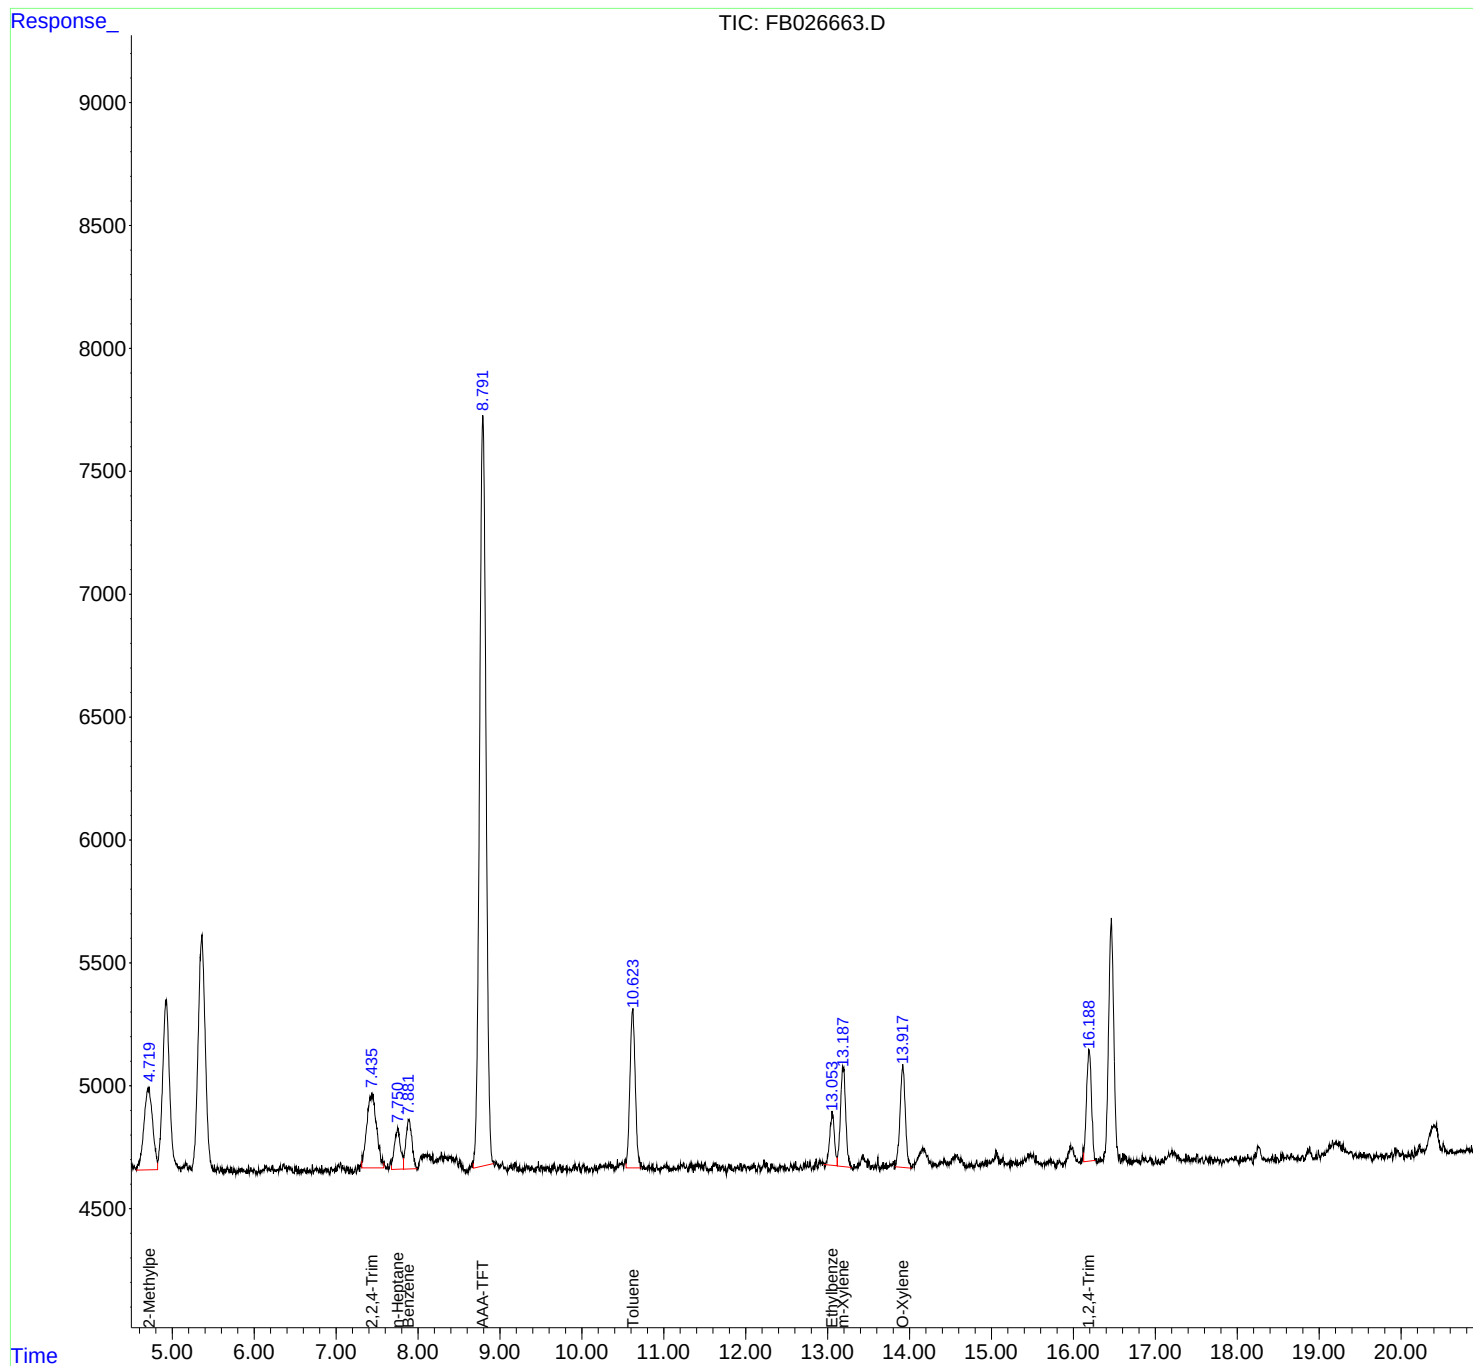

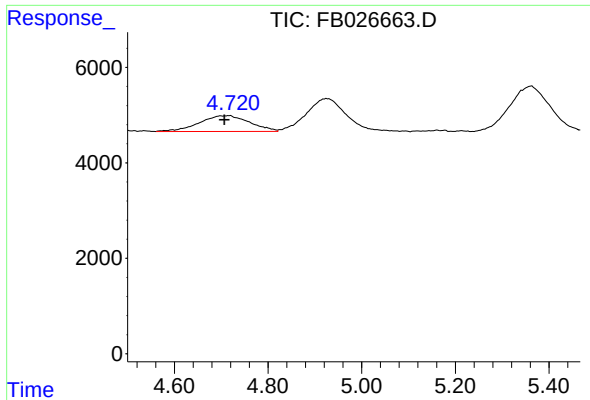


#1 2-Methylpentane

R.T.: 4.720 min
Delta R.T.: 0.013 min
Response: 24754
Conc: 1.31 ng/ml

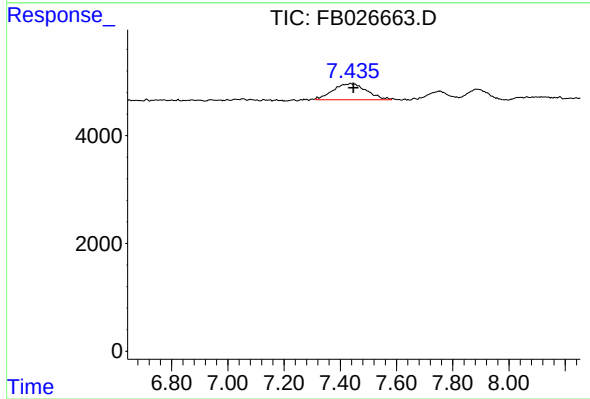


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: -0.012 min
Response: 24790
Conc: 1.20 ng/ml m

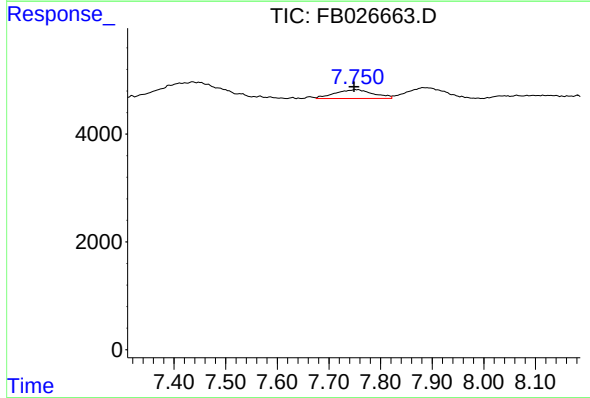


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.003 min
Response: 8452
Conc: 0.43 ng/ml

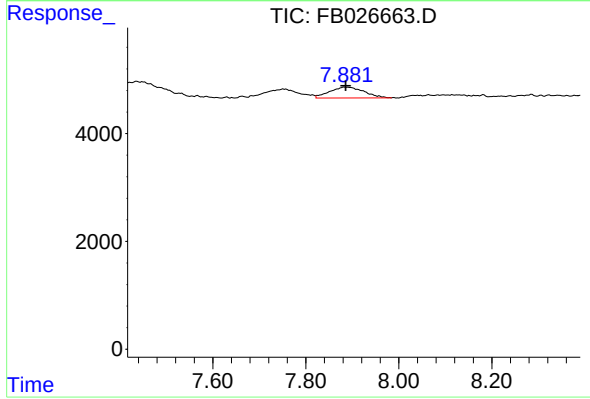


#4 Benzene

R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 10296
Conc: 0.45 ng/ml

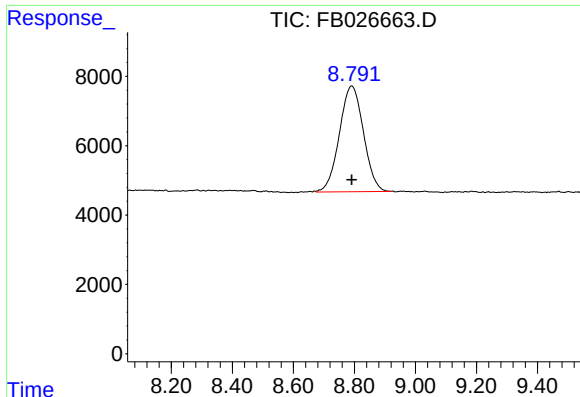


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 166702
Conc: 15.89 ng/ml

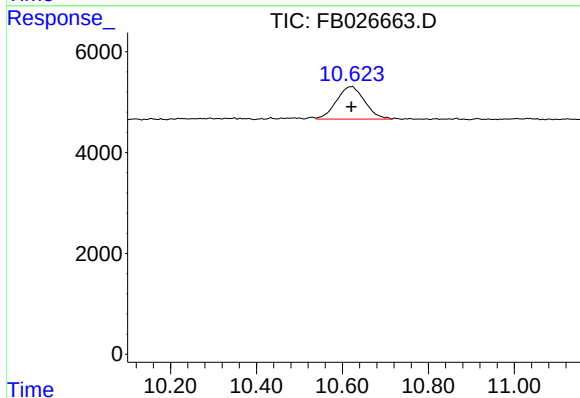


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.002 min
Response: 29100
Conc: 1.33 ng/ml

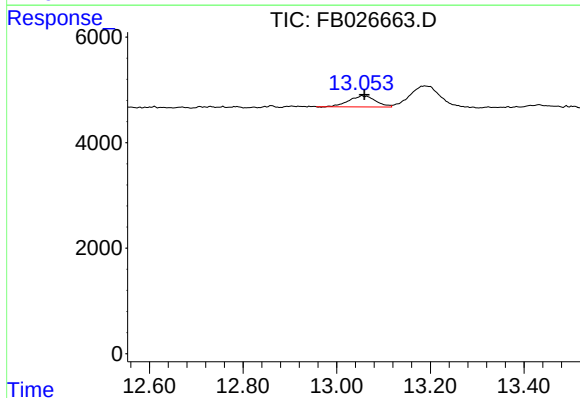


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 8356
Conc: 0.42 ng/ml

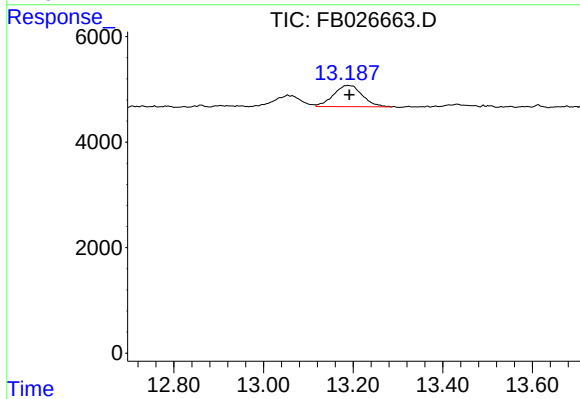


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.002 min
Response: 17956
Conc: 0.89 ng/ml

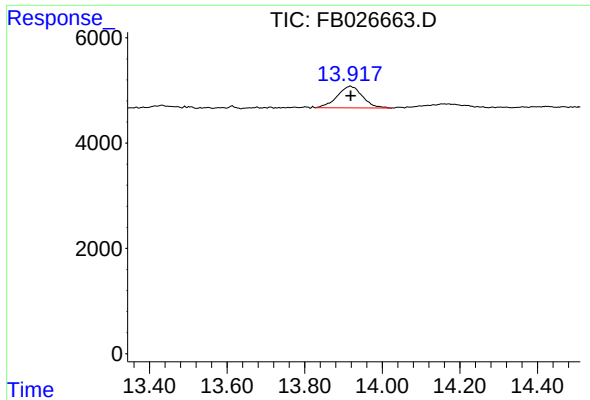

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.000 min
Response: 18626
Conc: 0.93 ng/ml

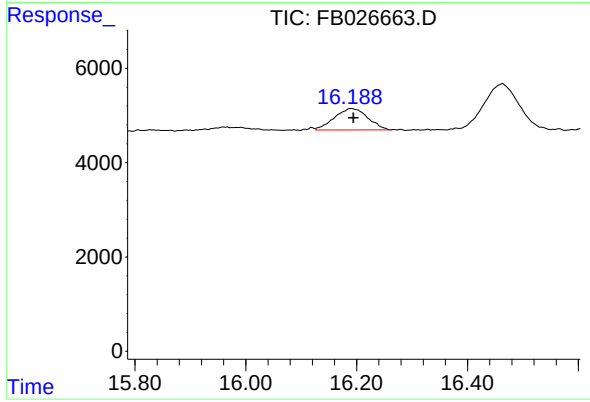

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.004 min
Response: 18916
Conc: 0.95 ng/ml