

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031020\
Data File : FB023850.D
Signal(s) : FID2B.CH
Acq On : 11 Mar 2020 2:41
Operator : DD/AJ
Sample : L1871-02
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 04:44:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.801	334089	15.871 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.678	991	0.032 ng/ml
2) t	2,2,4-Trimethylpentane	7.385	417	0.012 ng/ml
6) t	Toluene	10.636	1710	0.042 ng/ml
7) t	Ethylbenzene	13.135	1196	0.031 ng/ml
8) t	m-Xylene	13.135	1196	0.032 ng/ml
9) t	O-Xylene	13.939	465	0.013 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031020\
Data File : FB023850.D
Signal(s) : FID2B.CH
Acq On : 11 Mar 2020 2:41
Operator : DD/AJ
Sample : L1871-02
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 04:44:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

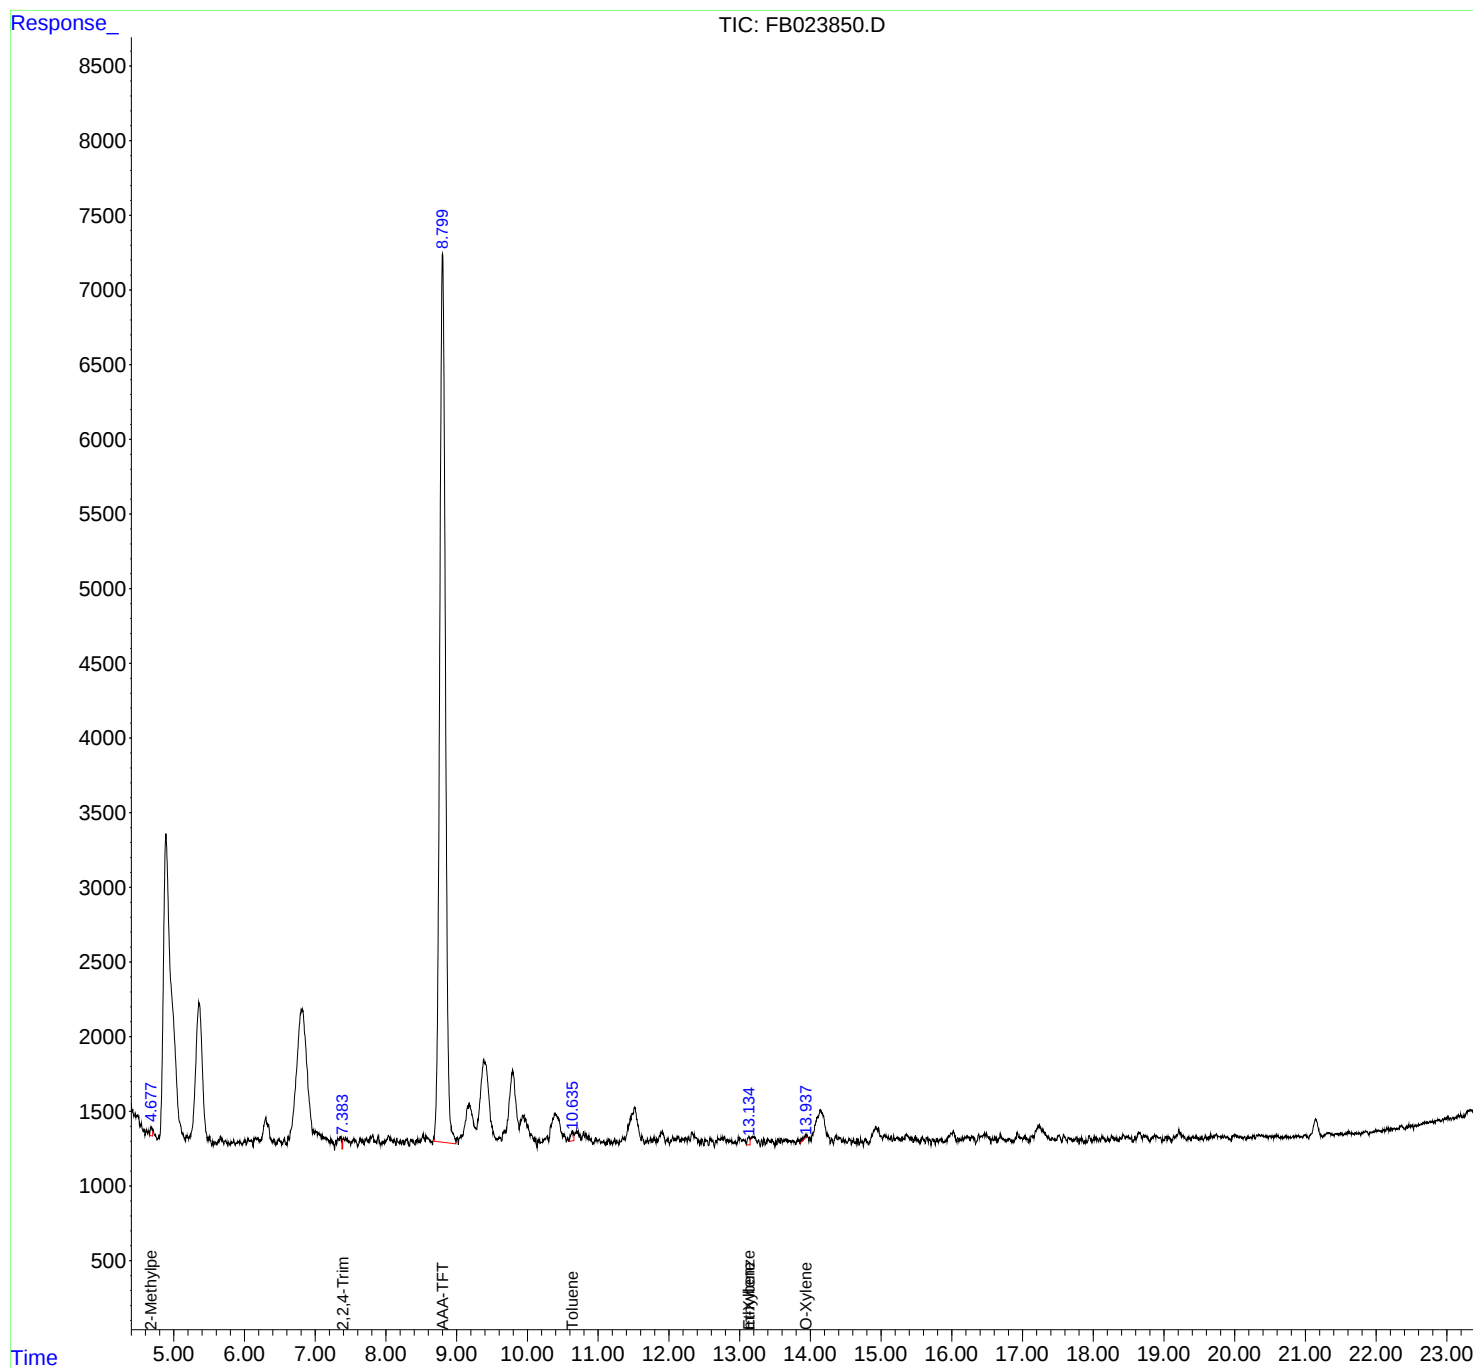

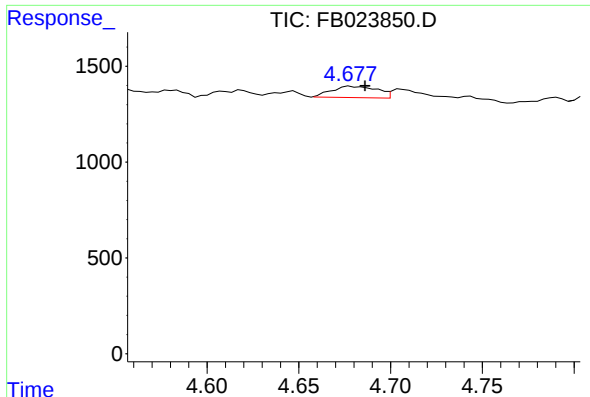


#1 2-Methylpentane

R.T.: 4.678 min
Delta R.T.: -0.008 min
Response: 991
Conc: 0.03 ng/ml

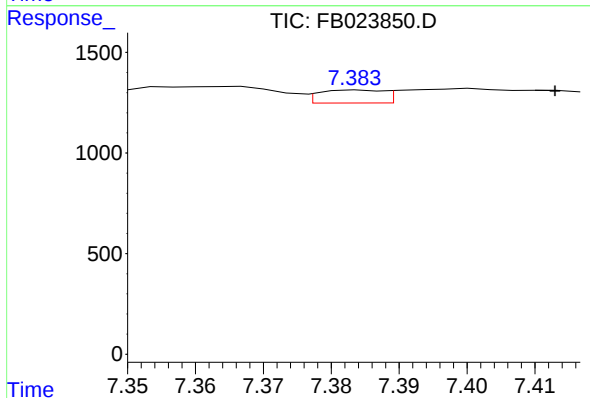


#2 2,2,4-Trimethylpentane

R.T.: 7.385 min
Delta R.T.: -0.028 min
Response: 417
Conc: 0.01 ng/ml

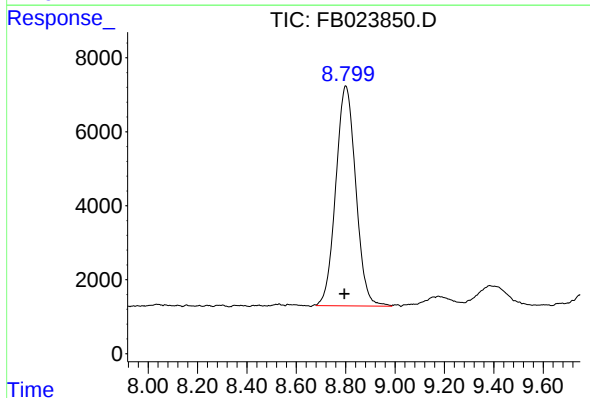


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.006 min
Response: 334089
Conc: 15.87 ng/ml

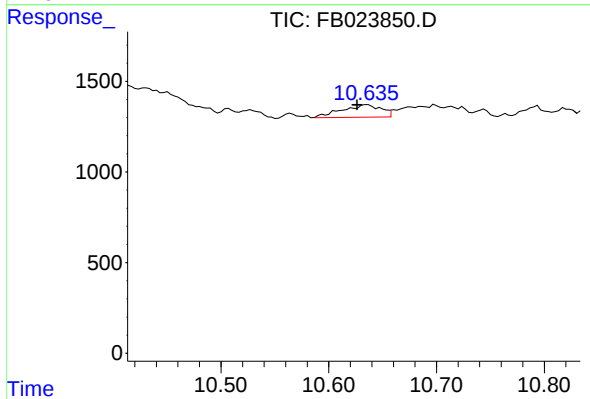


#6 Toluene

R.T.: 10.636 min
Delta R.T.: 0.010 min
Response: 1710
Conc: 0.04 ng/ml

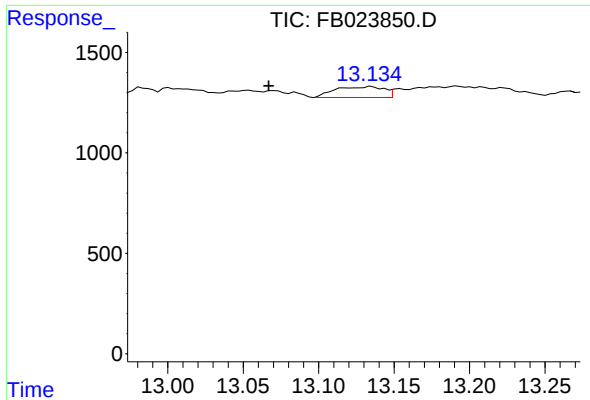


#7 Ethylbenzene

R.T.: 13.135 min
Delta R.T.: 0.068 min
Response: 1196
Conc: 0.03 ng/ml

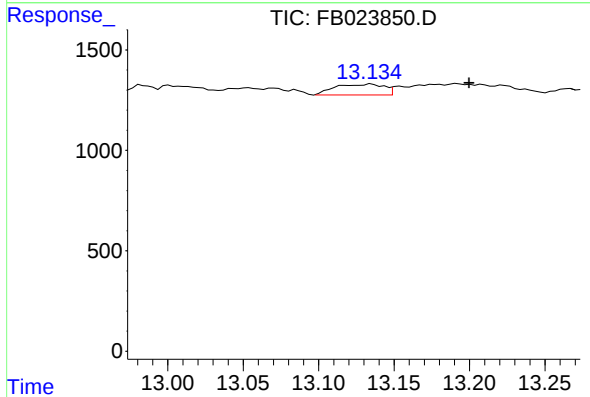

#8 m-Xylene

R.T.: 13.135 min
Delta R.T.: -0.065 min
Response: 1196
Conc: 0.03 ng/ml

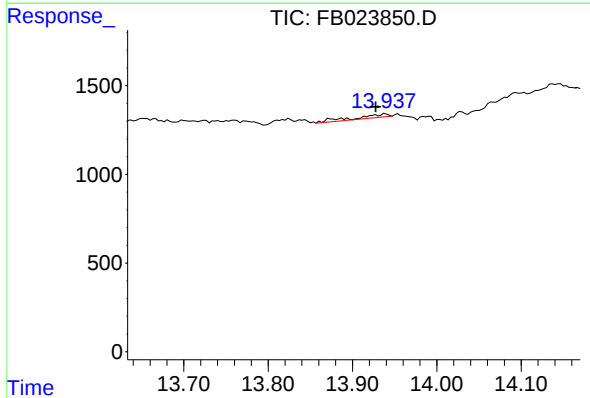

#9 O-Xylene

R.T.: 13.939 min
Delta R.T.: 0.012 min
Response: 465
Conc: 0.01 ng/ml