

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
Data File : FB026671.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2022 12:13
Operator : AJ/MA
Sample : N1831-01
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 00:38:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	166447	15.862 ng/ml
Target Compounds			
6) t Toluene	10.618	8080	0.369 ng/ml
8) t m-Xylene	13.189	8776	0.435 ng/ml
9) t O-Xylene	13.921	7753	0.389 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	47053	2.362 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
Data File : FB026671.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2022 12:13
Operator : AJ/MA
Sample : N1831-01
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 00:38:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

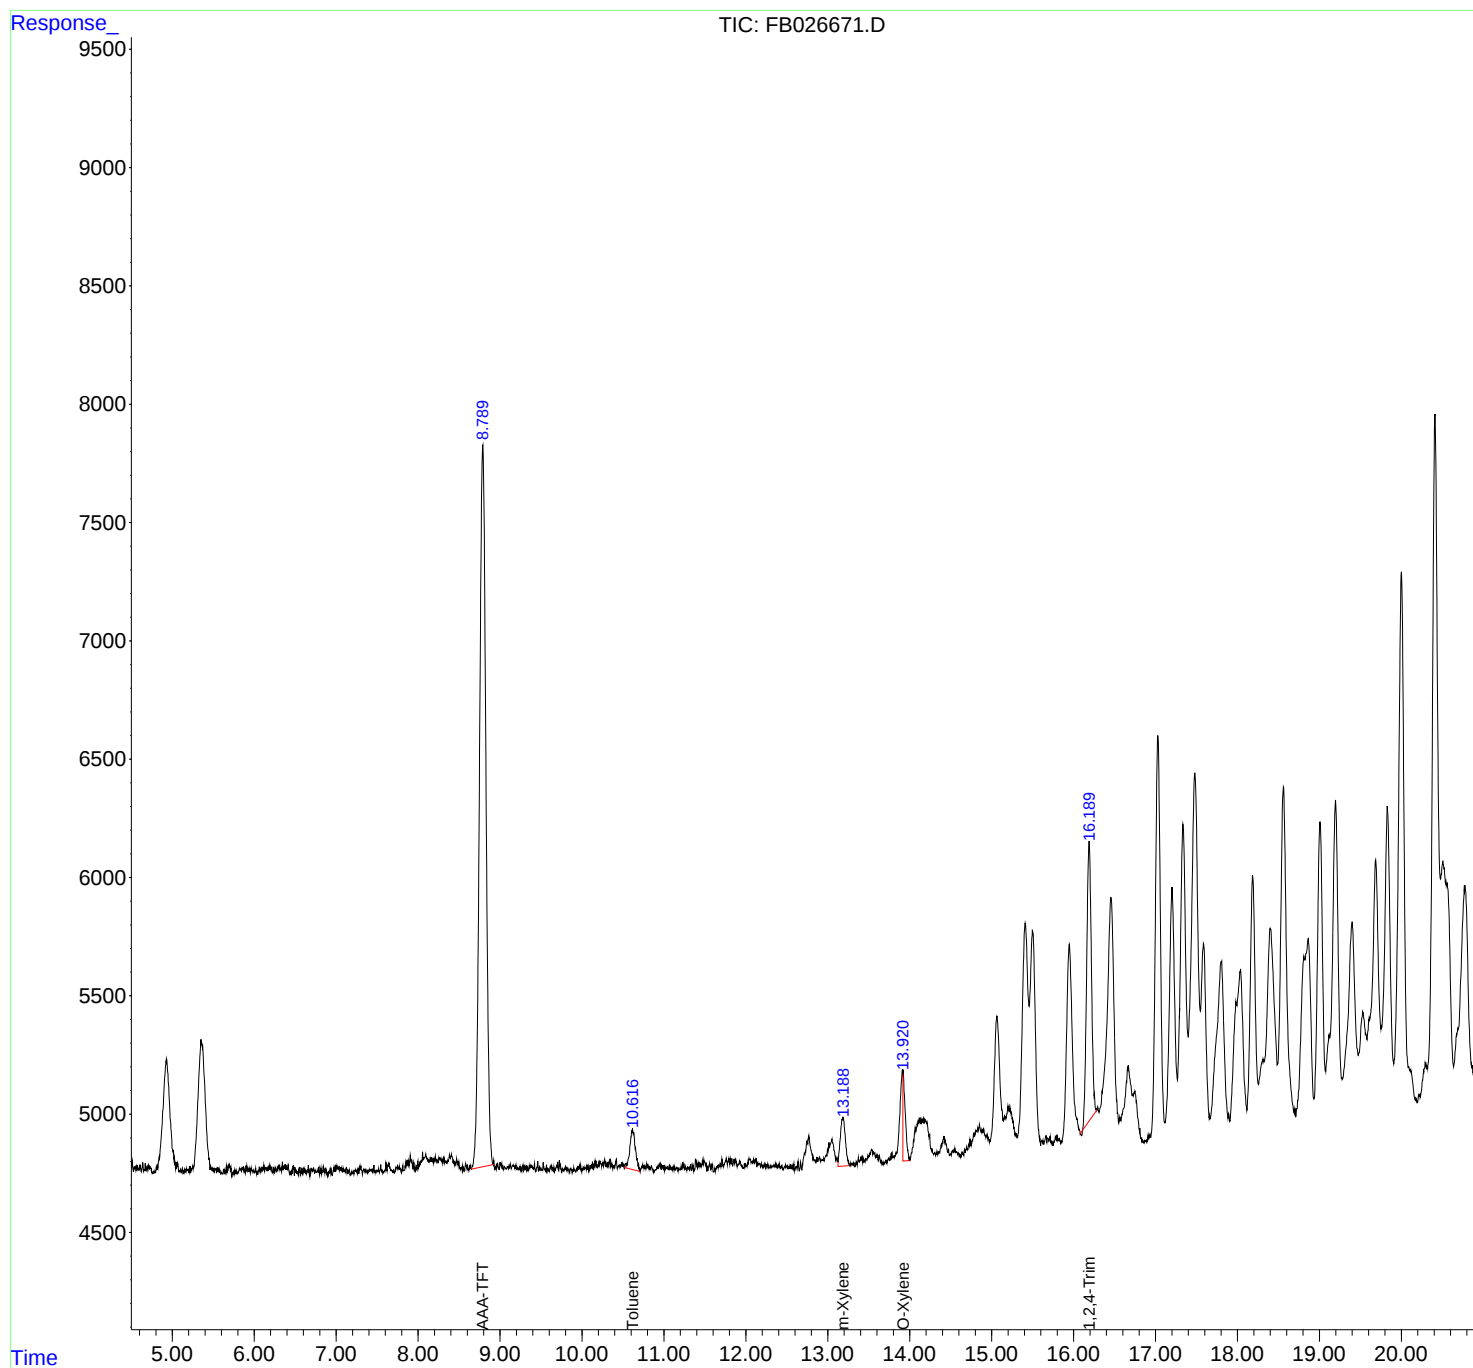

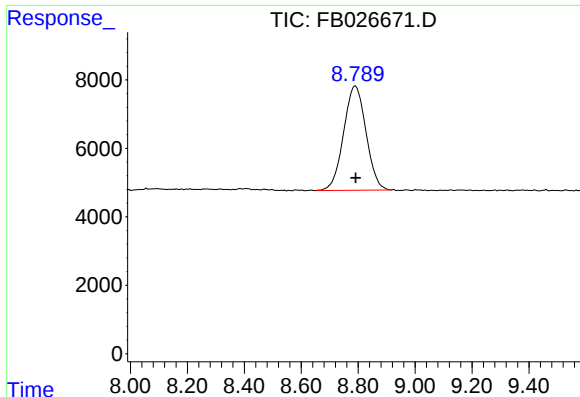


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 166447
Conc: 15.86 ng/ml

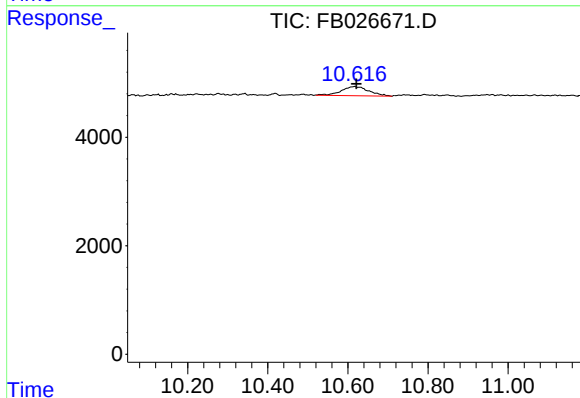


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 8080
Conc: 0.37 ng/ml

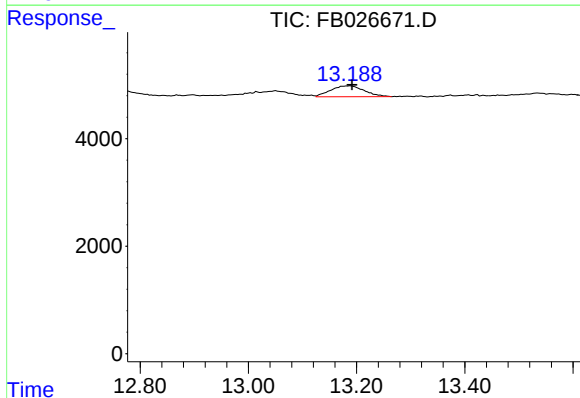


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: -0.002 min
Response: 8776
Conc: 0.44 ng/ml

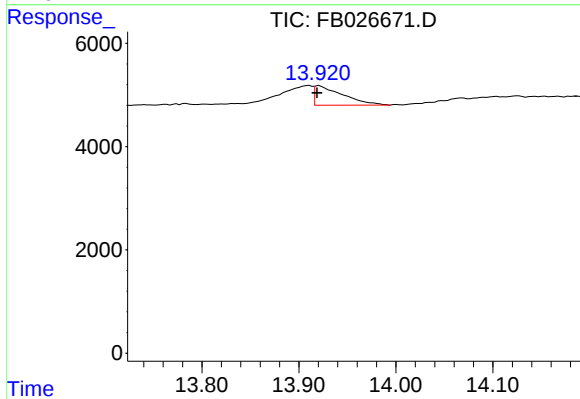

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.002 min
Response: 7753
Conc: 0.39 ng/ml

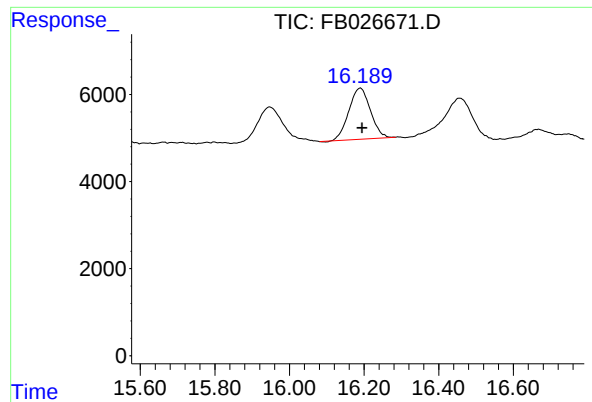

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.004 min
Response: 47053
Conc: 2.36 ng/ml