

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
 Data File : FB026672.D
 Signal(s) : FID2B.CH
 Acq On : 10 Mar 2022 12:51
 Operator : AJ/MA
 Sample : N1831-01MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 11 00:38:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	191803	18.278 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	368989	19.489 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	264963	12.783 ng/ml
3) t n-Heptane	7.747	92329	4.665 ng/ml
4) t Benzene	7.884	206446	8.947 ng/ml
6) t Toluene	10.617	541550	24.736 ng/ml
7) t Ethylbenzene	13.054	154693	7.697 ng/ml
8) t m-Xylene	13.187	284544	14.119 ng/ml
9) t O-Xylene	13.914	299882	15.032 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	250979	12.597 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
Data File : FB026672.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2022 12:51
Operator : AJ/MA
Sample : N1831-01MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 00:38:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

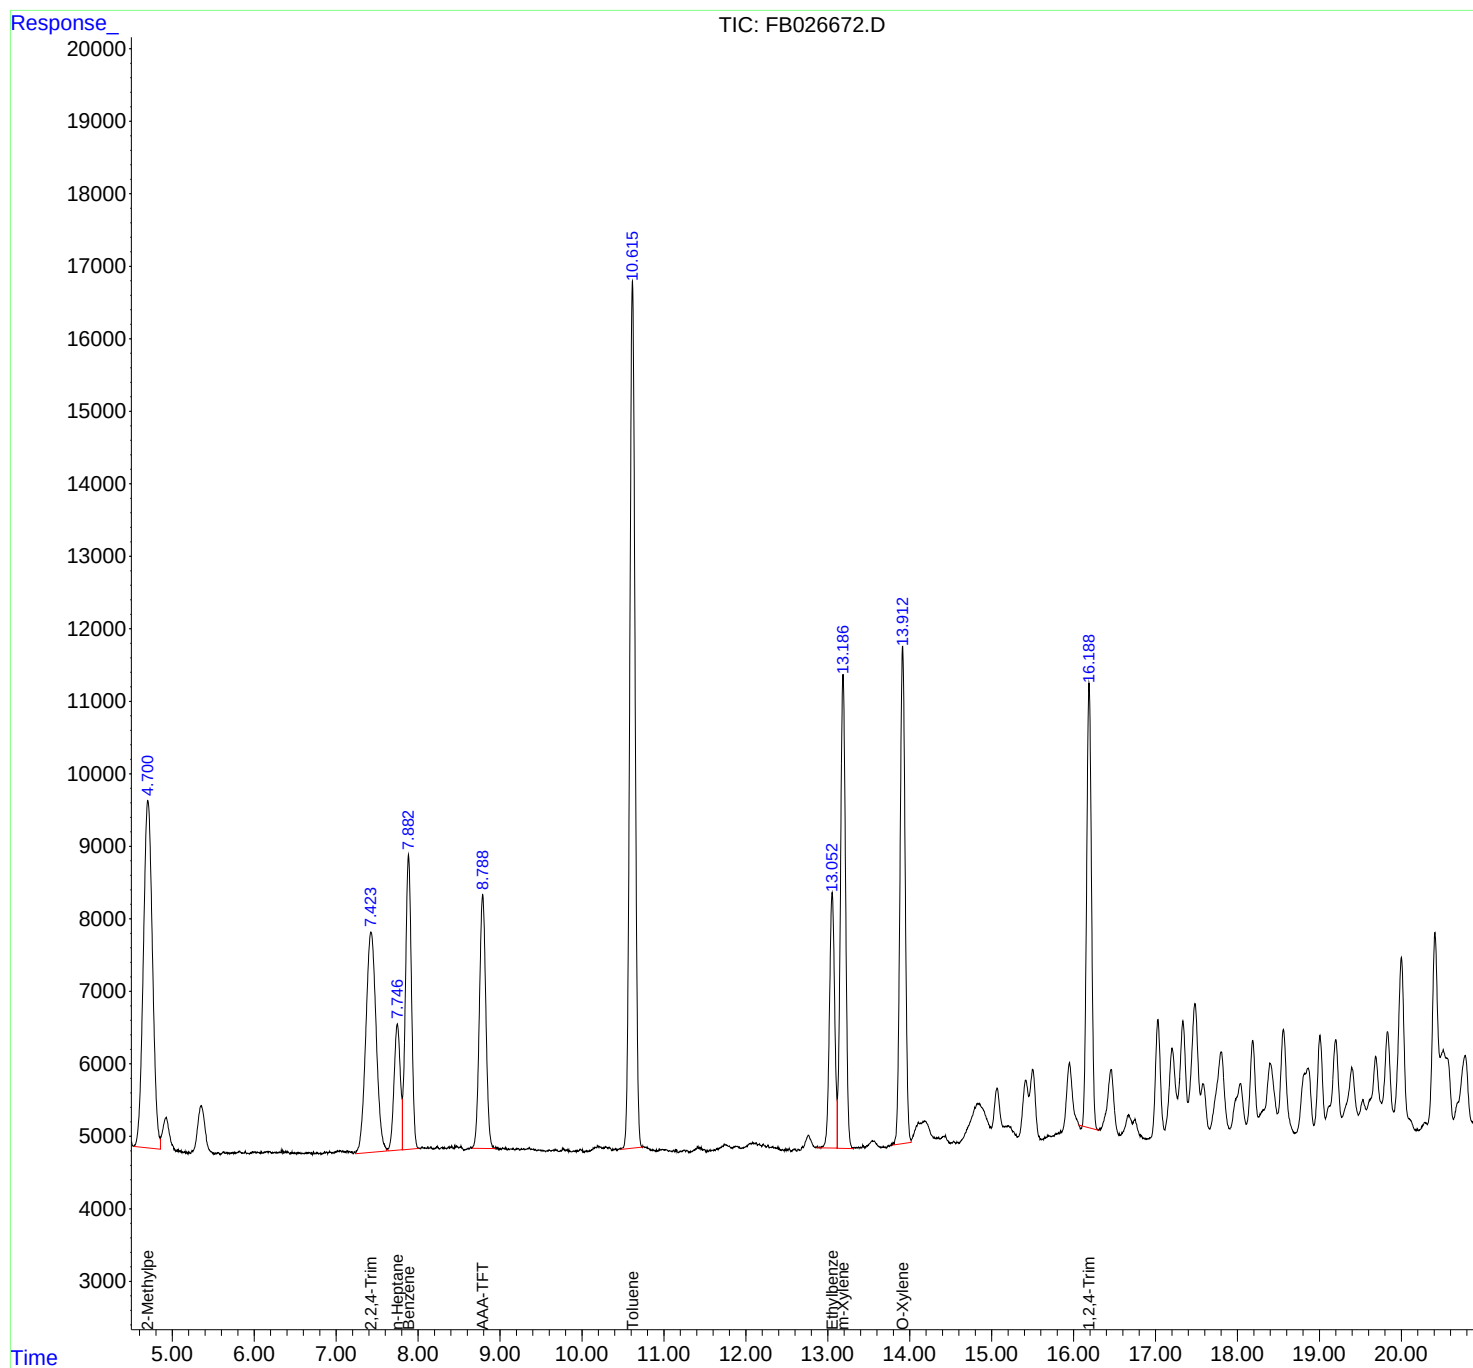

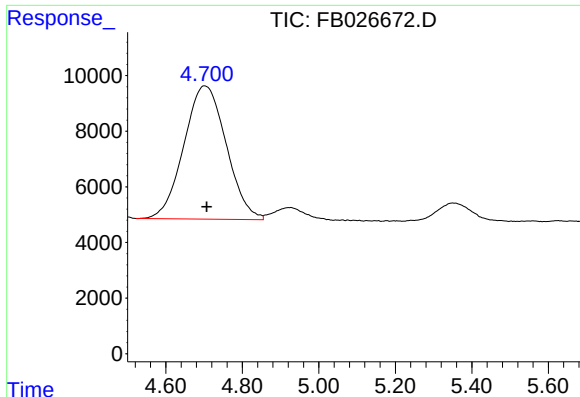


#1 2-Methylpentane

R.T.: 4.702 min
Delta R.T.: -0.005 min
Response: 368989
Conc: 19.49 ng/ml

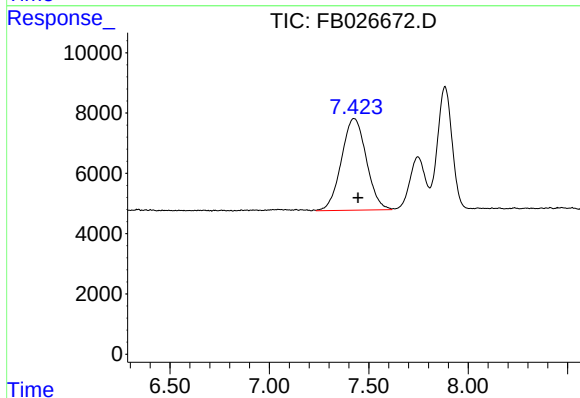


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.023 min
Response: 264963
Conc: 12.78 ng/ml

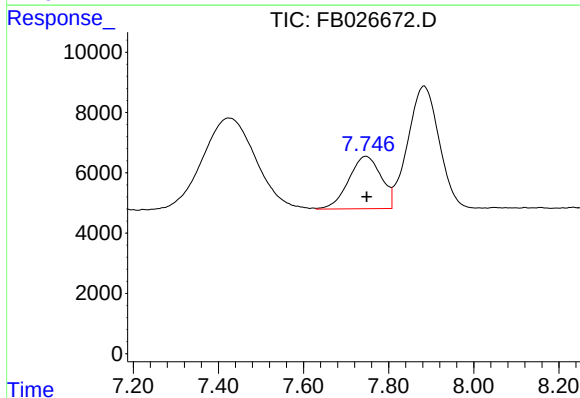


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.001 min
Response: 92329
Conc: 4.66 ng/ml

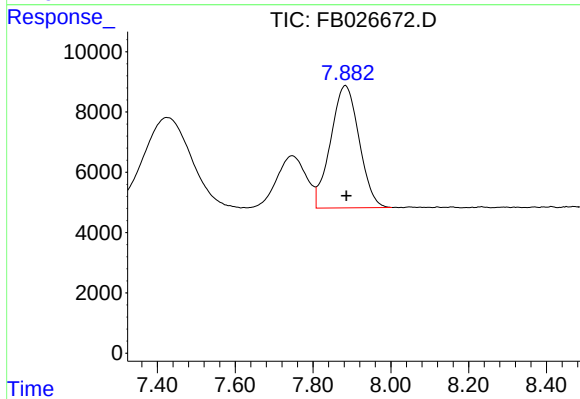


#4 Benzene

R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 206446
Conc: 8.95 ng/ml

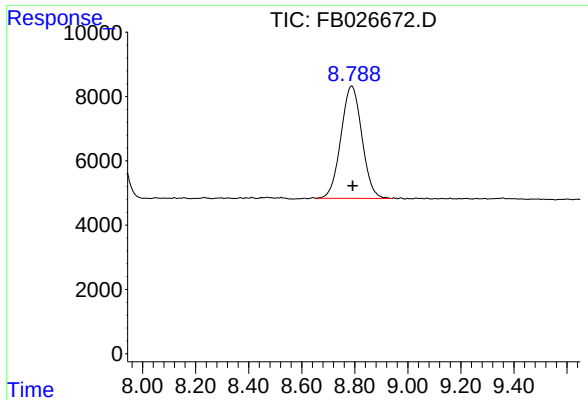


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 191803
Conc: 18.28 ng/ml

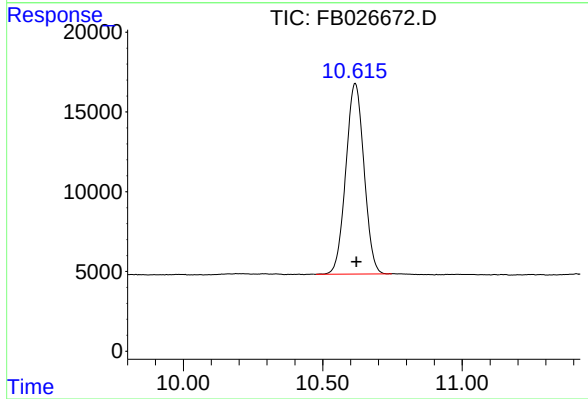


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 541550
Conc: 24.74 ng/ml

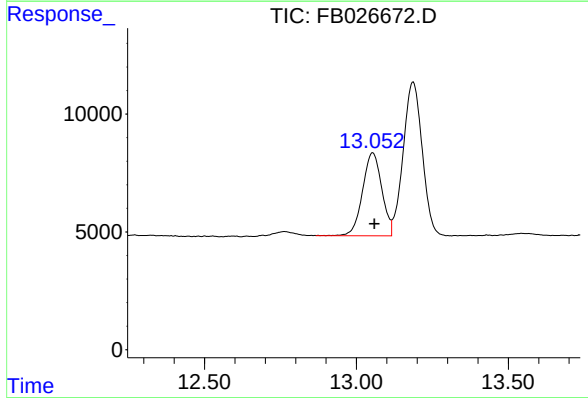


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 154693
Conc: 7.70 ng/ml

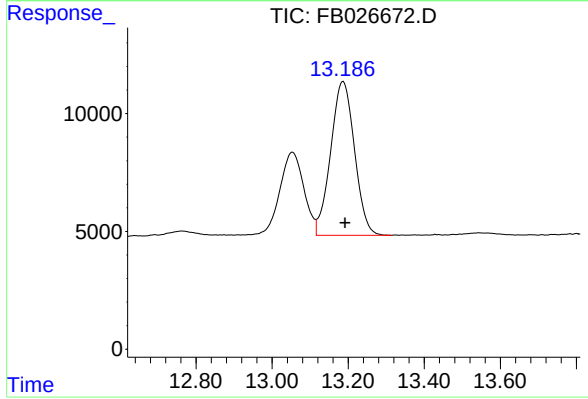

#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 284544
Conc: 14.12 ng/ml

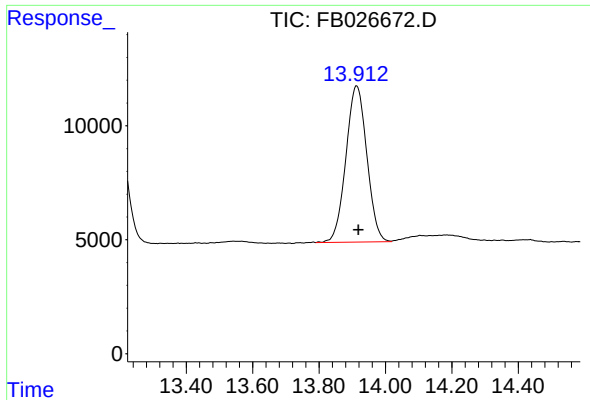


#9 O-Xylene

R.T.: 13.914 min

Delta R.T.: -0.005 min

Response: 299882

Conc: 15.03 ng/ml

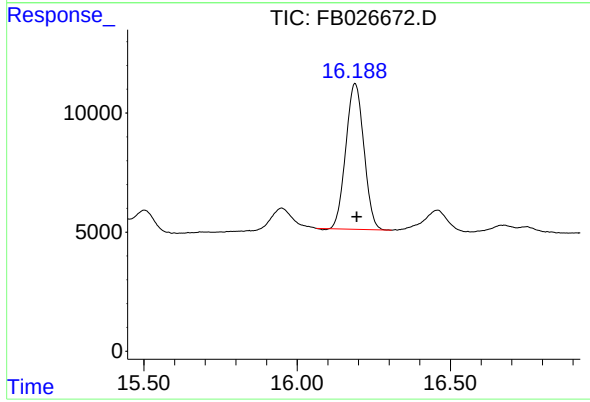

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min

Delta R.T.: -0.005 min

Response: 250979

Conc: 12.60 ng/ml