

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
 Data File : FB026673.D
 Signal(s) : FID2B.CH
 Acq On : 10 Mar 2022 14:31
 Operator : AJ/MA
 Sample : N1831-01MSD
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 11 00:38:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	180165	17.169 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	387074	20.444 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	309804	14.947 ng/ml
3) t n-Heptane	7.747	108074	5.460 ng/ml
4) t Benzene	7.883	185150	8.024 ng/ml
6) t Toluene	10.616	480606	21.953 ng/ml
7) t Ethylbenzene	13.052	140599	6.996 ng/ml
8) t m-Xylene	13.185	246632	12.238 ng/ml
9) t O-Xylene	13.912	260673	13.066 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	200937	10.085 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
Data File : FB026673.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2022 14:31
Operator : AJ/MA
Sample : N1831-01MSD
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 00:38:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

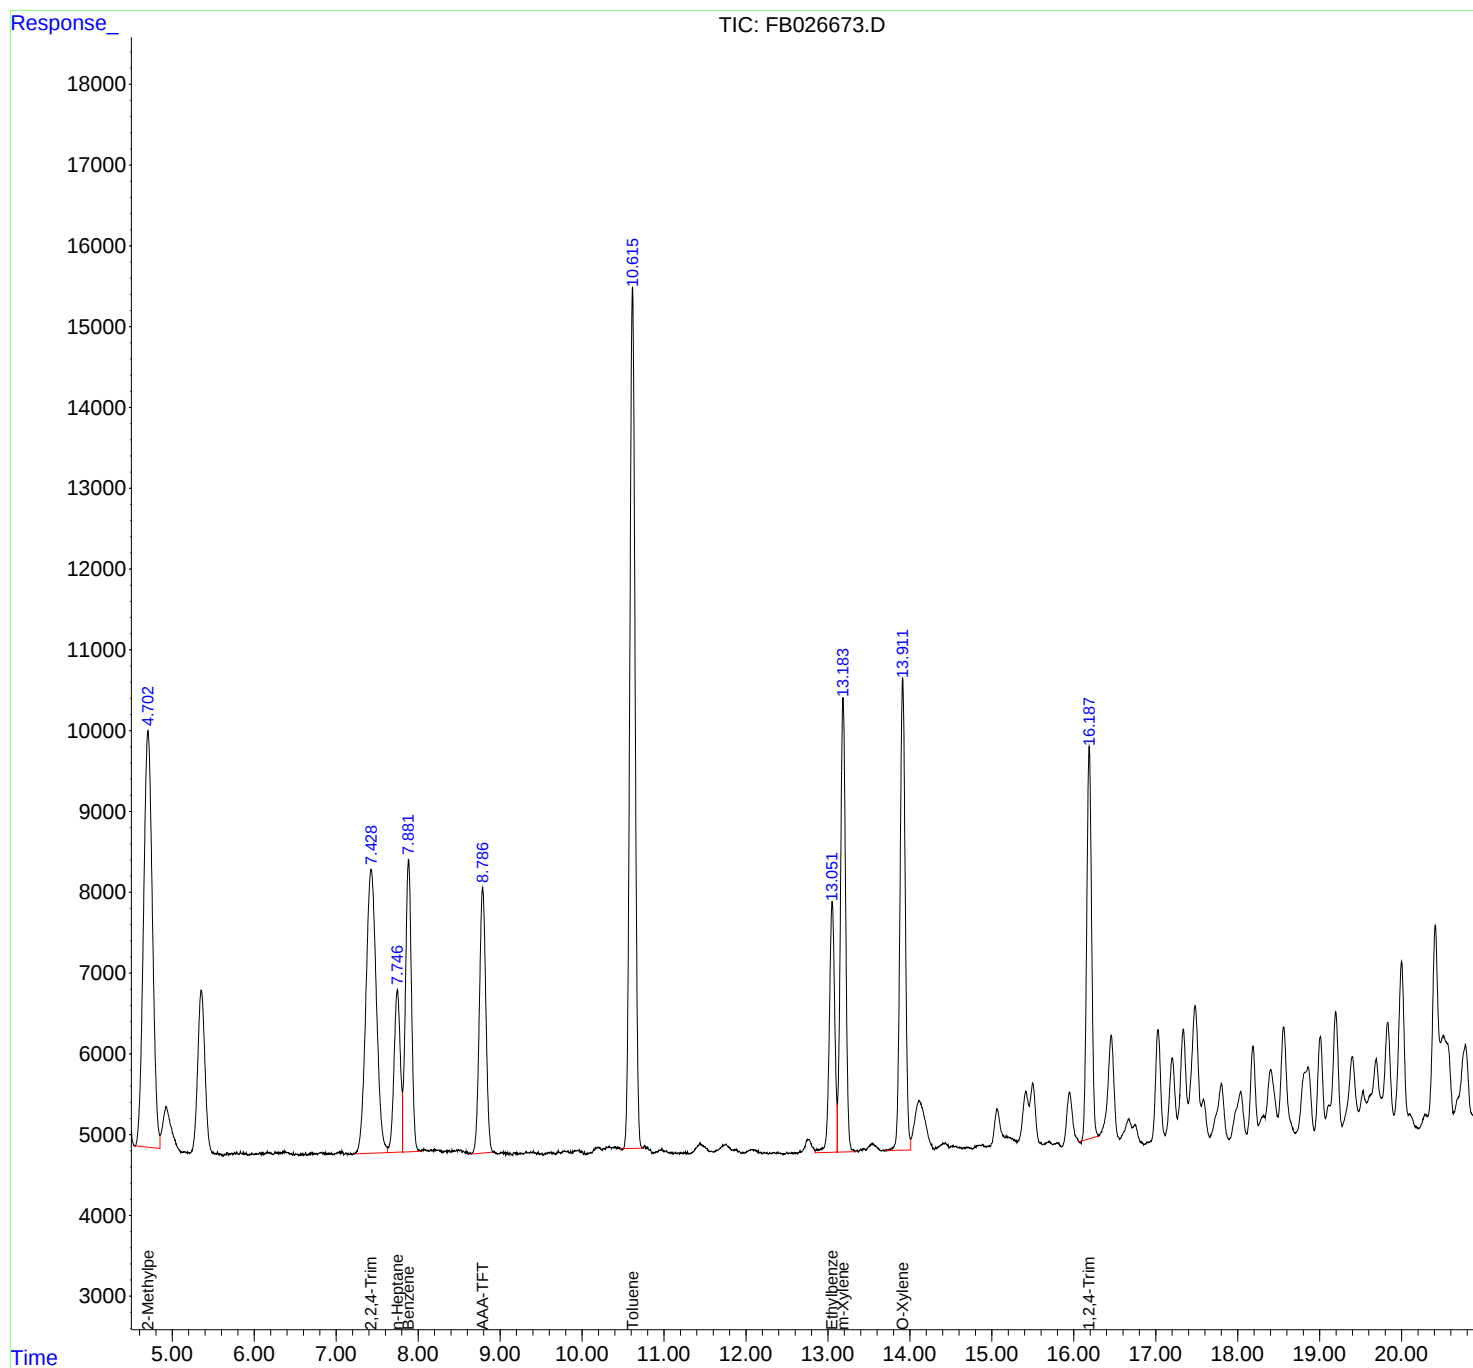

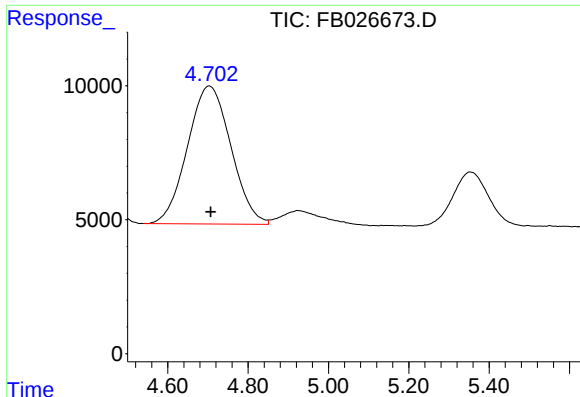


#1 2-Methylpentane

R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 387074
Conc: 20.44 ng/ml

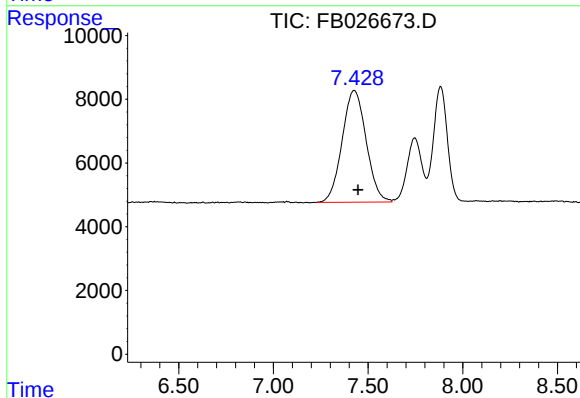


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.021 min
Response: 309804
Conc: 14.95 ng/ml

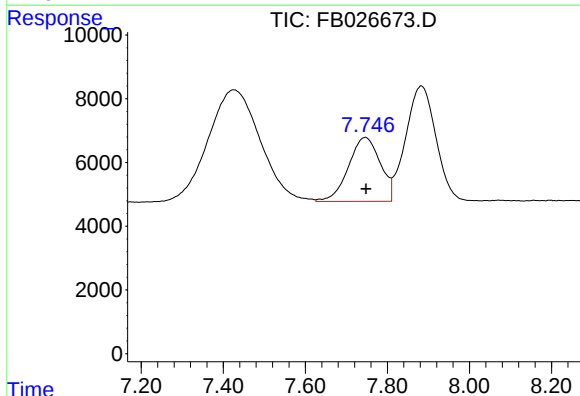


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.001 min
Response: 108074
Conc: 5.46 ng/ml

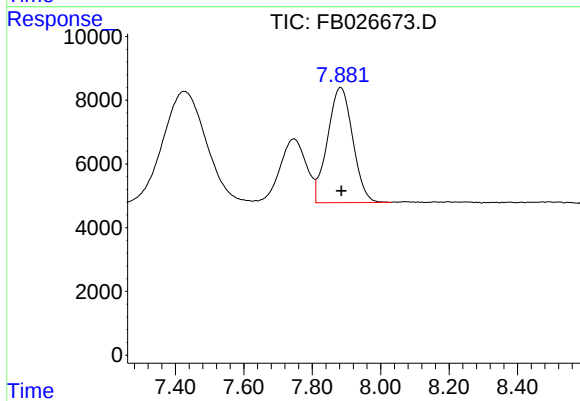


#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 185150
Conc: 8.02 ng/ml

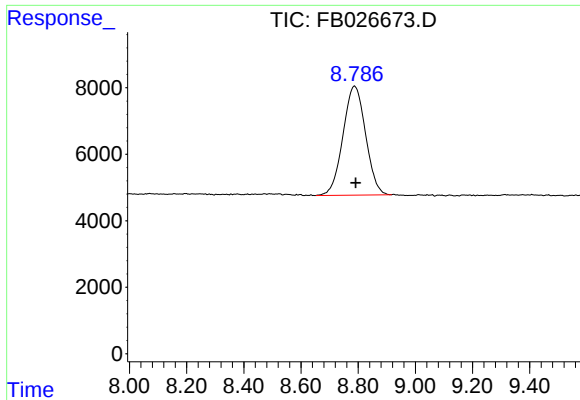


#5 AAA-TFT
 R.T.: 8.787 min
 Delta R.T.: -0.004 min
 Response: 180165
 Conc: 17.17 ng/ml

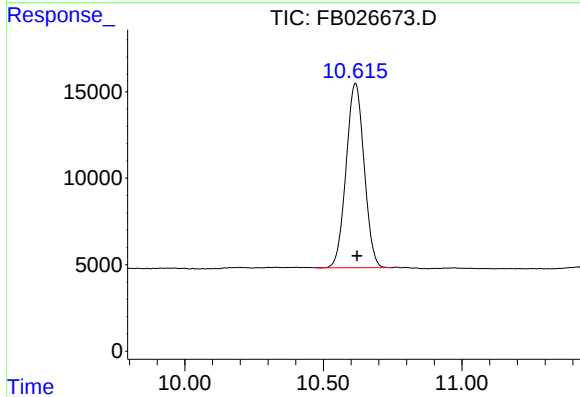


#6 Toluene
 R.T.: 10.616 min
 Delta R.T.: -0.005 min
 Response: 480606
 Conc: 21.95 ng/ml

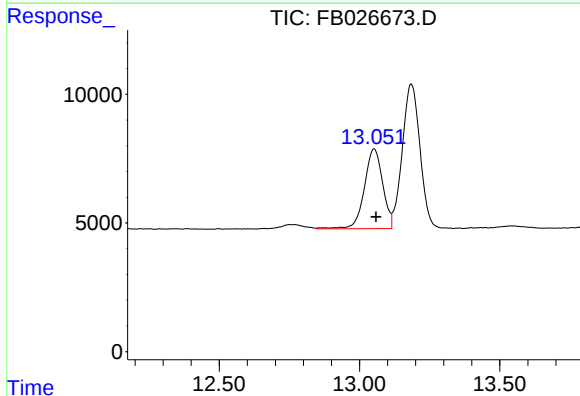

#7 Ethylbenzene
 R.T.: 13.052 min
 Delta R.T.: -0.006 min
 Response: 140599
 Conc: 7.00 ng/ml

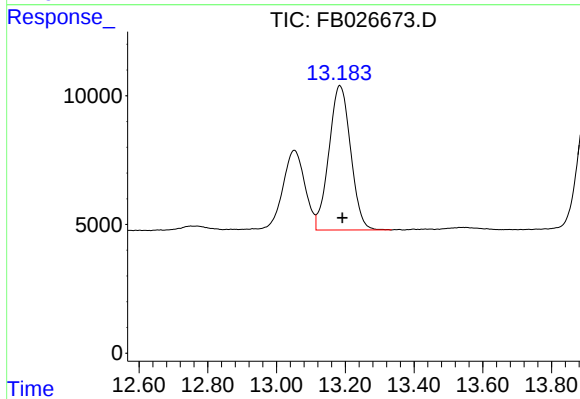


#8 m-Xylene
 R.T.: 13.185 min
 Delta R.T.: -0.007 min
 Response: 246632
 Conc: 12.24 ng/ml

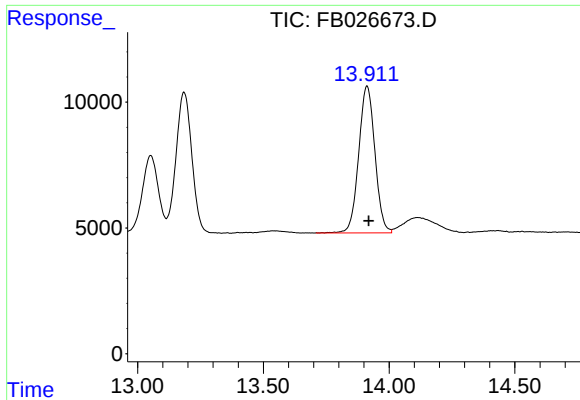

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.006 min
Response: 260673
Conc: 13.07 ng/ml

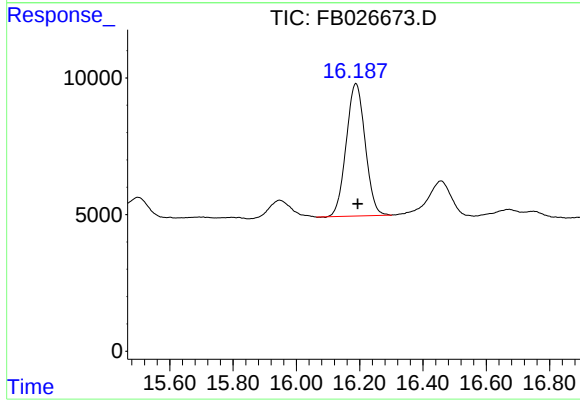

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.006 min
Response: 200937
Conc: 10.08 ng/ml