

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
 Data File : FB026679.D
 Signal(s) : FID2B.CH
 Acq On : 10 Mar 2022 19:03
 Operator : AJ/MA
 Sample : N1645-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 11 00:39:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	219882	20.954 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	19020	1.005 ng/ml
2) t 2,2,4-Trimethylpentane	7.489	3554	0.171 ng/ml
3) t n-Heptane	7.744	4594	0.232 ng/ml
4) t Benzene	7.879	7824	0.339 ng/ml
6) t Toluene	10.615	25824	1.180 ng/ml
7) t Ethylbenzene	13.053	8247	0.410 ng/ml
8) t m-Xylene	13.182	15923	0.790 ng/ml
9) t O-Xylene	13.920	15195	0.762 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	15262	0.766 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
Data File : FB026679.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2022 19:03
Operator : AJ/MA
Sample : N1645-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 00:39:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

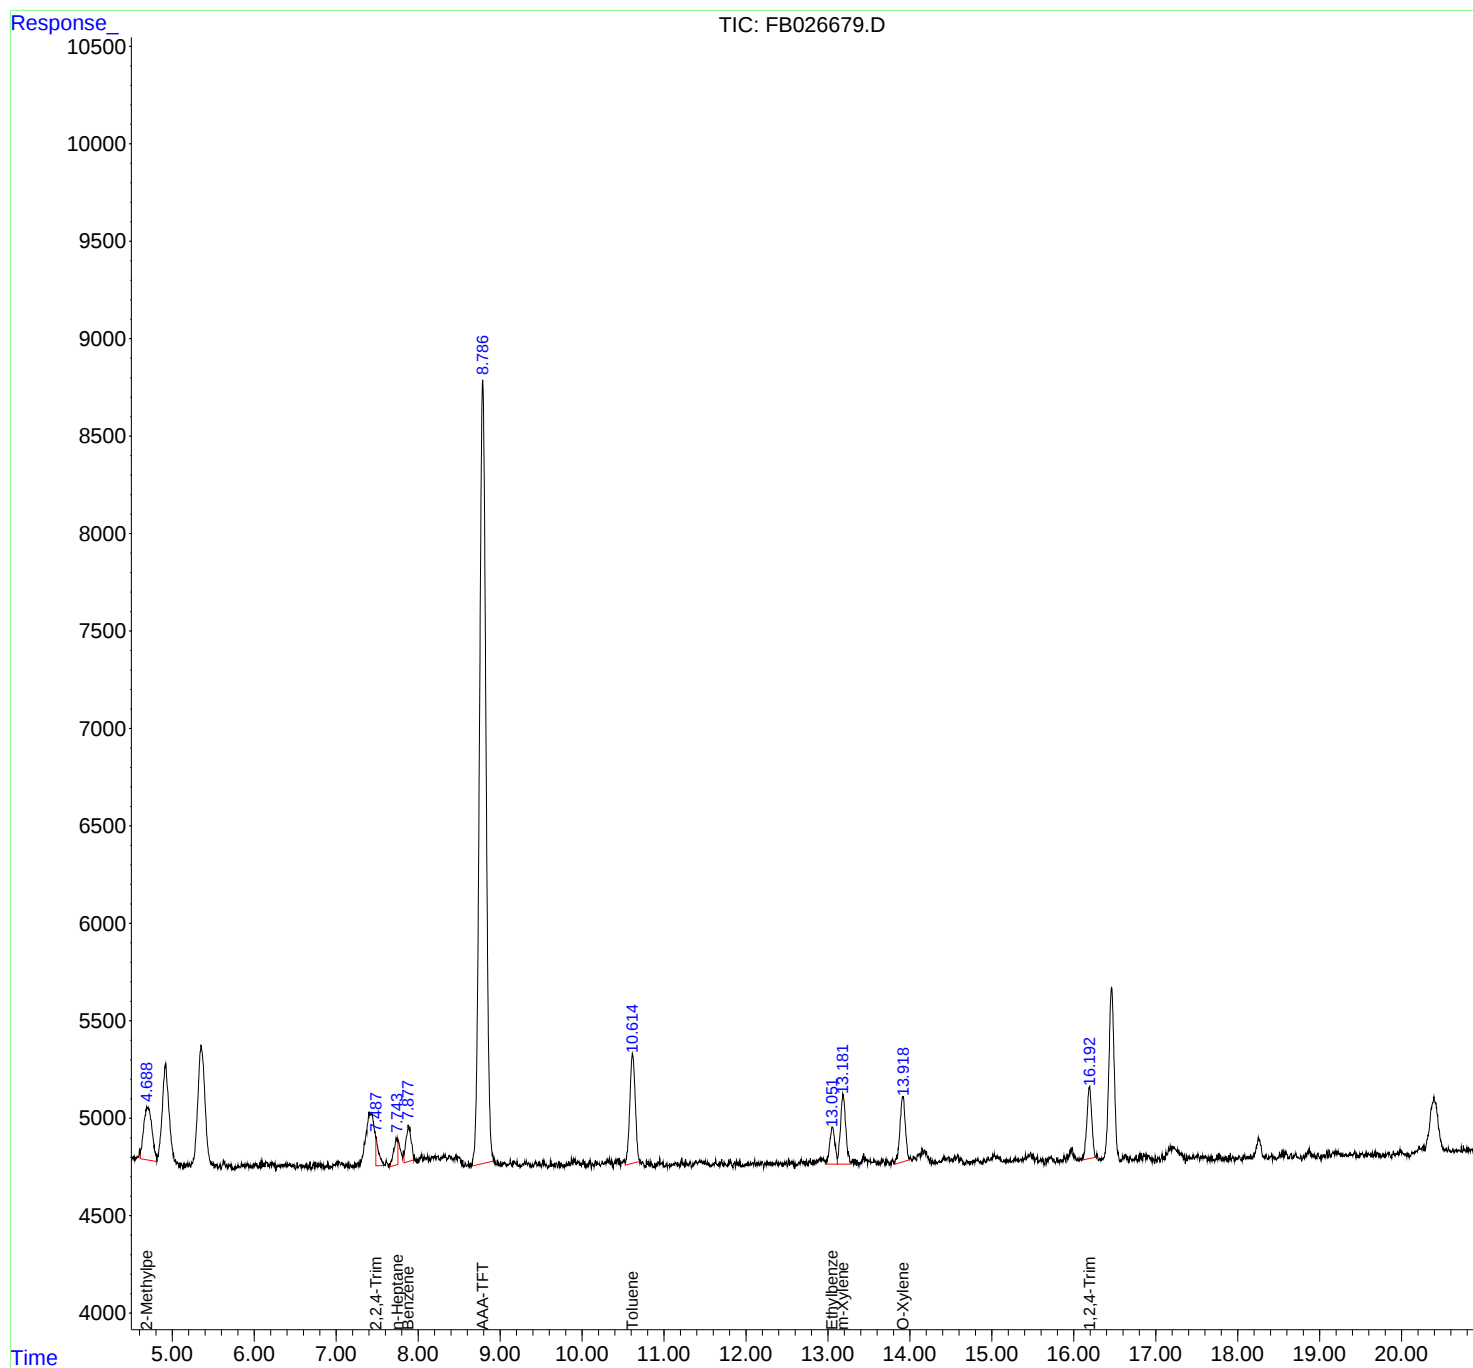

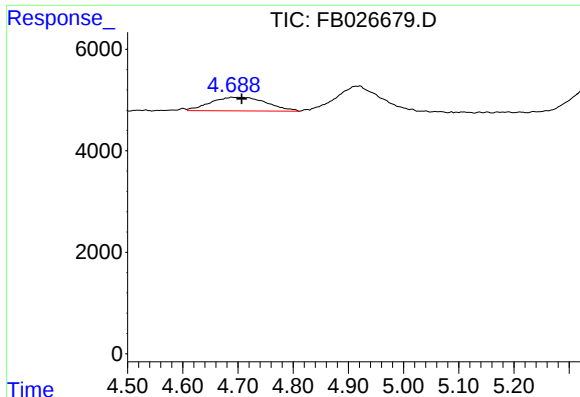


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.017 min
Response: 19020
Conc: 1.00 ng/ml

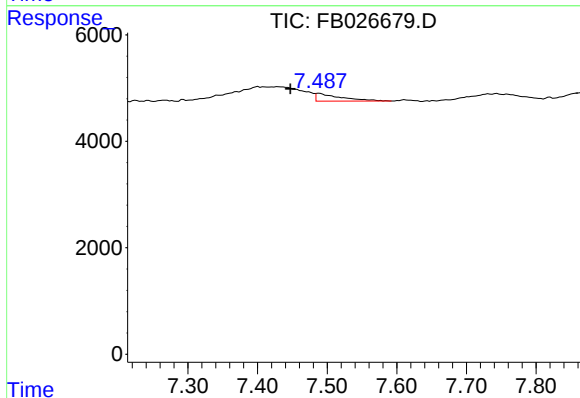


#2 2,2,4-Trimethylpentane

R.T.: 7.489 min
Delta R.T.: 0.042 min
Response: 3554
Conc: 0.17 ng/ml

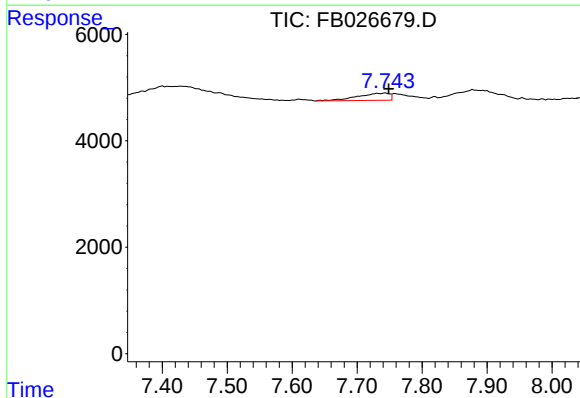


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.004 min
Response: 4594
Conc: 0.23 ng/ml

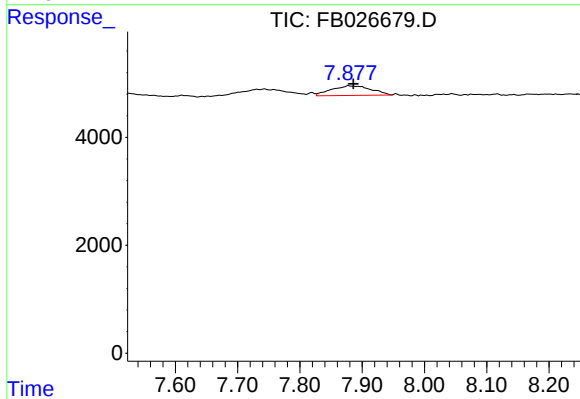


#4 Benzene

R.T.: 7.879 min
Delta R.T.: -0.007 min
Response: 7824
Conc: 0.34 ng/ml

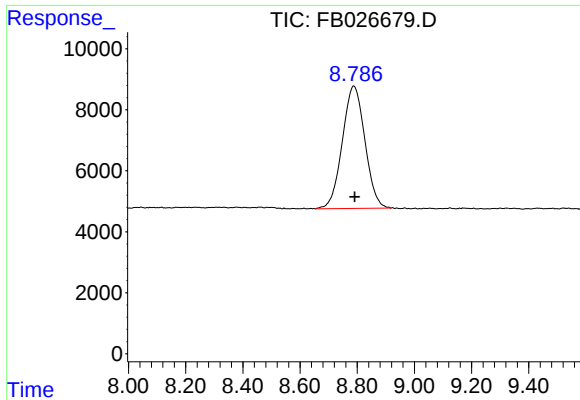


#5 AAA-TFT

R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 219882
Conc: 20.95 ng/ml

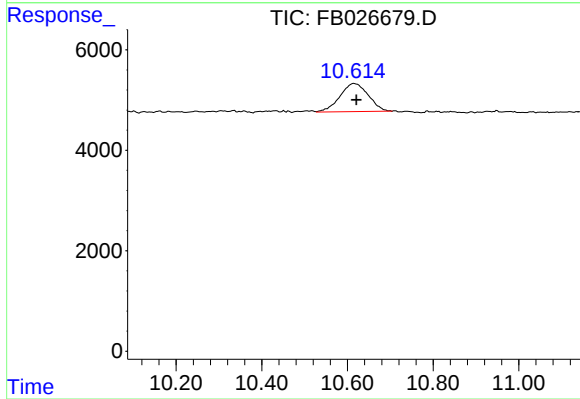


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.006 min
Response: 25824
Conc: 1.18 ng/ml

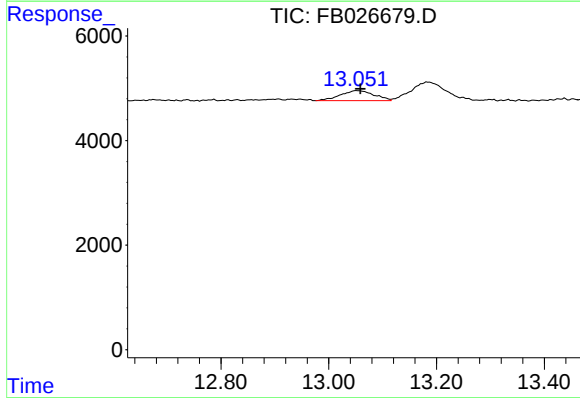


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 8247
Conc: 0.41 ng/ml

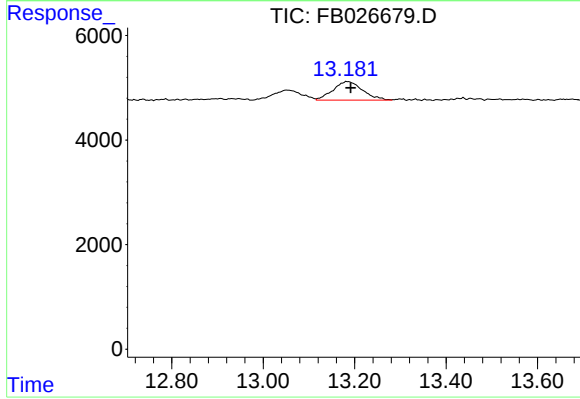


#8 m-Xylene

R.T.: 13.182 min
Delta R.T.: -0.009 min
Response: 15923
Conc: 0.79 ng/ml

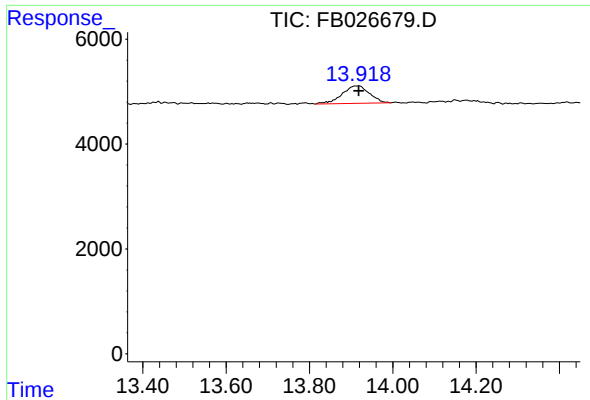

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.001 min
Response: 15195
Conc: 0.76 ng/ml

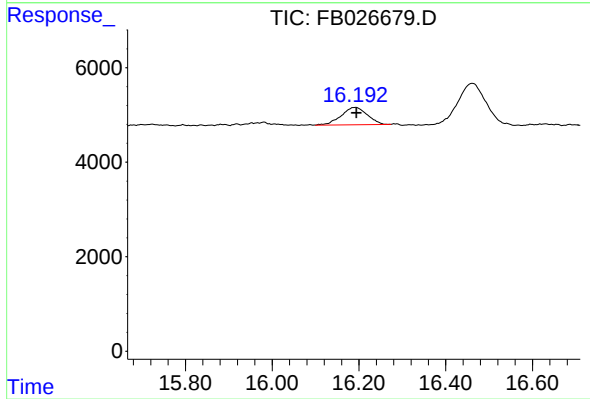

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 15262
Conc: 0.77 ng/ml