

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
 Data File : FB026675.D
 Signal(s) : FID2B.CH
 Acq On : 10 Mar 2022 16:30
 Operator : AJ/MA
 Sample : N1645-03
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 11 00:52:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Wed Mar 09 03:13:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.790	187046	17.825 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.697	17340	0.916 ng/mlm
2) t	2,2,4-Trimethylpentane	7.424	23516	1.135 ng/mlm
3) t	n-Heptane	7.750	6251	0.316 ng/mlm
4) t	Benzene	7.887	6940	0.301 ng/mlm
6) t	Toluene	10.622	23203	1.060 ng/ml
7) t	Ethylbenzene	13.056	7881	0.392 ng/ml
8) t	m-Xylene	13.191	15911	0.790 ng/ml
9) t	O-Xylene	13.914	17765	0.890 ng/ml
10) t	1,2,4-Trimethylbenzene	16.185	18561	0.932 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031022\
Data File : FB026675.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2022 16:30
Operator : AJ/MA
Sample : N1645-03
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 11 00:52:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Wed Mar 09 03:13:41 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

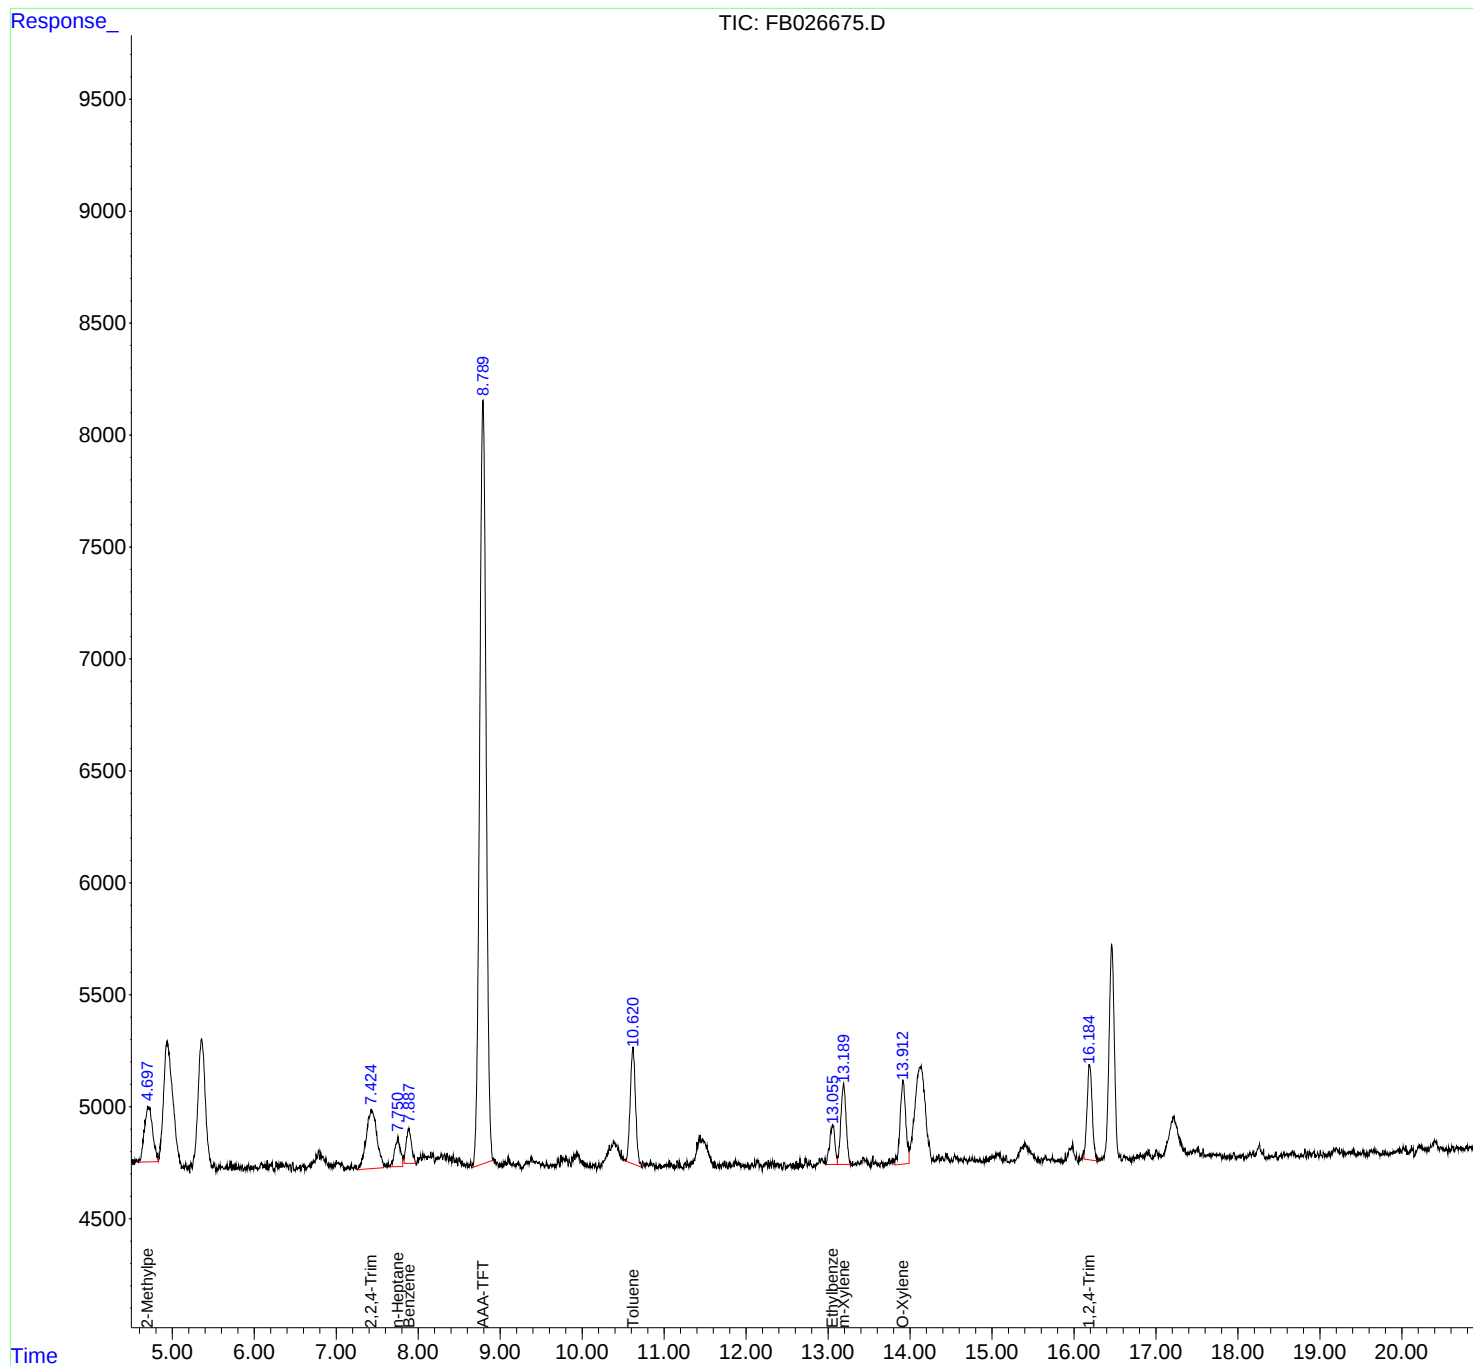

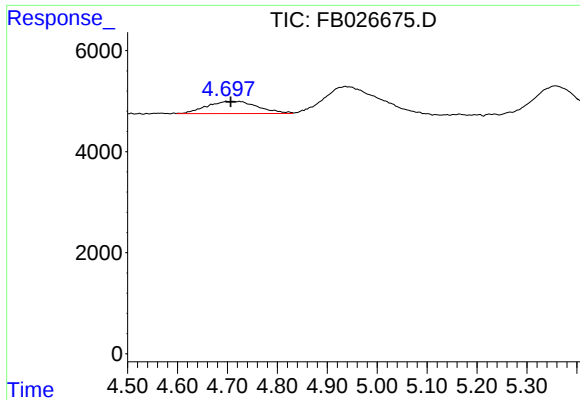


#1 2-Methylpentane

R.T.: 4.697 min
Delta R.T.: -0.010 min
Response: 17340
Conc: 0.92 ng/ml m

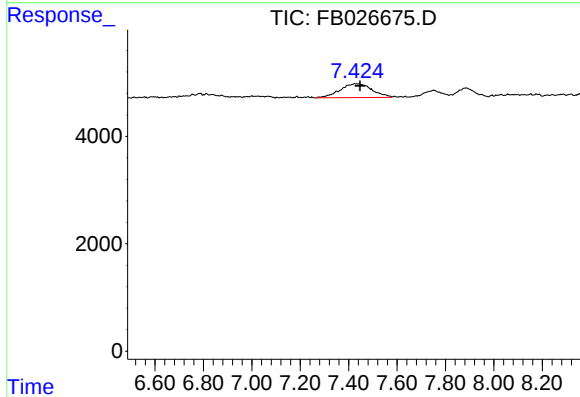


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.024 min
Response: 23516
Conc: 1.13 ng/ml m

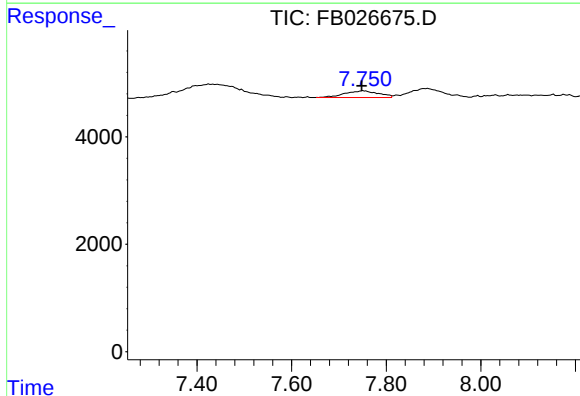


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 6251
Conc: 0.32 ng/ml m

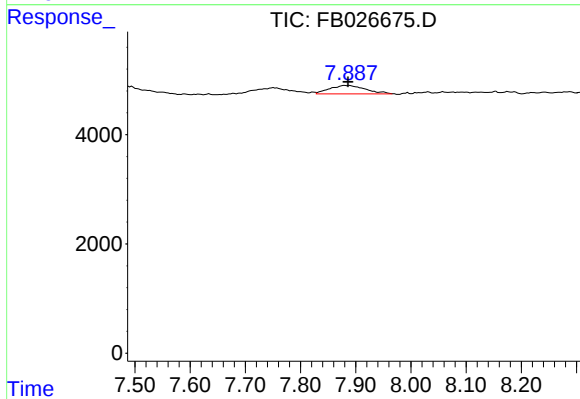


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 6940
Conc: 0.30 ng/ml m

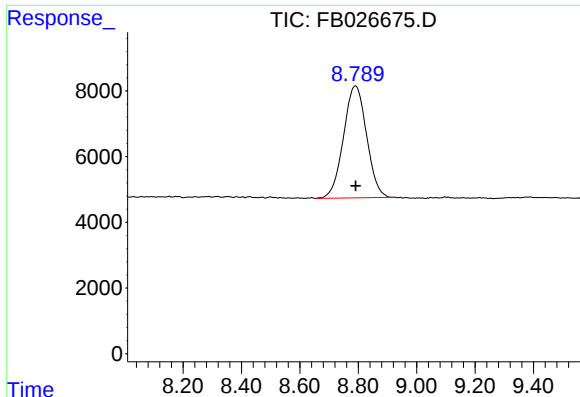


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.001 min
Response: 187046
Conc: 17.83 ng/ml

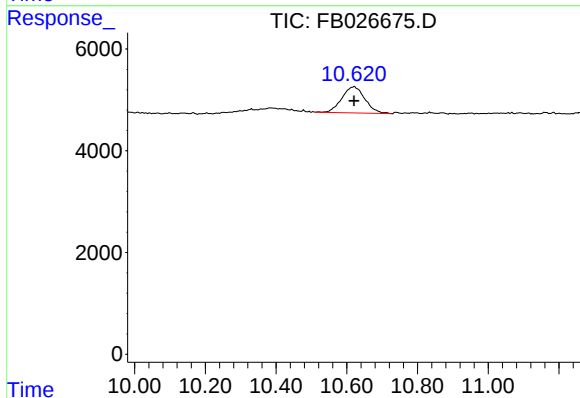


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 23203
Conc: 1.06 ng/ml

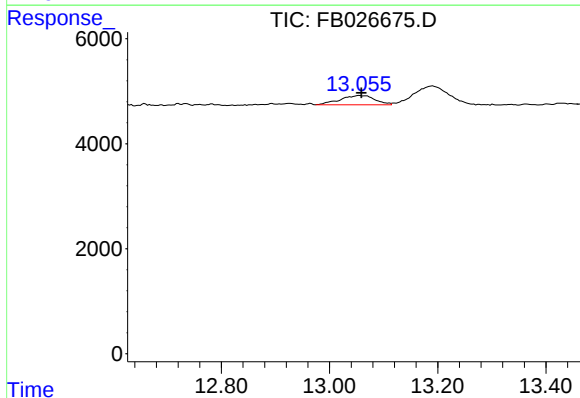


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 7881
Conc: 0.39 ng/ml

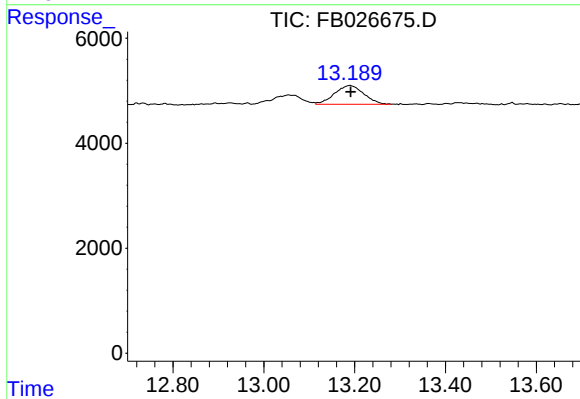


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 15911
Conc: 0.79 ng/ml

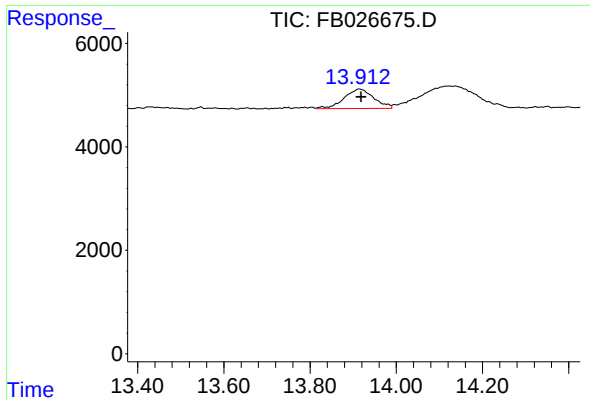

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.005 min
Response: 17765
Conc: 0.89 ng/ml

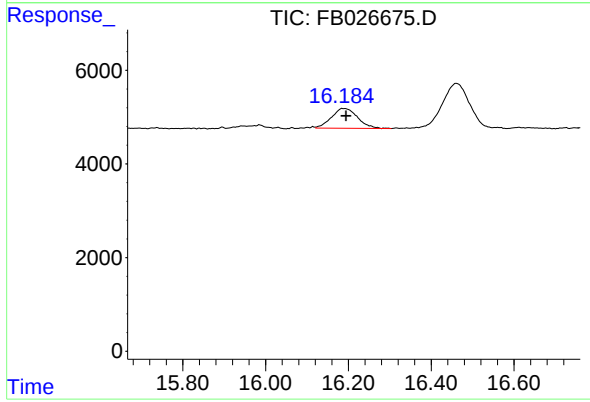

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.009 min
Response: 18561
Conc: 0.93 ng/ml