

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031025\
Data File : FB031573.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2025 11:24
Operator : YP/AJ
Sample : Q1515-02 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 11 01:25:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Thu Mar 06 13:17:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	426449	18.832 ng/ml
Target Compounds			
6) t Toluene	10.616	10901	0.276 ng/ml
7) t Ethylbenzene	13.058	5287	0.150 ng/ml
8) t m-Xylene	13.197	8681	0.225 ng/ml
9) t O-Xylene	13.923	11341	0.307 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	13513	0.478 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031025\
Data File : FB031573.D
Signal(s) : FID2B.CH
Acq On : 10 Mar 2025 11:24
Operator : YP/AJ
Sample : Q1515-02 50X
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 11 01:25:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Thu Mar 06 13:17:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

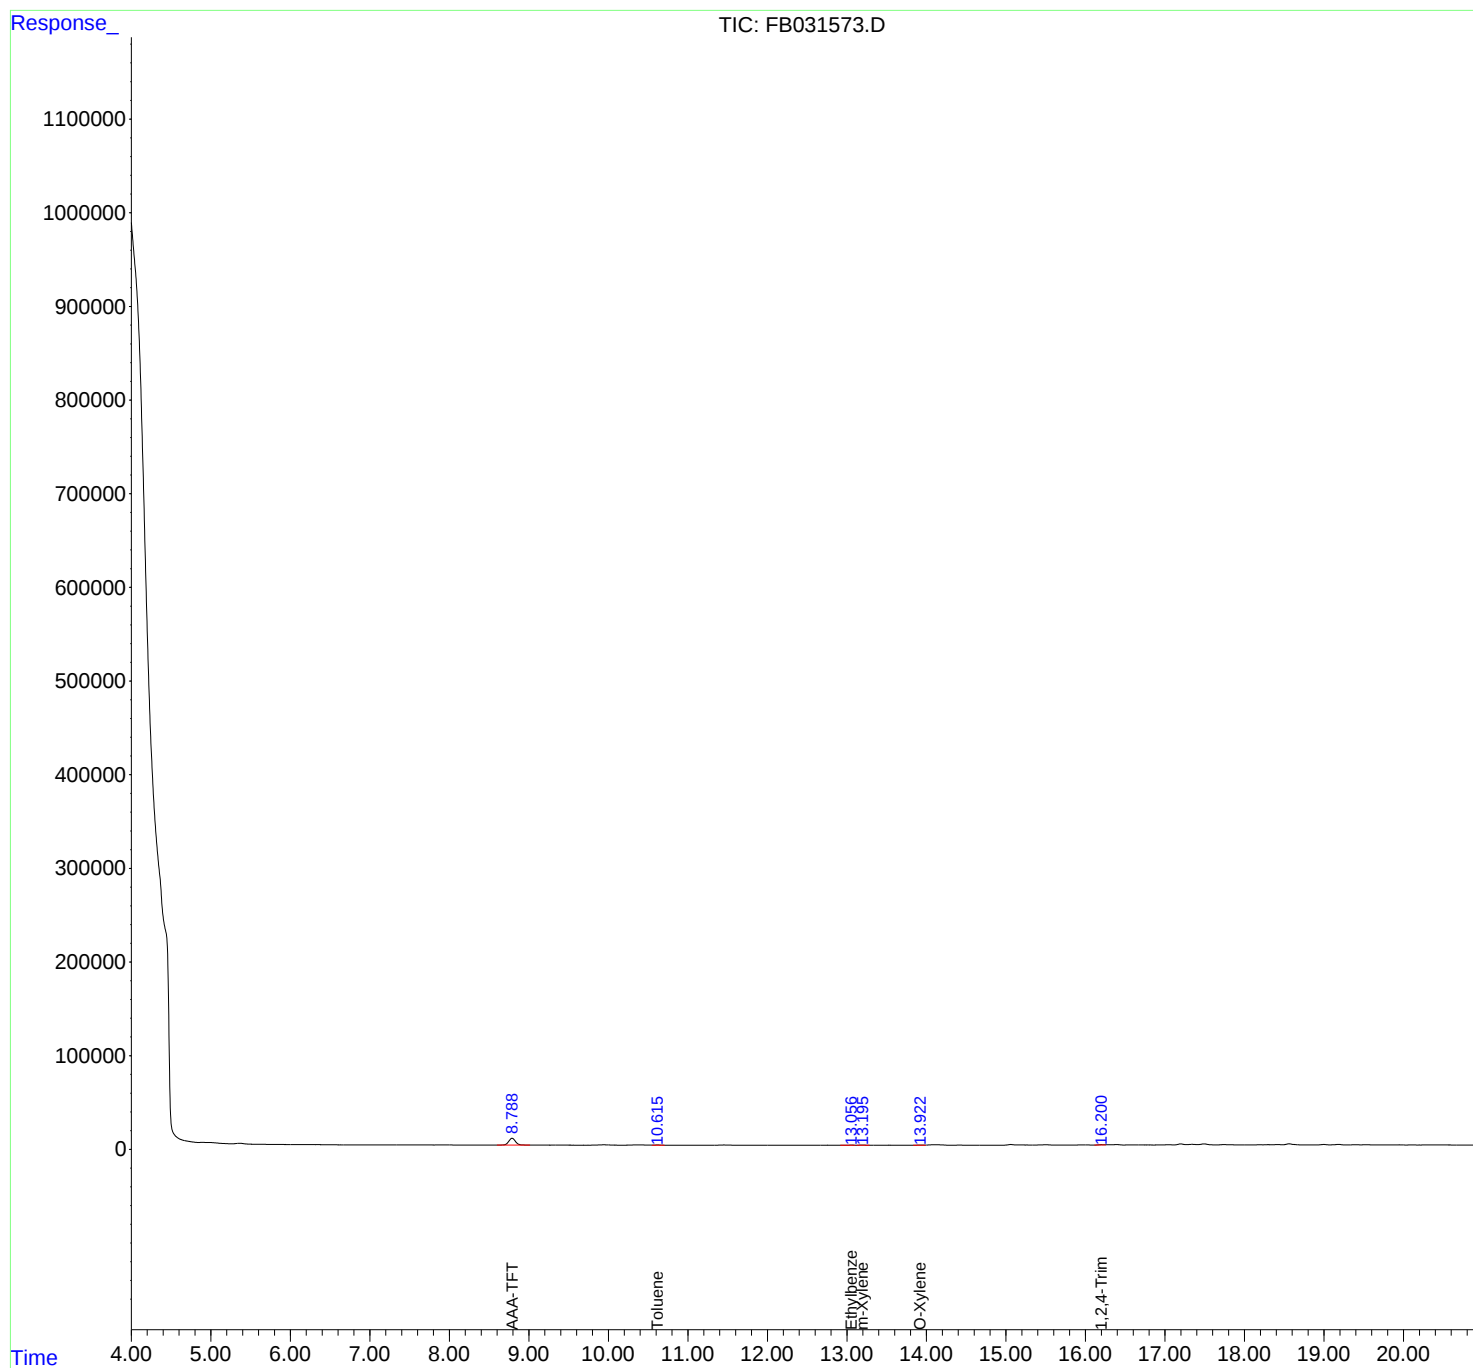


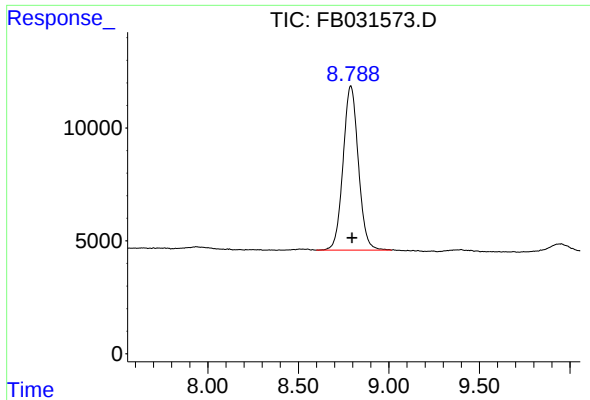

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.007 min
Response: 426449
Conc: 18.83 ng/ml

Instrument :
FID_B
ClientSampleId :

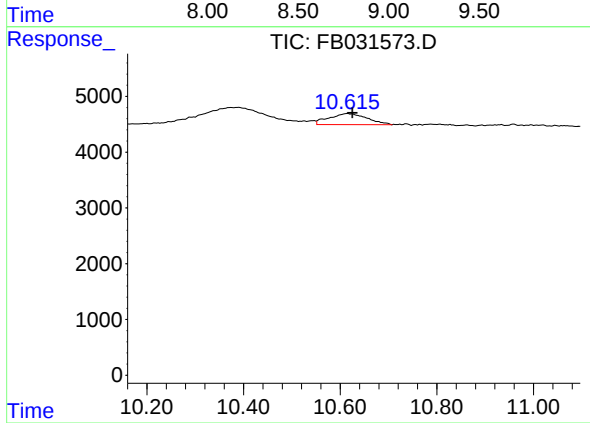


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.010 min
Response: 10901
Conc: 0.28 ng/ml

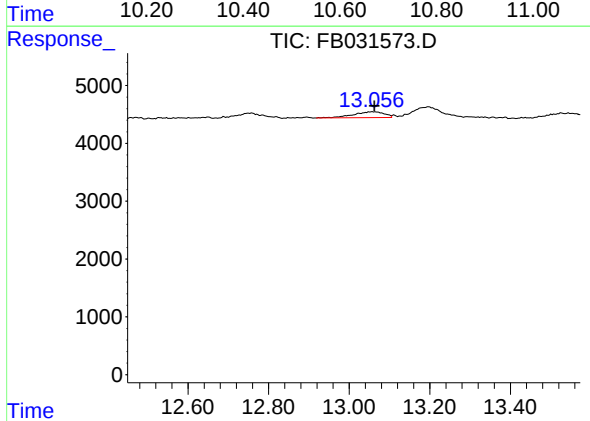


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.005 min
Response: 5287
Conc: 0.15 ng/ml

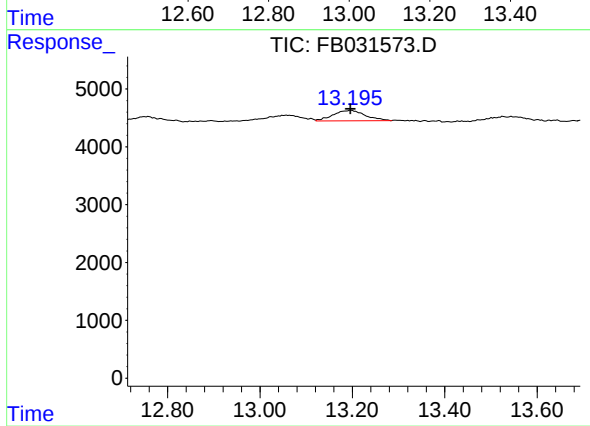

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.001 min
Response: 8681
Conc: 0.23 ng/ml

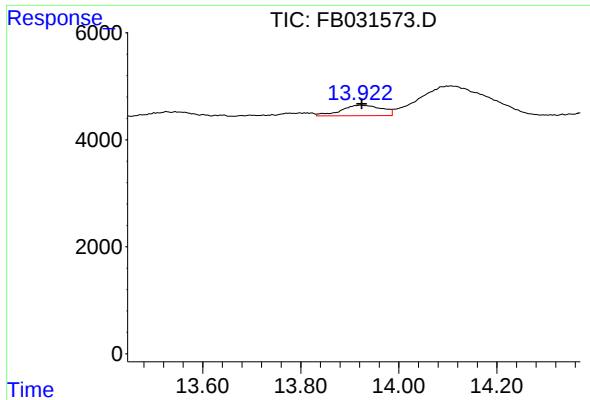

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.001 min
Response: 11341
Conc: 0.31 ng/ml

Instrument :
FID_B
ClientSampleId :

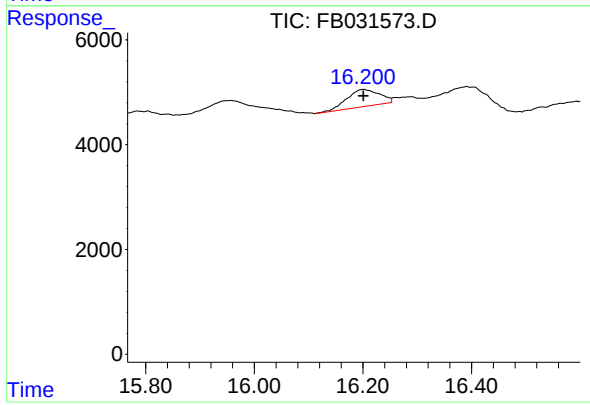

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.002 min
Response: 13513
Conc: 0.48 ng/ml