

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
 Data File : FB020147.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2019 00:41
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 12 09:25:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	490704	18.692 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.898	986197	29.235 ng/ml
2) t 2,2,4-Trimethylpentane	7.659	896298	27.331 ng/ml
3) t n-Heptane	7.993	394117	9.470 ng/ml
4) t Benzene	8.131	437805	9.404 ng/ml
6) t Toluene	10.885	1012423	27.398 ng/ml
7) t Ethylbenzene	13.338	212791	9.044 ng/ml
8) t m-Xylene	13.471	403547	18.918 ng/ml
9) t O-Xylene	14.203	384161	20.280 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	392136	19.773 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
Data File : FB020147.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2019 00:41
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 12 09:25:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

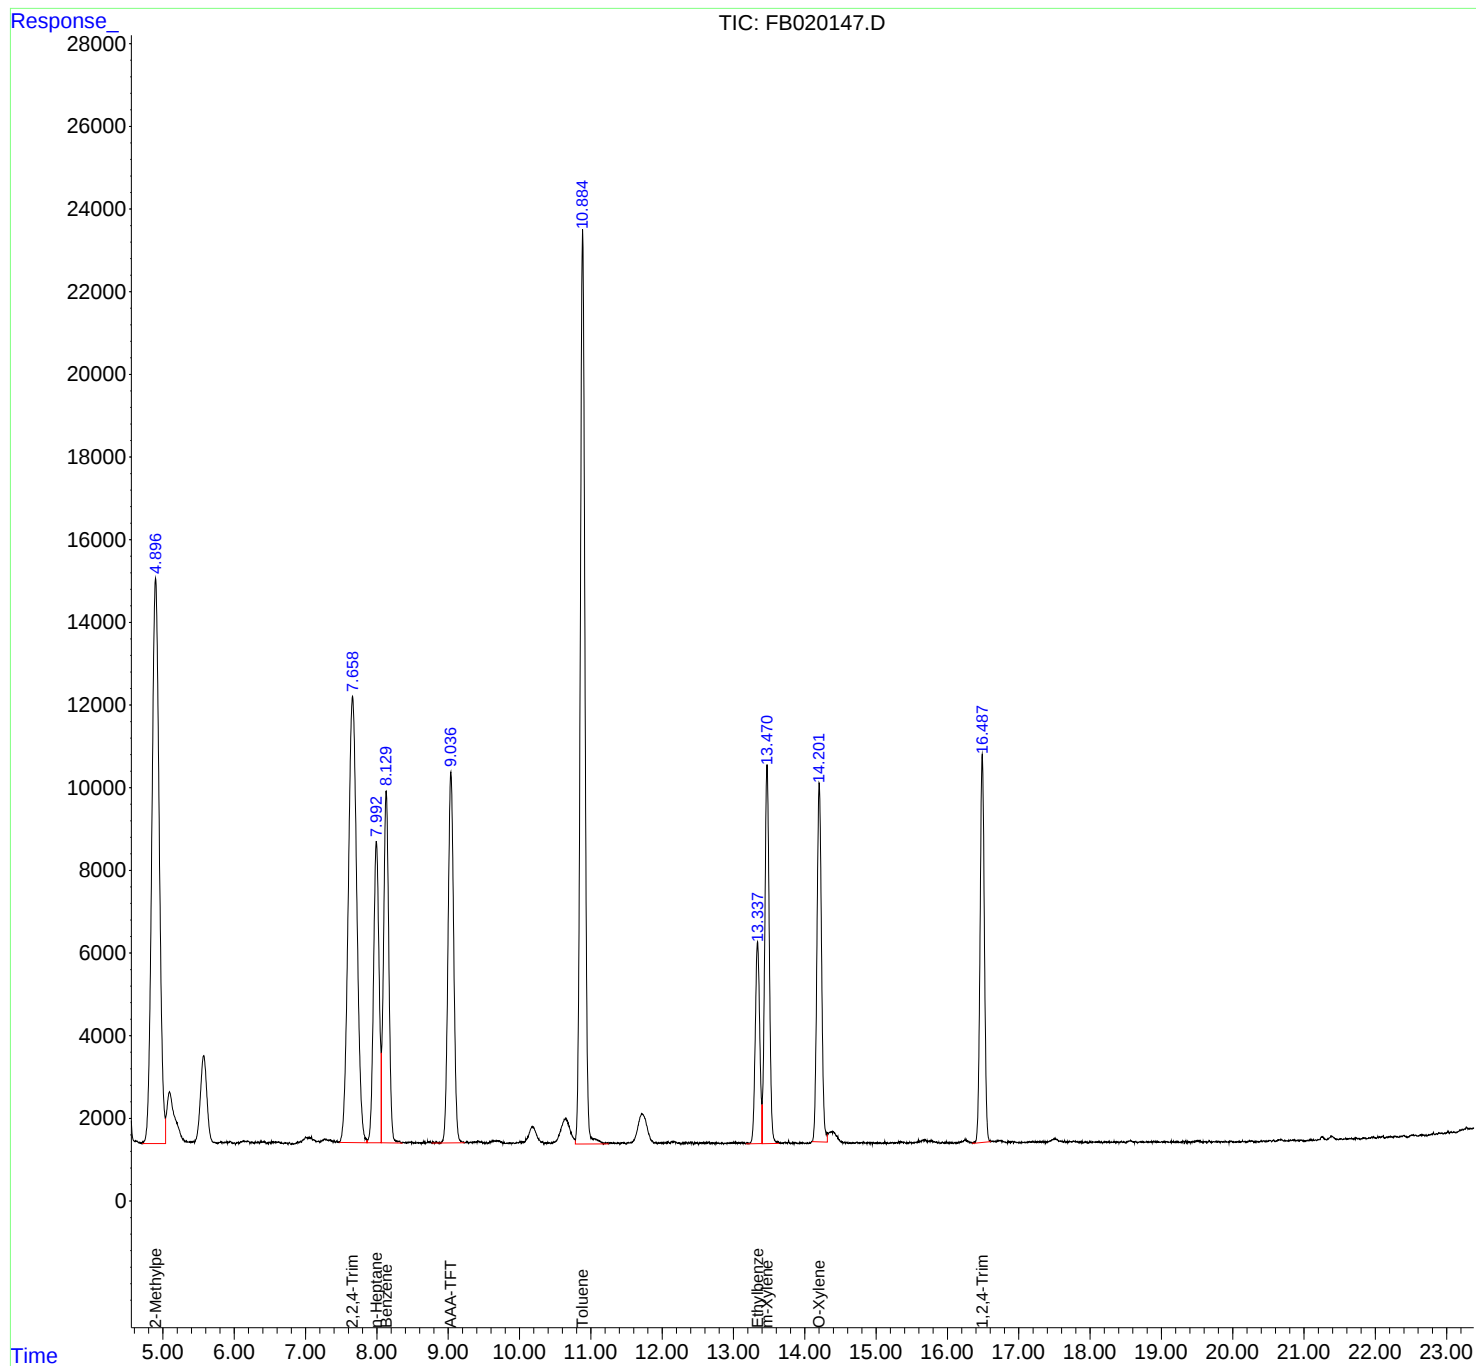


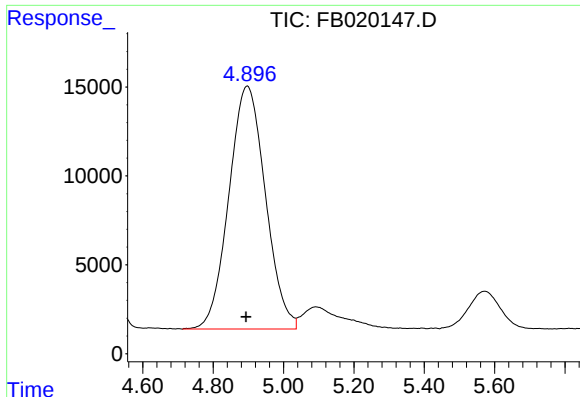

#1 2-Methylpentane


R.T.: 4.898 min
Delta R.T.: 0.004 min
Response: 986197
Conc: 29.24 ng/ml

Instrument :
FID_B
ClientSampleId :

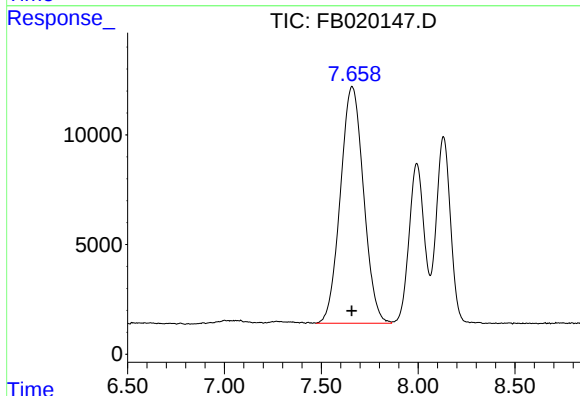


#2 2,2,4-Trimethylpentane

R.T.: 7.659 min
Delta R.T.: 0.002 min
Response: 896298
Conc: 27.33 ng/ml

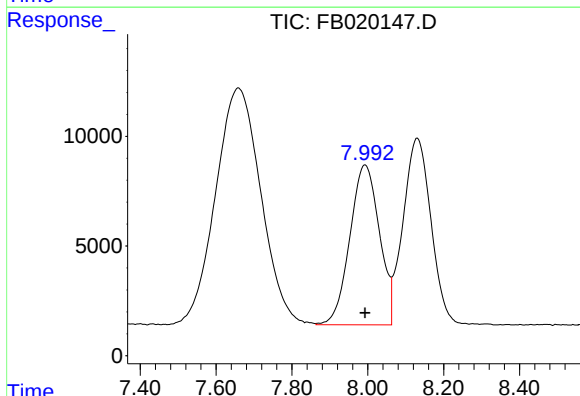


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 394117
Conc: 9.47 ng/ml

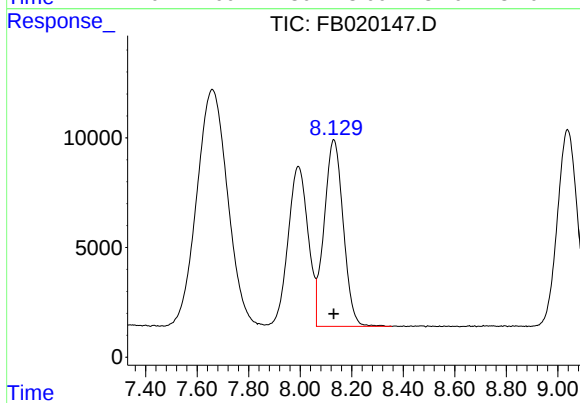

#4 Benzene


R.T.: 8.131 min
Delta R.T.: 0.000 min
Response: 437805
Conc: 9.40 ng/ml

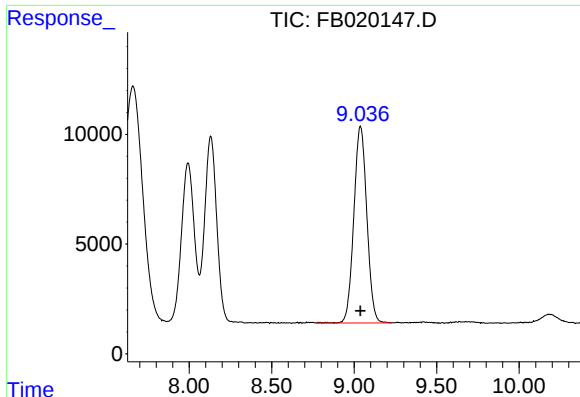

#5 AAA-TFT


R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 490704
Conc: 18.69 ng/ml

Instrument :
FID_B
ClientSampleId :

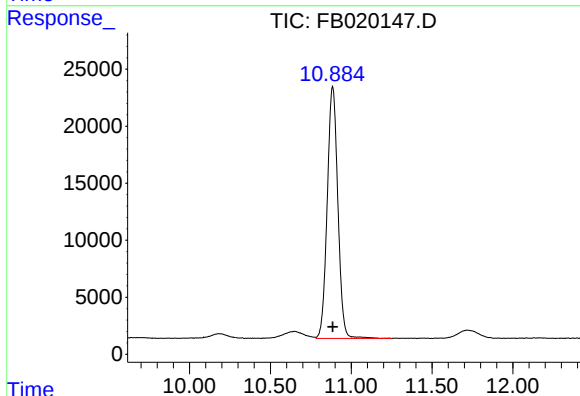


#6 Toluene

R.T.: 10.885 min
Delta R.T.: 0.000 min
Response: 1012423
Conc: 27.40 ng/ml

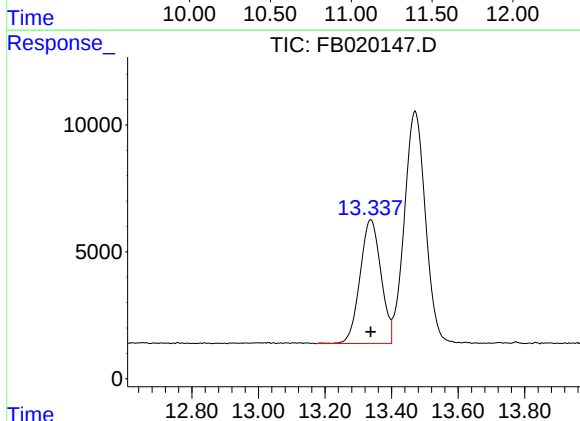


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: 0.000 min
Response: 212791
Conc: 9.04 ng/ml

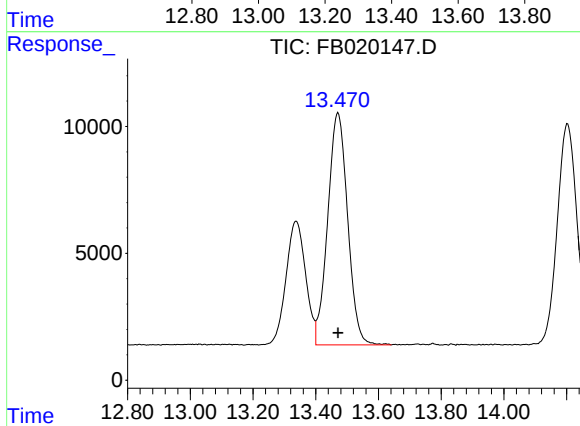

#8 m-Xylene


R.T.: 13.471 min
Delta R.T.: 0.000 min
Response: 403547
Conc: 18.92 ng/ml

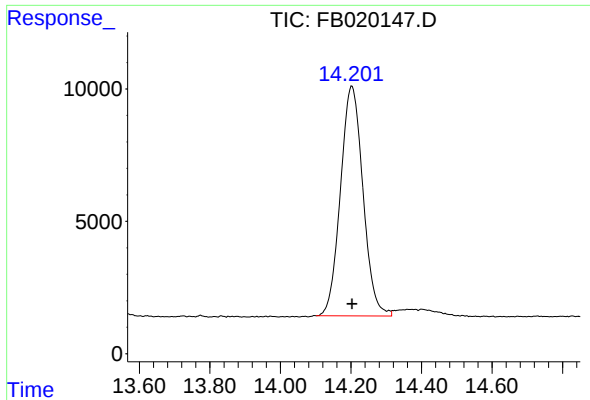

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: 0.000 min
Response: 384161
Conc: 20.28 ng/ml

Instrument :
FID_B
ClientSampleId :

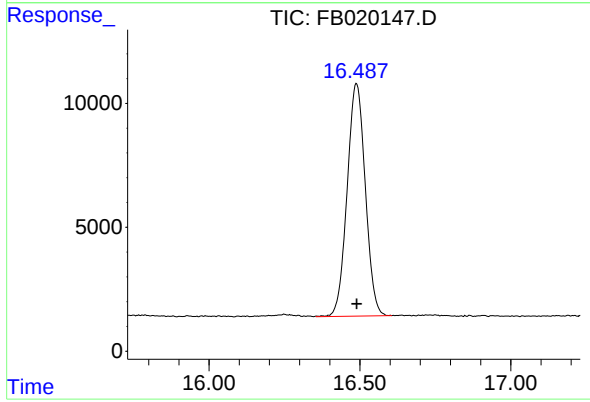

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: 0.000 min
Response: 392136
Conc: 19.77 ng/ml