

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
 Data File : FB020129.D
 Signal(s) : FID2B.CH
 Acq On : 11 Mar 2019 15:42
 Operator : MJ/SJ
 Sample : BSF0311S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0311S1

Integration File: Calibration.e
 Quant Time: Mar 12 09:24:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	523885	19.955 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	1044119	30.952 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	975919	29.759 ng/ml
3) t n-Heptane	7.995	431303	10.364 ng/ml
4) t Benzene	8.133	474229	10.186 ng/ml
6) t Toluene	10.888	1081655	29.271 ng/ml
7) t Ethylbenzene	13.340	228641	9.718 ng/ml
8) t m-Xylene	13.474	428197	20.073 ng/ml
9) t O-Xylene	14.205	398243	21.023 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	415722	20.962 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
Data File : FB020129.D
Signal(s) : FID2B.CH
Acq On : 11 Mar 2019 15:42
Operator : MJ/SJ
Sample : BSF0311S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0311S1

Integration File: Calibration.e
Quant Time: Mar 12 09:24:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

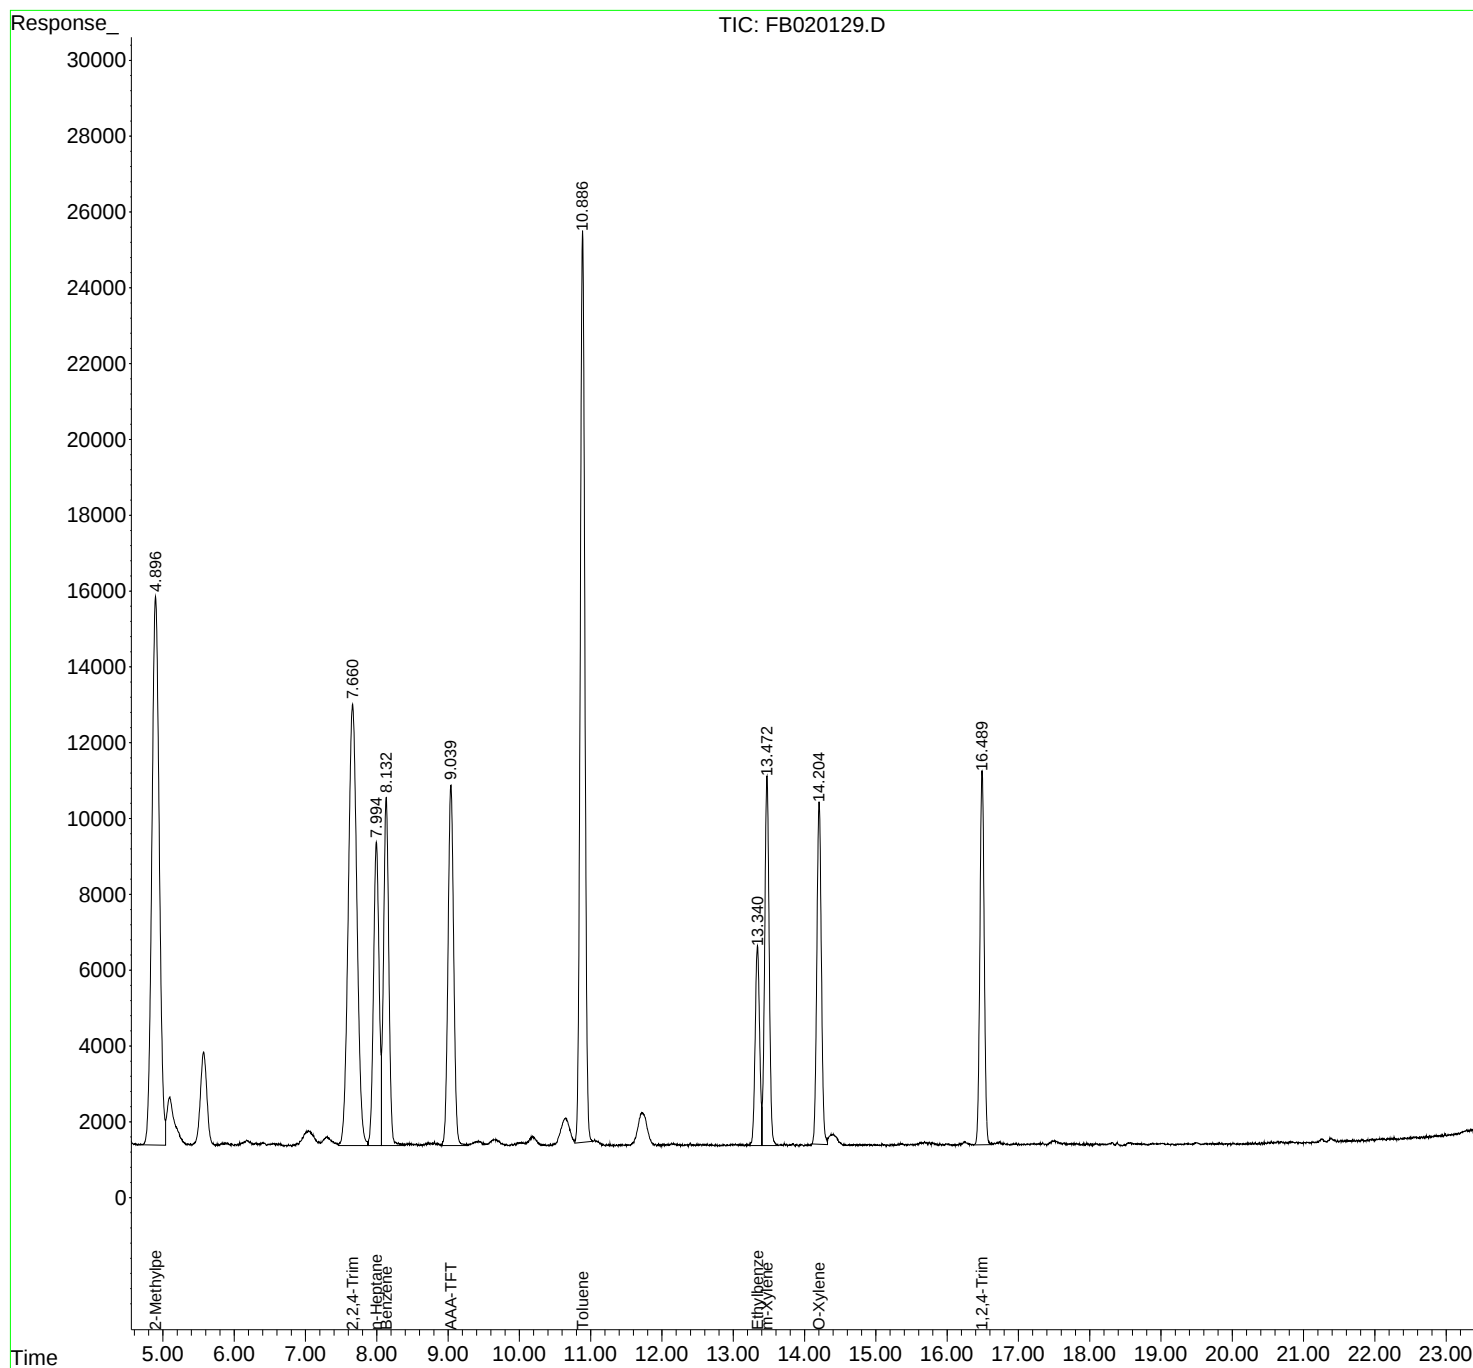


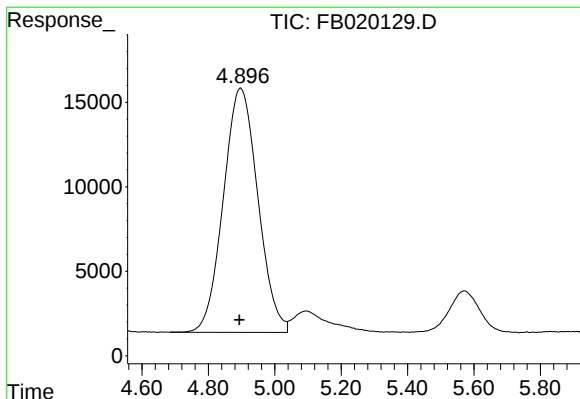

#1 2-Methylpentane


R.T.: 4.897 min
Delta R.T.: 0.003 min
Response: 1044119
Conc: 30.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0311S1

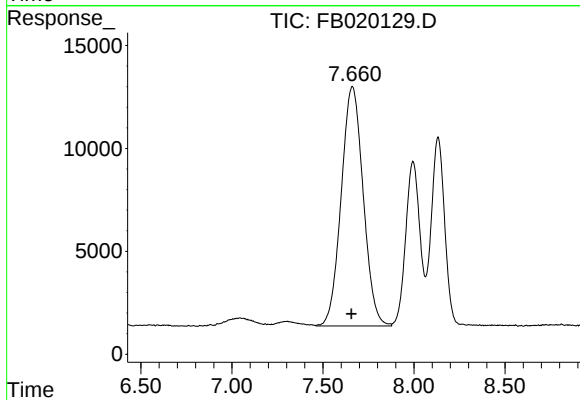


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: 0.004 min
Response: 975919
Conc: 29.76 ng/ml

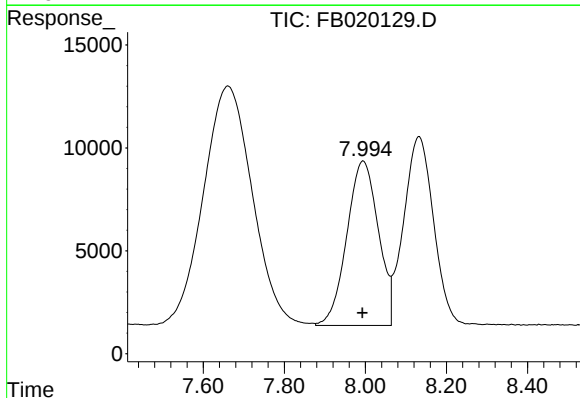


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.002 min
Response: 431303
Conc: 10.36 ng/ml

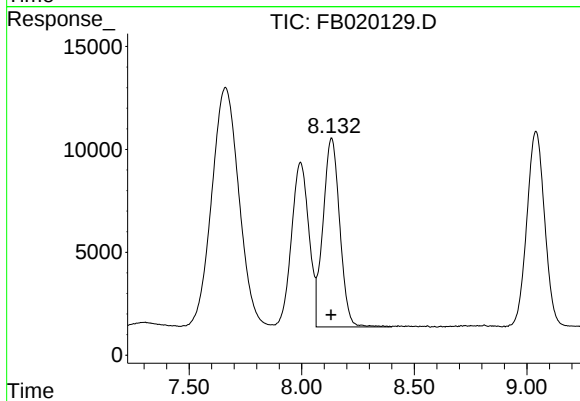

#4 Benzene


R.T.: 8.133 min
Delta R.T.: 0.002 min
Response: 474229
Conc: 10.19 ng/ml

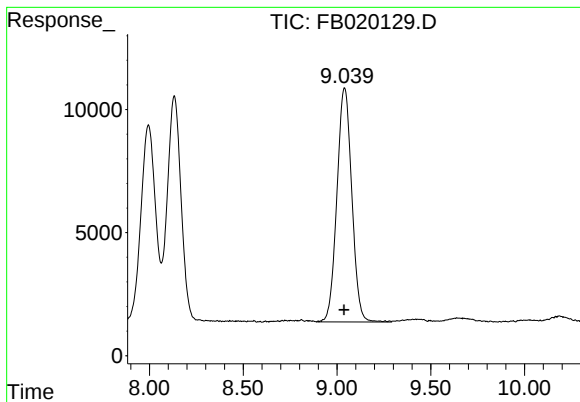

#5 AAA-TFT


R.T.: 9.040 min
Delta R.T.: 0.002 min
Response: 523885
Conc: 19.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0311S1

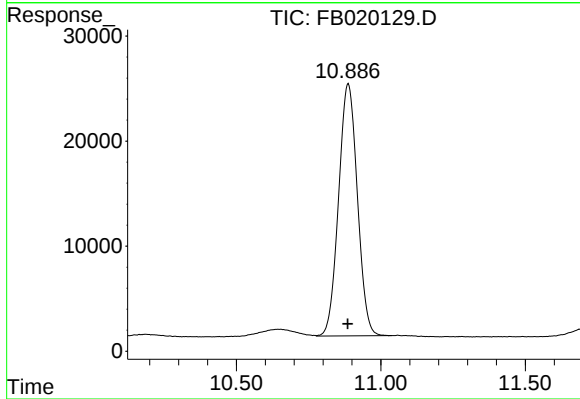


#6 Toluene

R.T.: 10.888 min
Delta R.T.: 0.002 min
Response: 1081655
Conc: 29.27 ng/ml

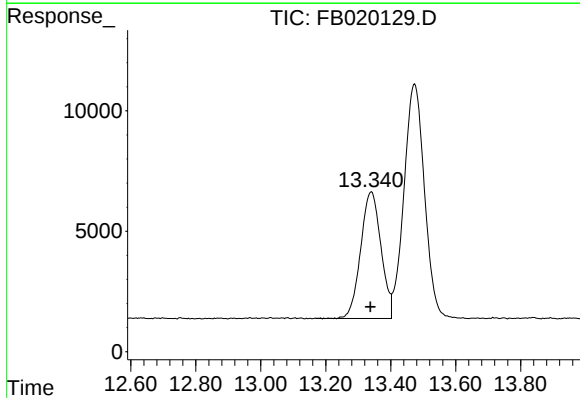


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: 0.003 min
Response: 228641
Conc: 9.72 ng/ml

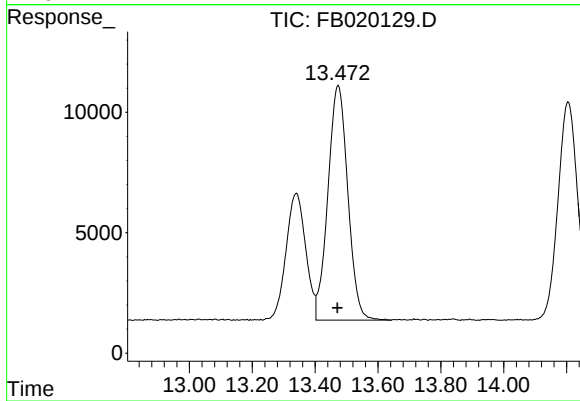

#8 m-Xylene


R.T.: 13.474 min
Delta R.T.: 0.002 min
Response: 428197
Conc: 20.07 ng/ml

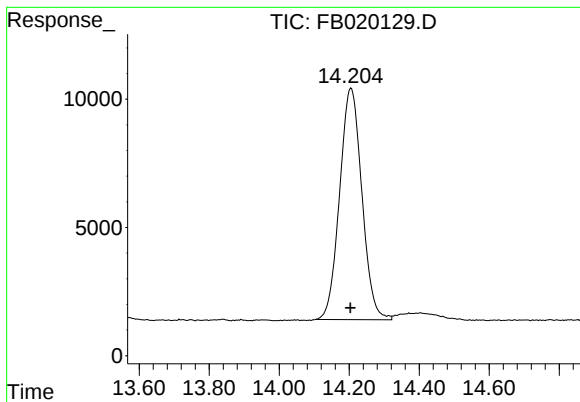

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.002 min
Response: 398243
Conc: 21.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0311S1

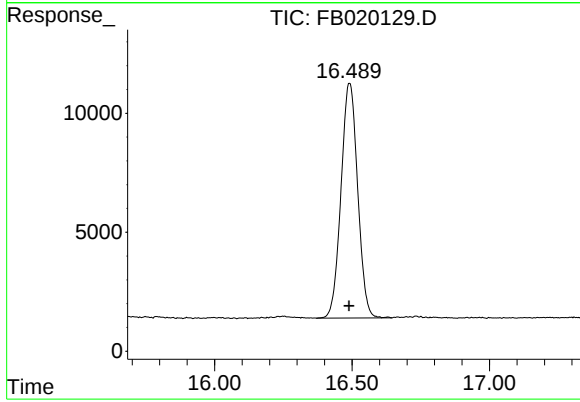

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.002 min
Response: 415722
Conc: 20.96 ng/ml