

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
 Data File : FB020145.D
 Signal(s) : FID2B.CH
 Acq On : 11 Mar 2019 23:41
 Operator : MJ/SJ
 Sample : K1835-01MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-3-1MS

Integration File: Calibration.e
 Quant Time: Mar 12 09:25:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	517548	19.714 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	928926	27.537 ng/ml
2) t 2,2,4-Trimethylpentane	7.659	845786	25.791 ng/ml
3) t n-Heptane	7.993	357678	8.594 ng/ml
4) t Benzene	8.131	427945	9.192 ng/ml
6) t Toluene	10.885	952587	25.778 ng/ml
7) t Ethylbenzene	13.338	204333	8.685 ng/ml
8) t m-Xylene	13.471	396406	18.583 ng/ml
9) t O-Xylene	14.204	382109	20.171 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	391903	19.761 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
Data File : FB020145.D
Signal(s) : FID2B.CH
Acq On : 11 Mar 2019 23:41
Operator : MJ/SJ
Sample : K1835-01MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-3-1MS

Integration File: Calibration.e
Quant Time: Mar 12 09:25:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

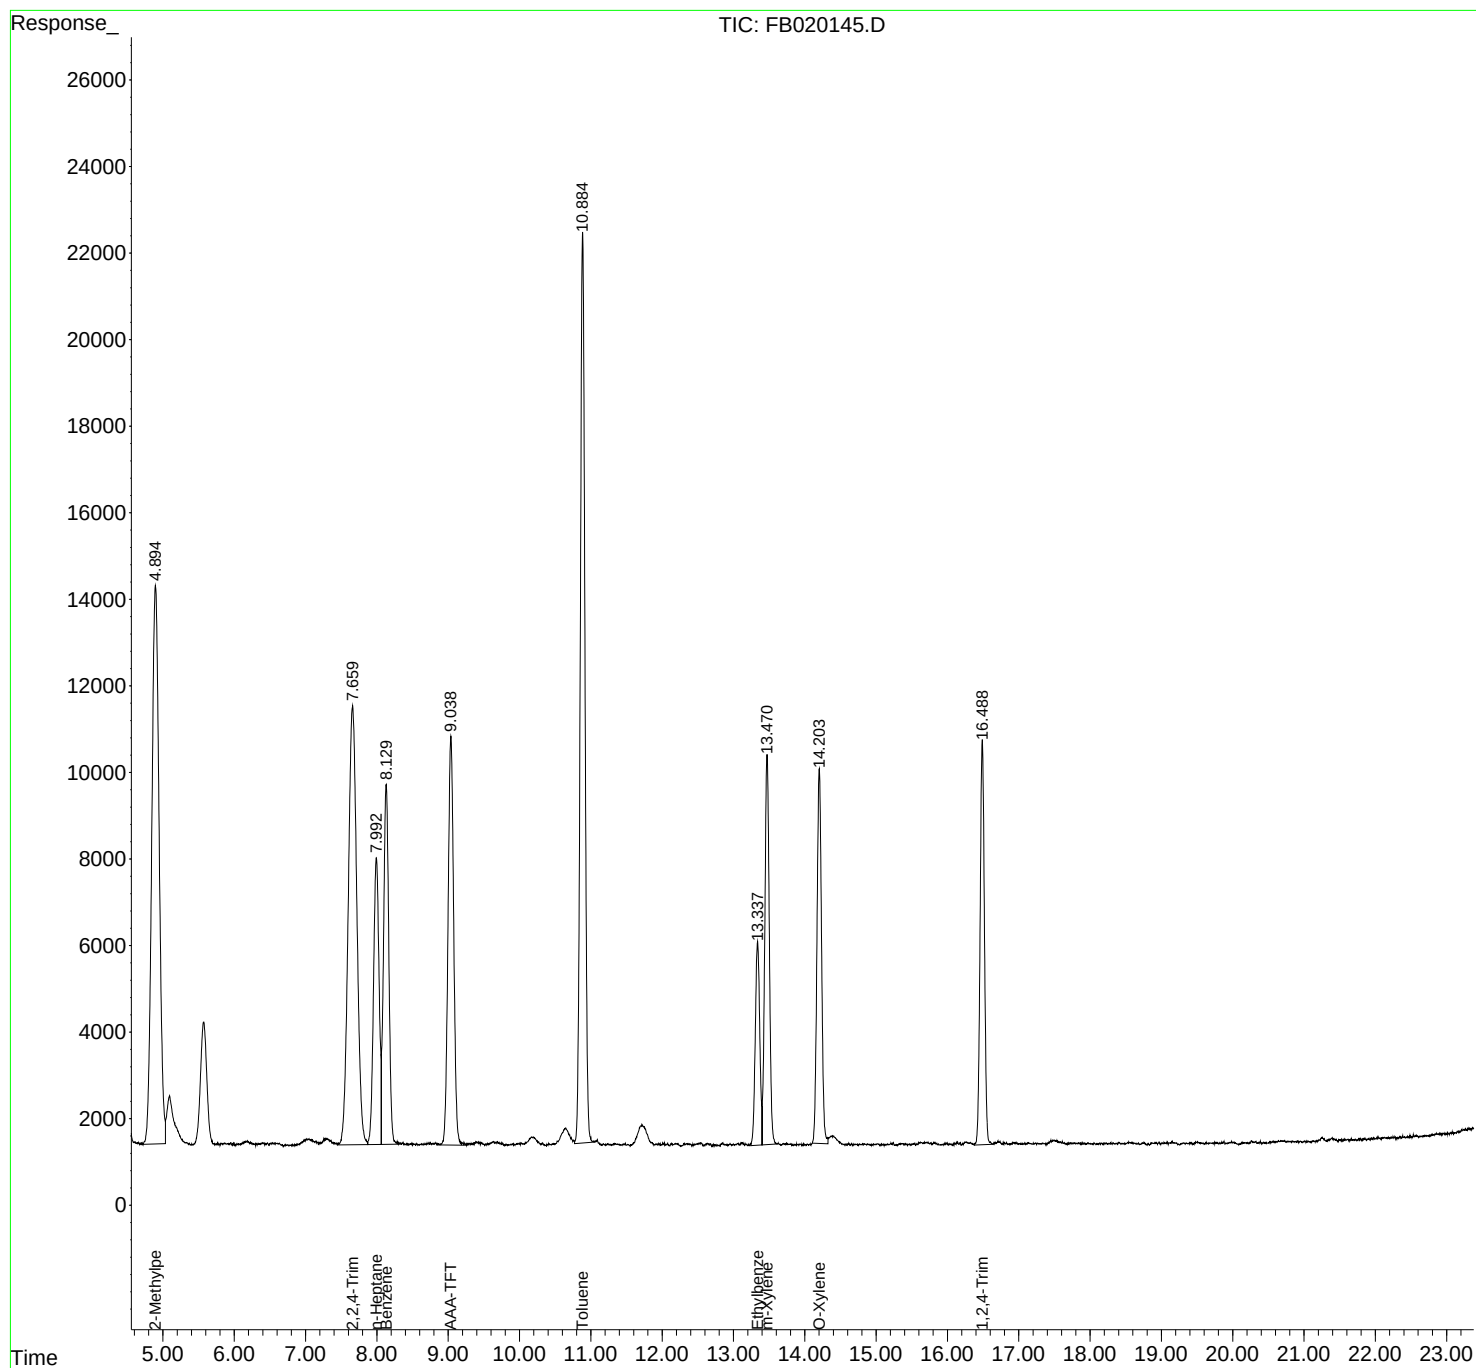


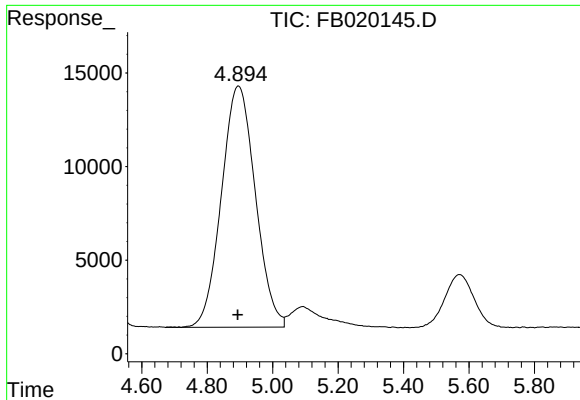

#1 2-Methylpentane


R.T.: 4.896 min
Delta R.T.: 0.002 min
Response: 928926
Conc: 27.54 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-1MS

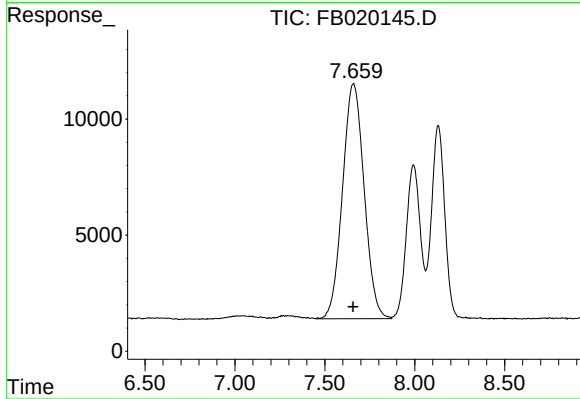


#2 2,2,4-Trimethylpentane

R.T.: 7.659 min
Delta R.T.: 0.002 min
Response: 845786
Conc: 25.79 ng/ml

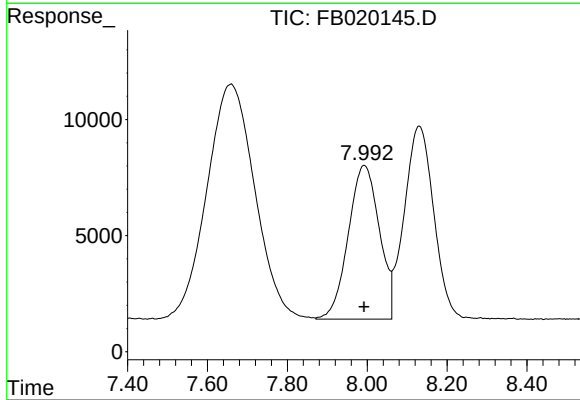


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 357678
Conc: 8.59 ng/ml

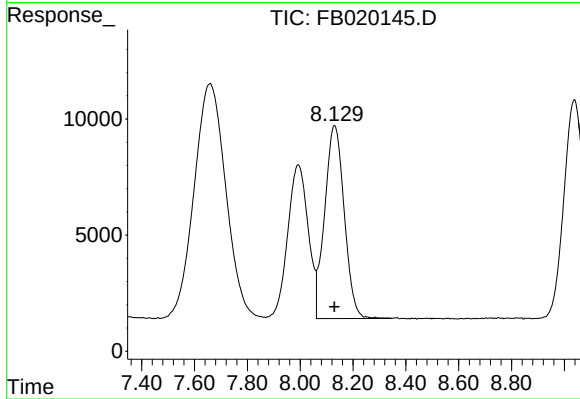

#4 Benzene


R.T.: 8.131 min
Delta R.T.: 0.000 min
Response: 427945
Conc: 9.19 ng/ml

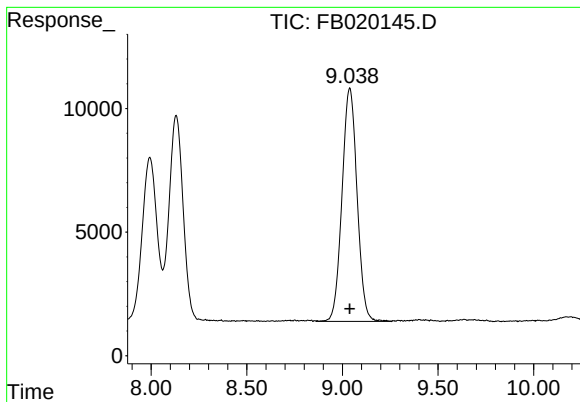

#5 AAA-TFT


R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 517548
Conc: 19.71 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-1MS

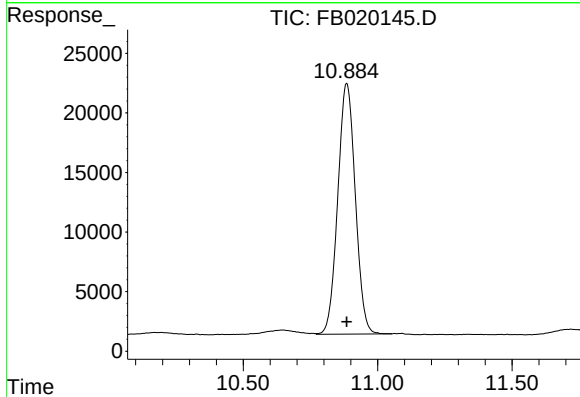


#6 Toluene

R.T.: 10.885 min
Delta R.T.: 0.000 min
Response: 952587
Conc: 25.78 ng/ml

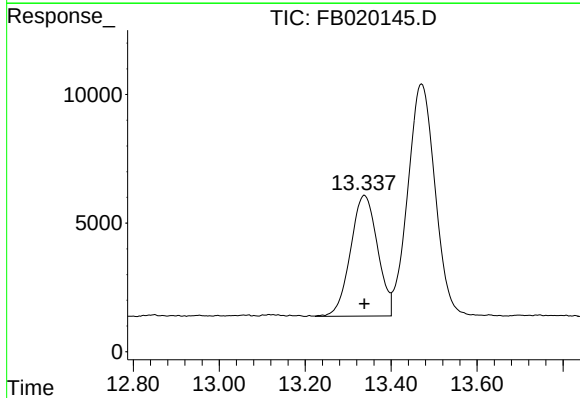


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: 0.000 min
Response: 204333
Conc: 8.68 ng/ml

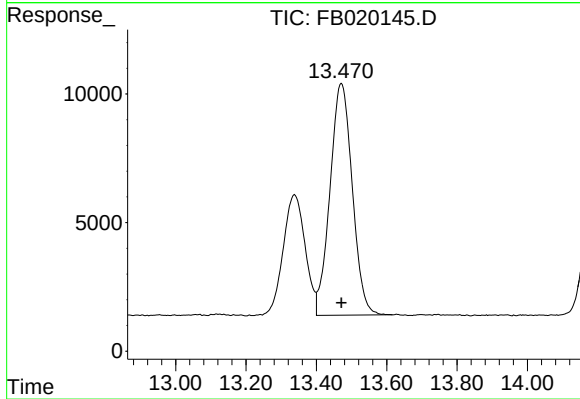

#8 m-Xylene


R.T.: 13.471 min
Delta R.T.: 0.000 min
Response: 396406
Conc: 18.58 ng/ml

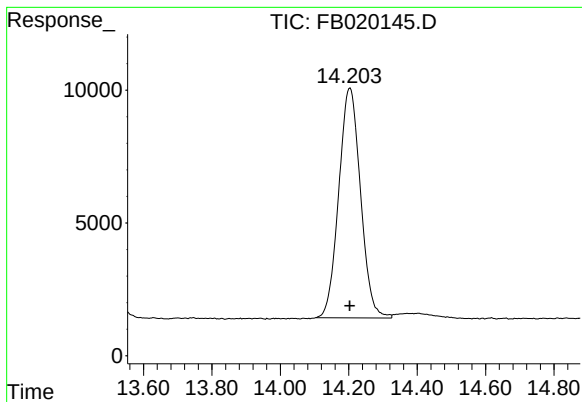

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: 0.000 min
Response: 382109
Conc: 20.17 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-1MS

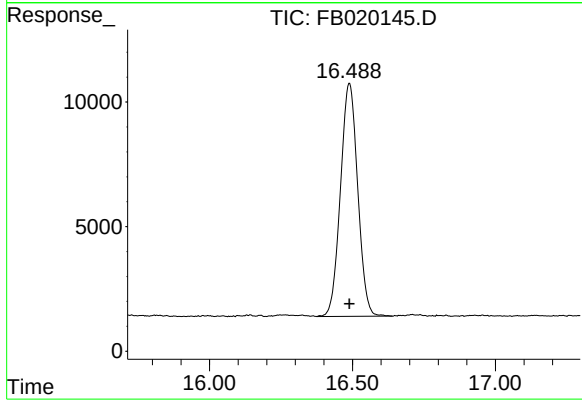

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: 0.000 min
Response: 391903
Conc: 19.76 ng/ml