

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
 Data File : FB020146.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2019 00:11
 Operator : MJ/SJ
 Sample : K1835-01MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-3-1MSD

Integration File: Calibration.e
 Quant Time: Mar 12 09:25:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	507026	19.313 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	891744	26.435 ng/ml
2) t 2,2,4-Trimethylpentane	7.660	800122	24.398 ng/ml
3) t n-Heptane	7.993	320677	7.705 ng/ml
4) t Benzene	8.131	420262	9.027 ng/ml
6) t Toluene	10.886	917587	24.831 ng/ml
7) t Ethylbenzene	13.338	196842	8.366 ng/ml
8) t m-Xylene	13.472	394573	18.497 ng/ml
9) t O-Xylene	14.203	378753	19.994 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	380988	19.211 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031119\
Data File : FB020146.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2019 00:11
Operator : MJ/SJ
Sample : K1835-01MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-3-1MSD

Integration File: Calibration.e
Quant Time: Mar 12 09:25:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

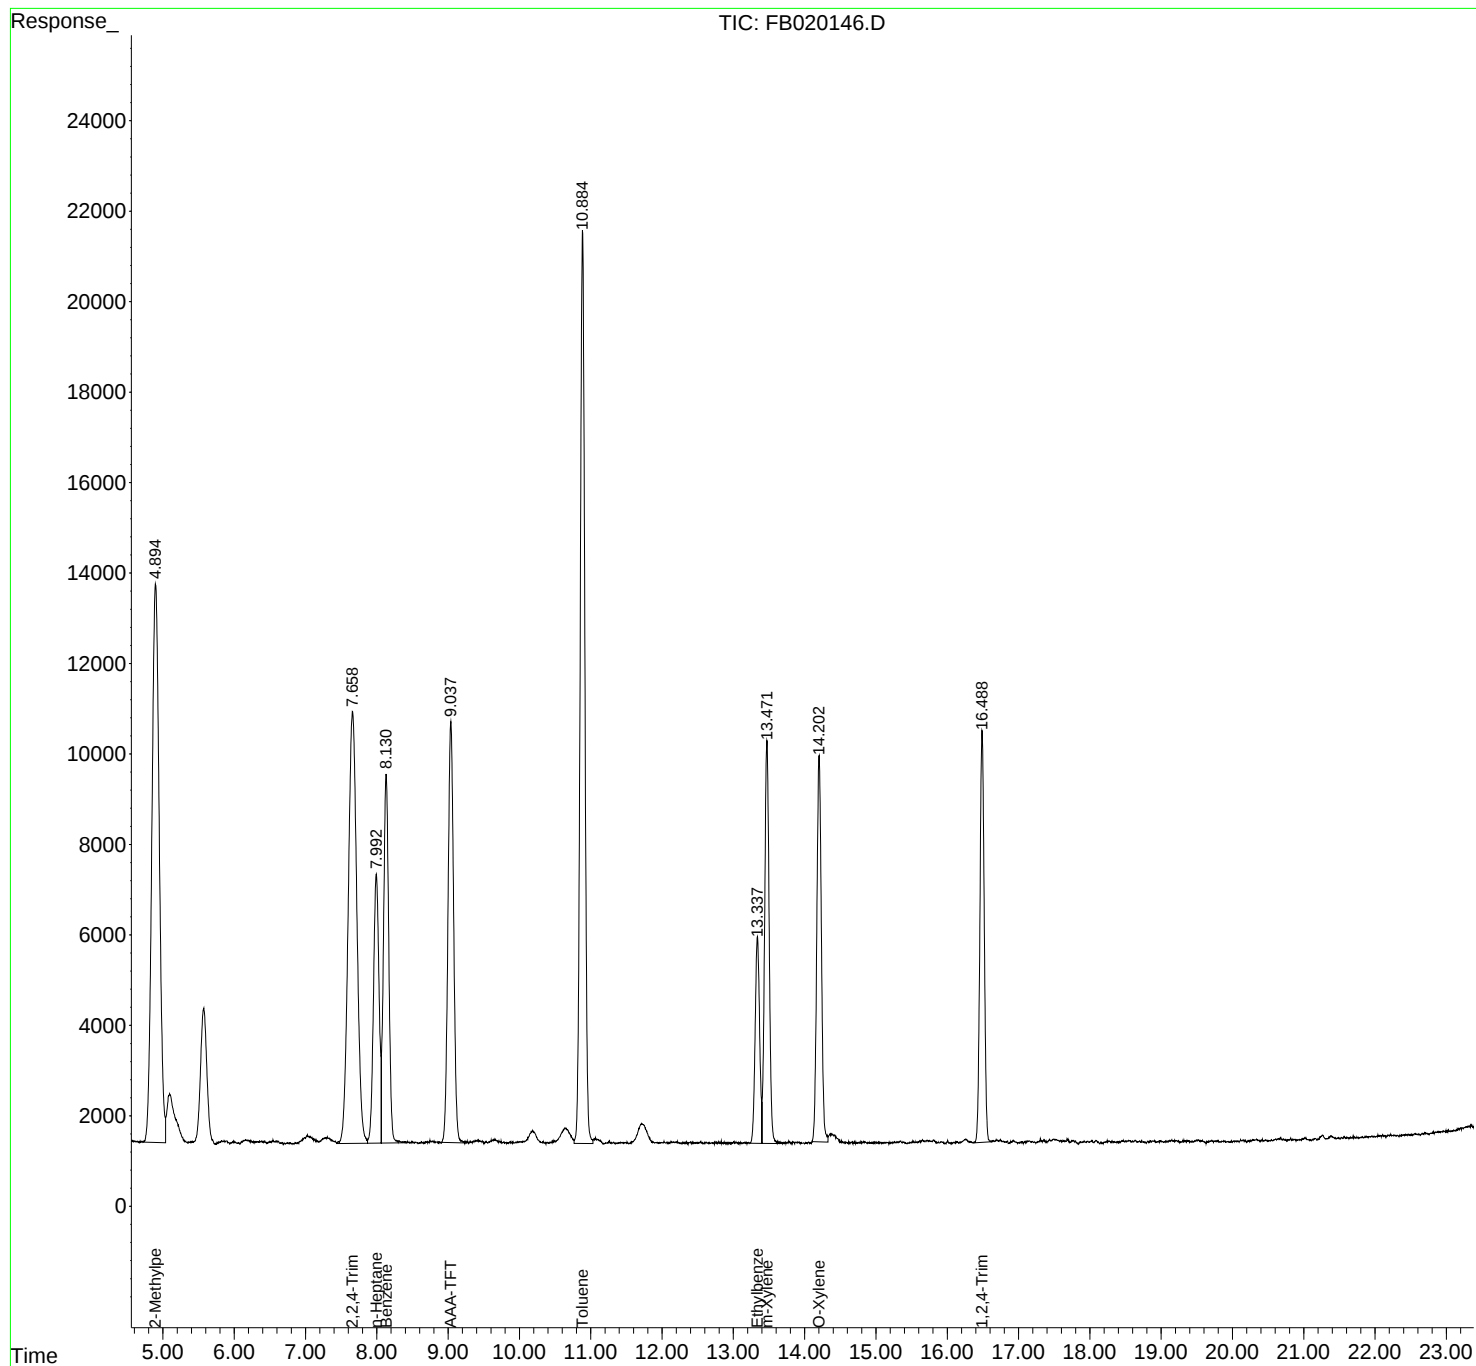


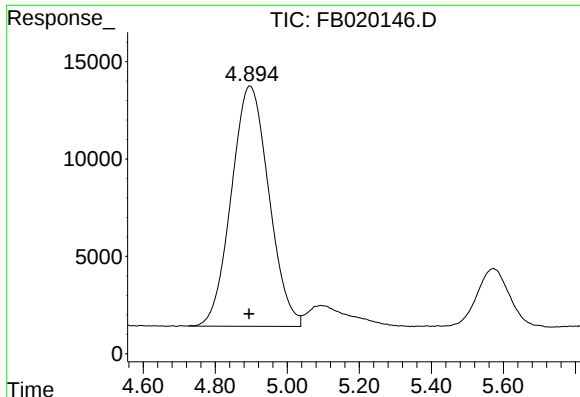

#1 2-Methylpentane


R.T.: 4.897 min
Delta R.T.: 0.003 min
Response: 891744
Conc: 26.44 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-1MSD

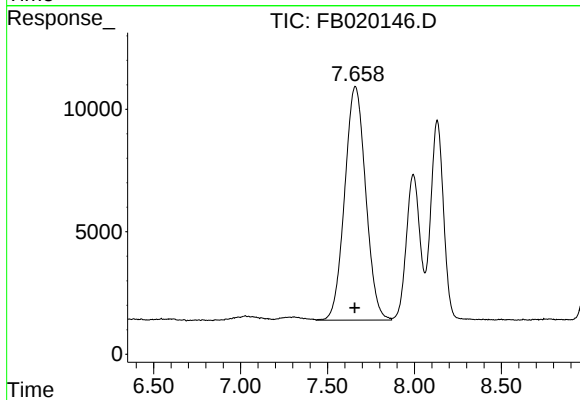


#2 2,2,4-Trimethylpentane

R.T.: 7.660 min
Delta R.T.: 0.003 min
Response: 800122
Conc: 24.40 ng/ml

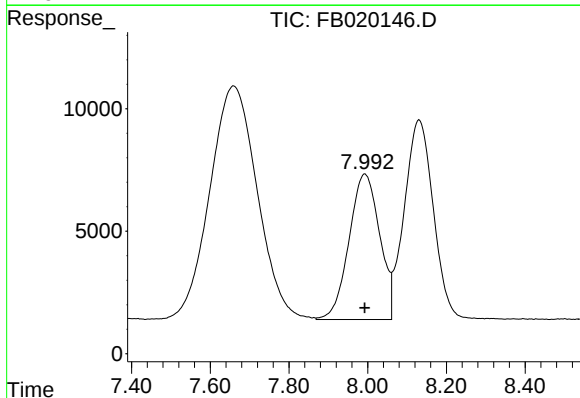


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 320677
Conc: 7.71 ng/ml

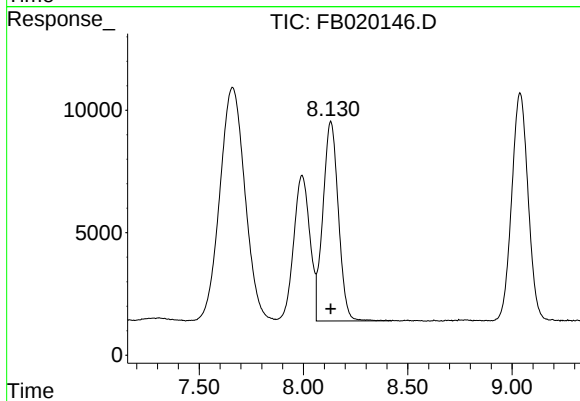

#4 Benzene


R.T.: 8.131 min
Delta R.T.: 0.000 min
Response: 420262
Conc: 9.03 ng/ml

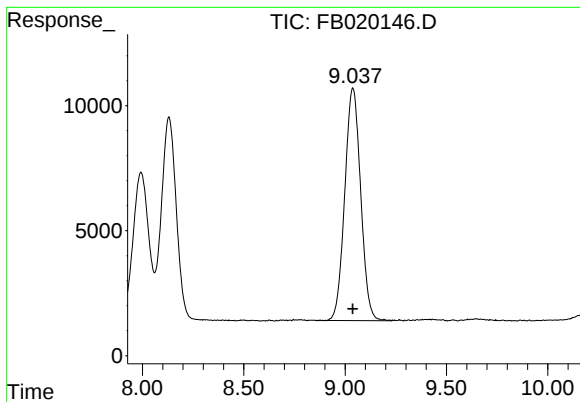

#5 AAA-TFT


R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 507026
Conc: 19.31 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-1MSD

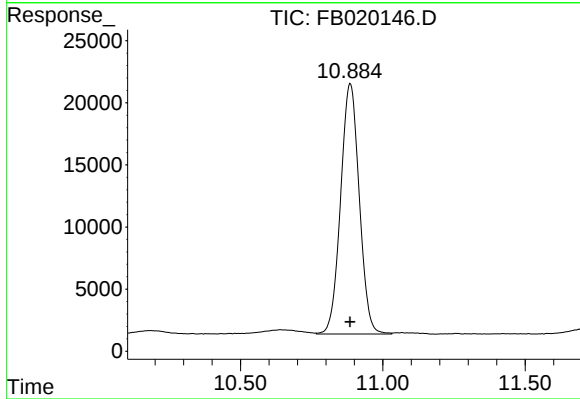


#6 Toluene

R.T.: 10.886 min
Delta R.T.: 0.000 min
Response: 917587
Conc: 24.83 ng/ml

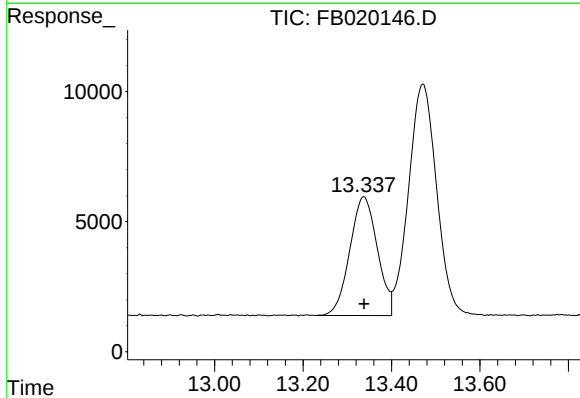


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: 0.000 min
Response: 196842
Conc: 8.37 ng/ml

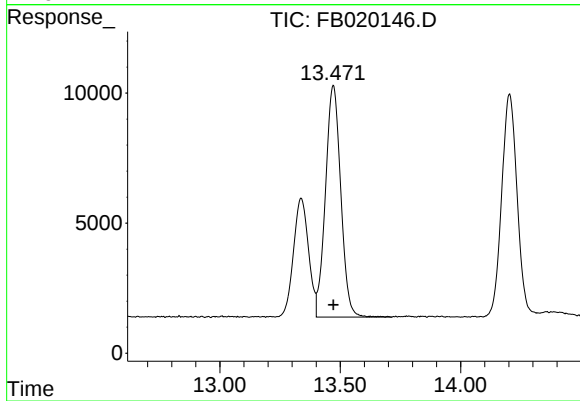

#8 m-Xylene


R.T.: 13.472 min
Delta R.T.: 0.000 min
Response: 394573
Conc: 18.50 ng/ml

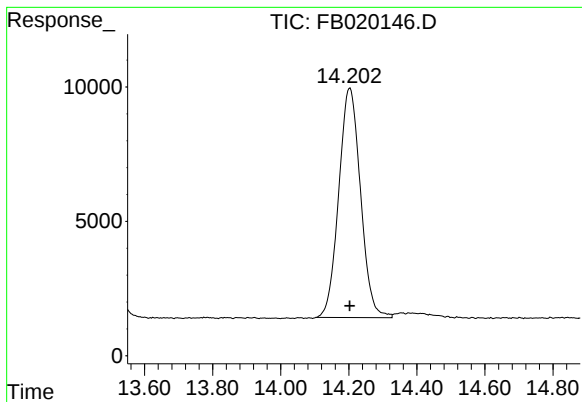

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: 0.000 min
Response: 378753
Conc: 19.99 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-3-1MSD

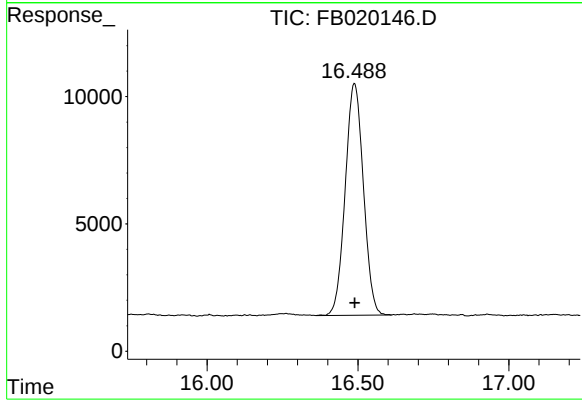

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: 0.000 min
Response: 380988
Conc: 19.21 ng/ml