

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031120\
 Data File : FB023883.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2020 1:36
 Operator : DD/AJ
 Sample : L1893-23
 Misc : 5.07g/5.00ml DI WATER
 ALS Vial : 26 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 12 02:22:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.859	10646169	505.740 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	2587144	83.713 ng/ml
2) t 2,2,4-Trimethylpentane	7.370	4124943	122.326 ng/ml
3) t n-Heptane	7.762	7399993	223.366 ng/ml
6) t Toluene	10.643	784726	19.246 ng/ml
7) t Ethylbenzene	13.057	3371545	88.245 ng/ml
8) t m-Xylene	13.199	1738105	47.209 ng/ml
9) t O-Xylene	13.932	550296	15.473 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	1340095	44.234 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031120\
Data File : FB023883.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2020 1:36
Operator : DD/AJ
Sample : L1893-23
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 26 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 12 02:22:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

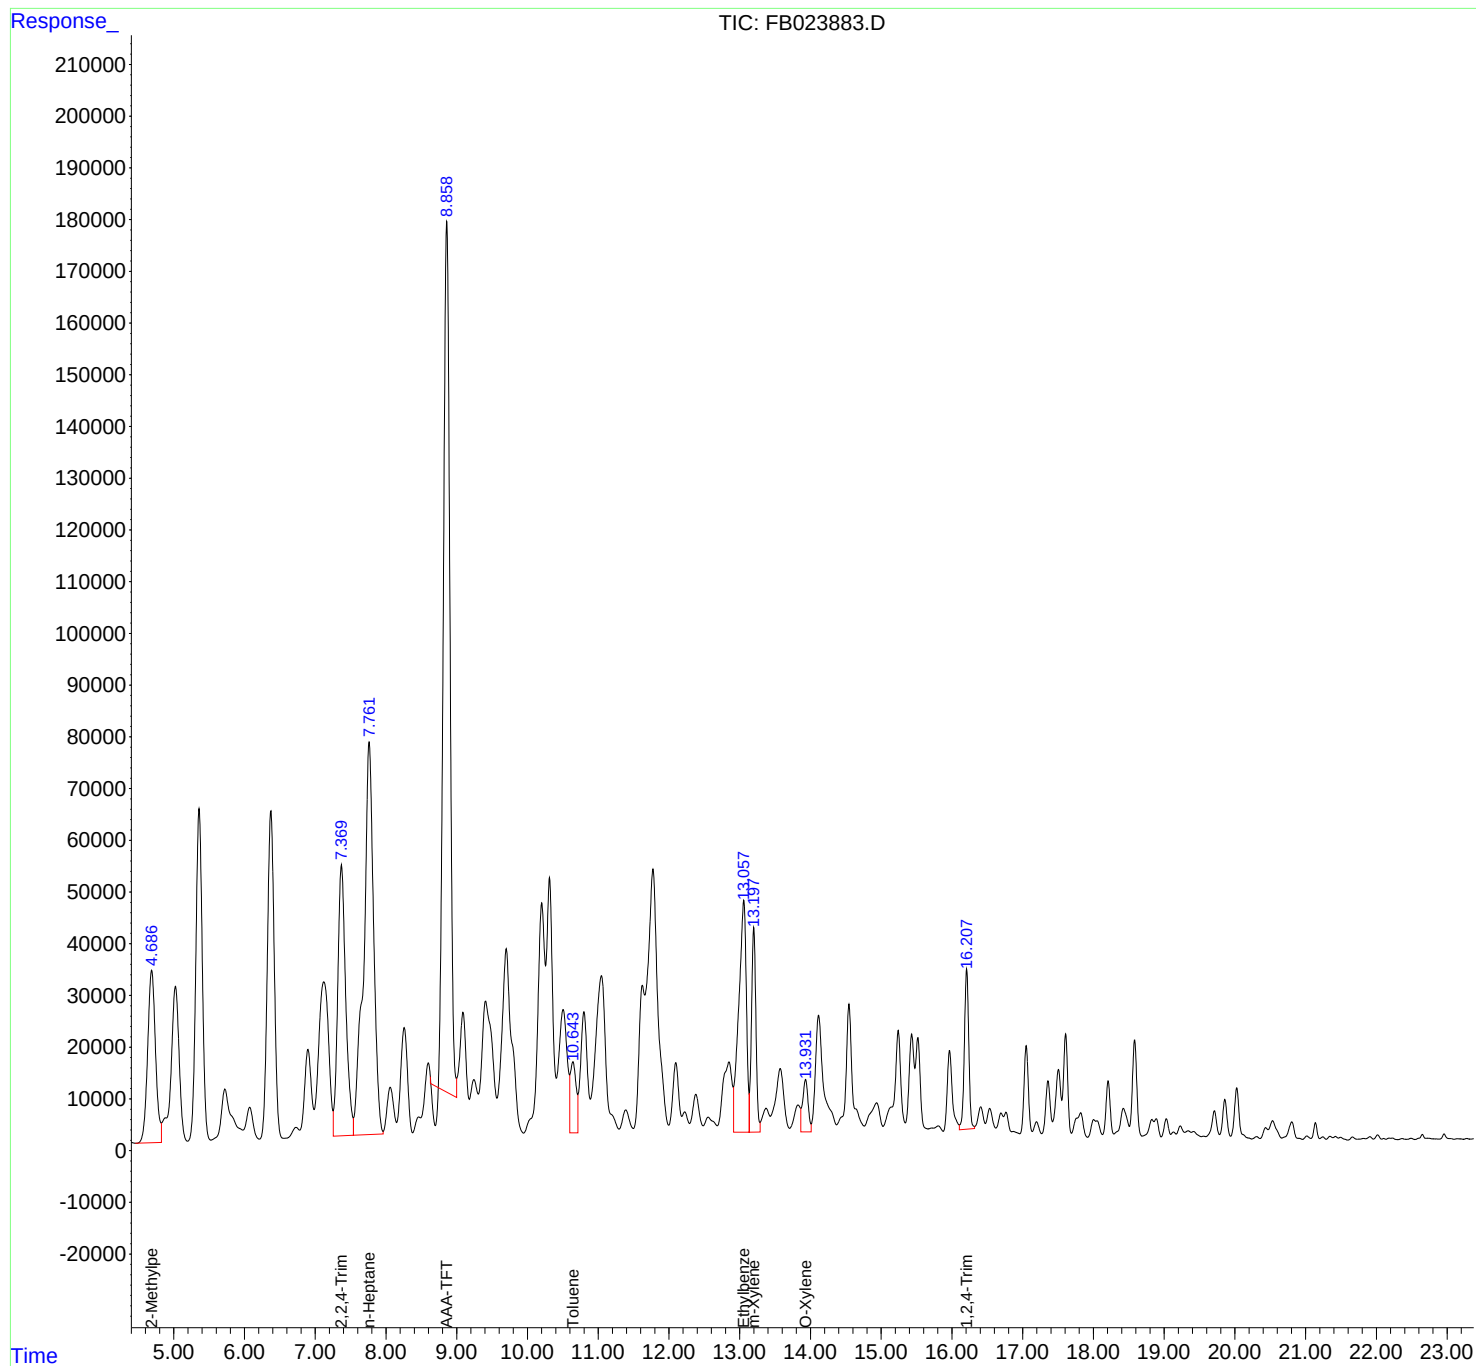

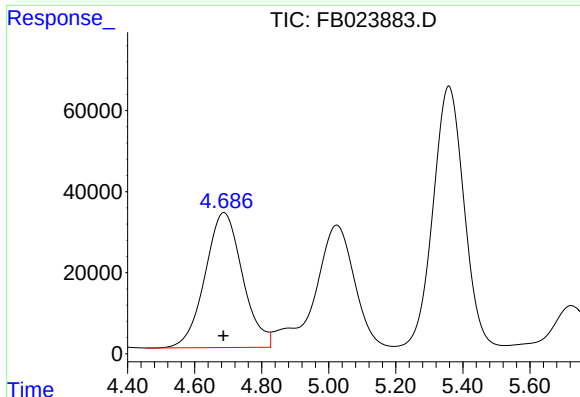


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.002 min
Response: 2587144
Conc: 83.71 ng/ml

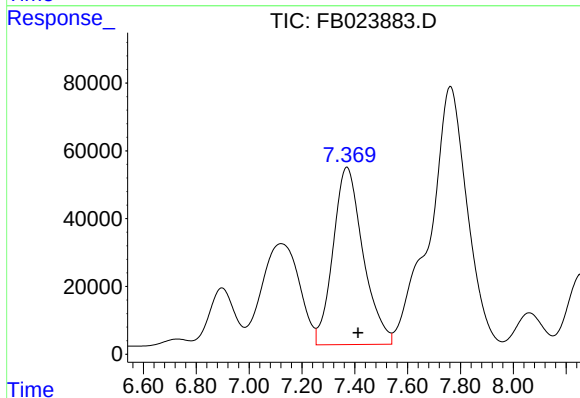


#2 2,2,4-Trimethylpentane

R.T.: 7.370 min
Delta R.T.: -0.042 min
Response: 4124943
Conc: 122.33 ng/ml

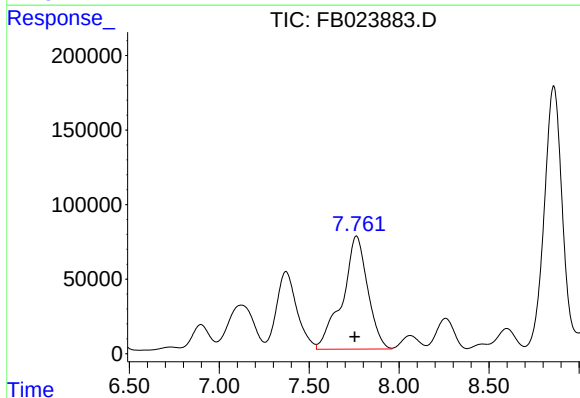


#3 n-Heptane

R.T.: 7.762 min
Delta R.T.: 0.009 min
Response: 7399993
Conc: 223.37 ng/ml

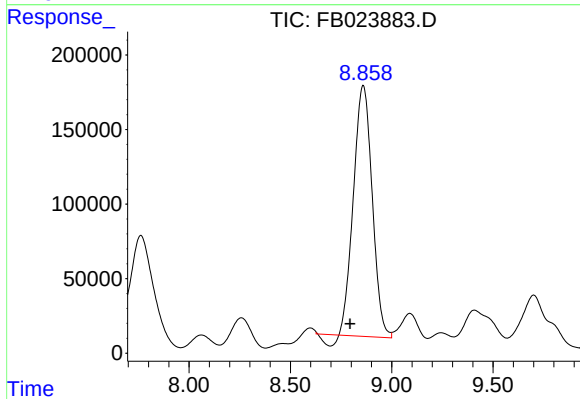


#5 AAA-TFT

R.T.: 8.859 min
Delta R.T.: 0.065 min
Response: 10646169
Conc: 505.74 ng/ml

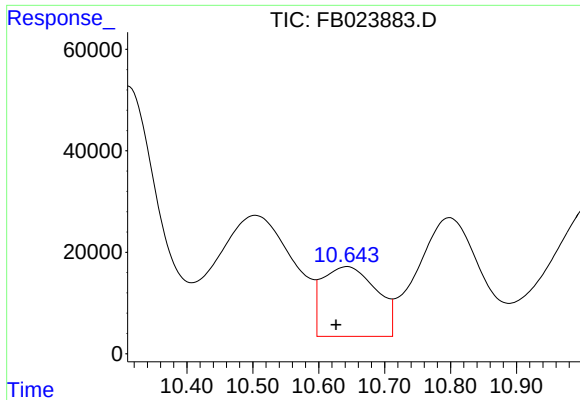


#6 Toluene

R.T.: 10.643 min
Delta R.T.: 0.016 min
Response: 784726
Conc: 19.25 ng/ml

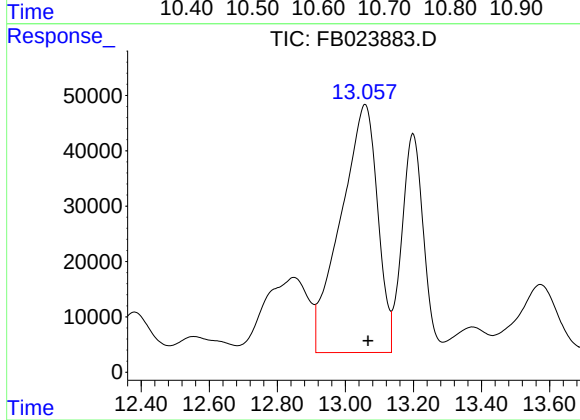


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.010 min
Response: 3371545
Conc: 88.25 ng/ml

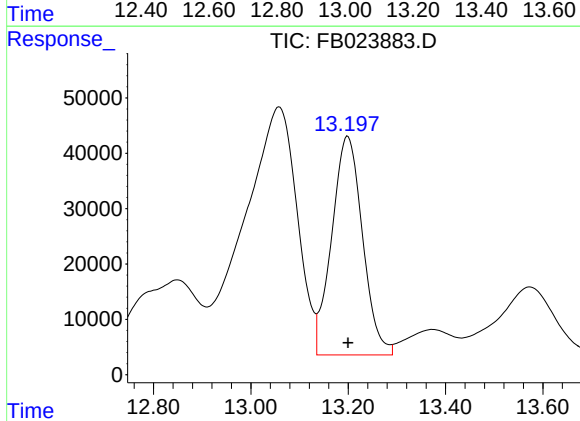


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: 0.000 min
Response: 1738105
Conc: 47.21 ng/ml

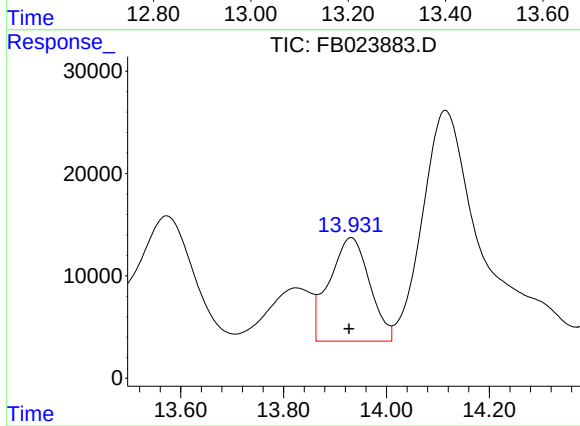

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.004 min
Response: 550296
Conc: 15.47 ng/ml

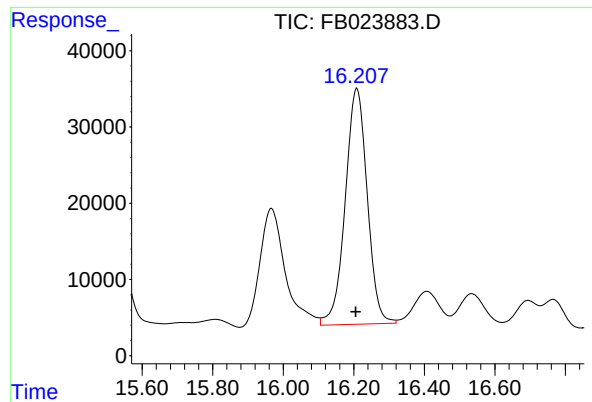

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.003 min
Response: 1340095
Conc: 44.23 ng/ml