

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031120\
 Data File : FB023876.D
 Signal(s) : FID2B.CH
 Acq On : 11 Mar 2020 21:31
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 12 01:47:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
 Quant Title :
 QLast Update : Thu Mar 05 11:03:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	388454	18.453 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	820339	26.544 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	878284	26.046 ng/ml
3) t n-Heptane	7.758	287500	8.678 ng/ml
4) t Benzene	7.892	394272	9.416 ng/ml
6) t Toluene	10.631	1143701	28.050 ng/ml
7) t Ethylbenzene	13.071	354654	9.283 ng/ml
8) t m-Xylene	13.204	686243	18.639 ng/ml
9) t O-Xylene	13.932	664293	18.678 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	583684	19.266 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031120\
Data File : FB023876.D
Signal(s) : FID2B.CH
Acq On : 11 Mar 2020 21:31
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 18 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 12 01:47:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030520.M
Quant Title :
QLast Update : Thu Mar 05 11:03:12 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

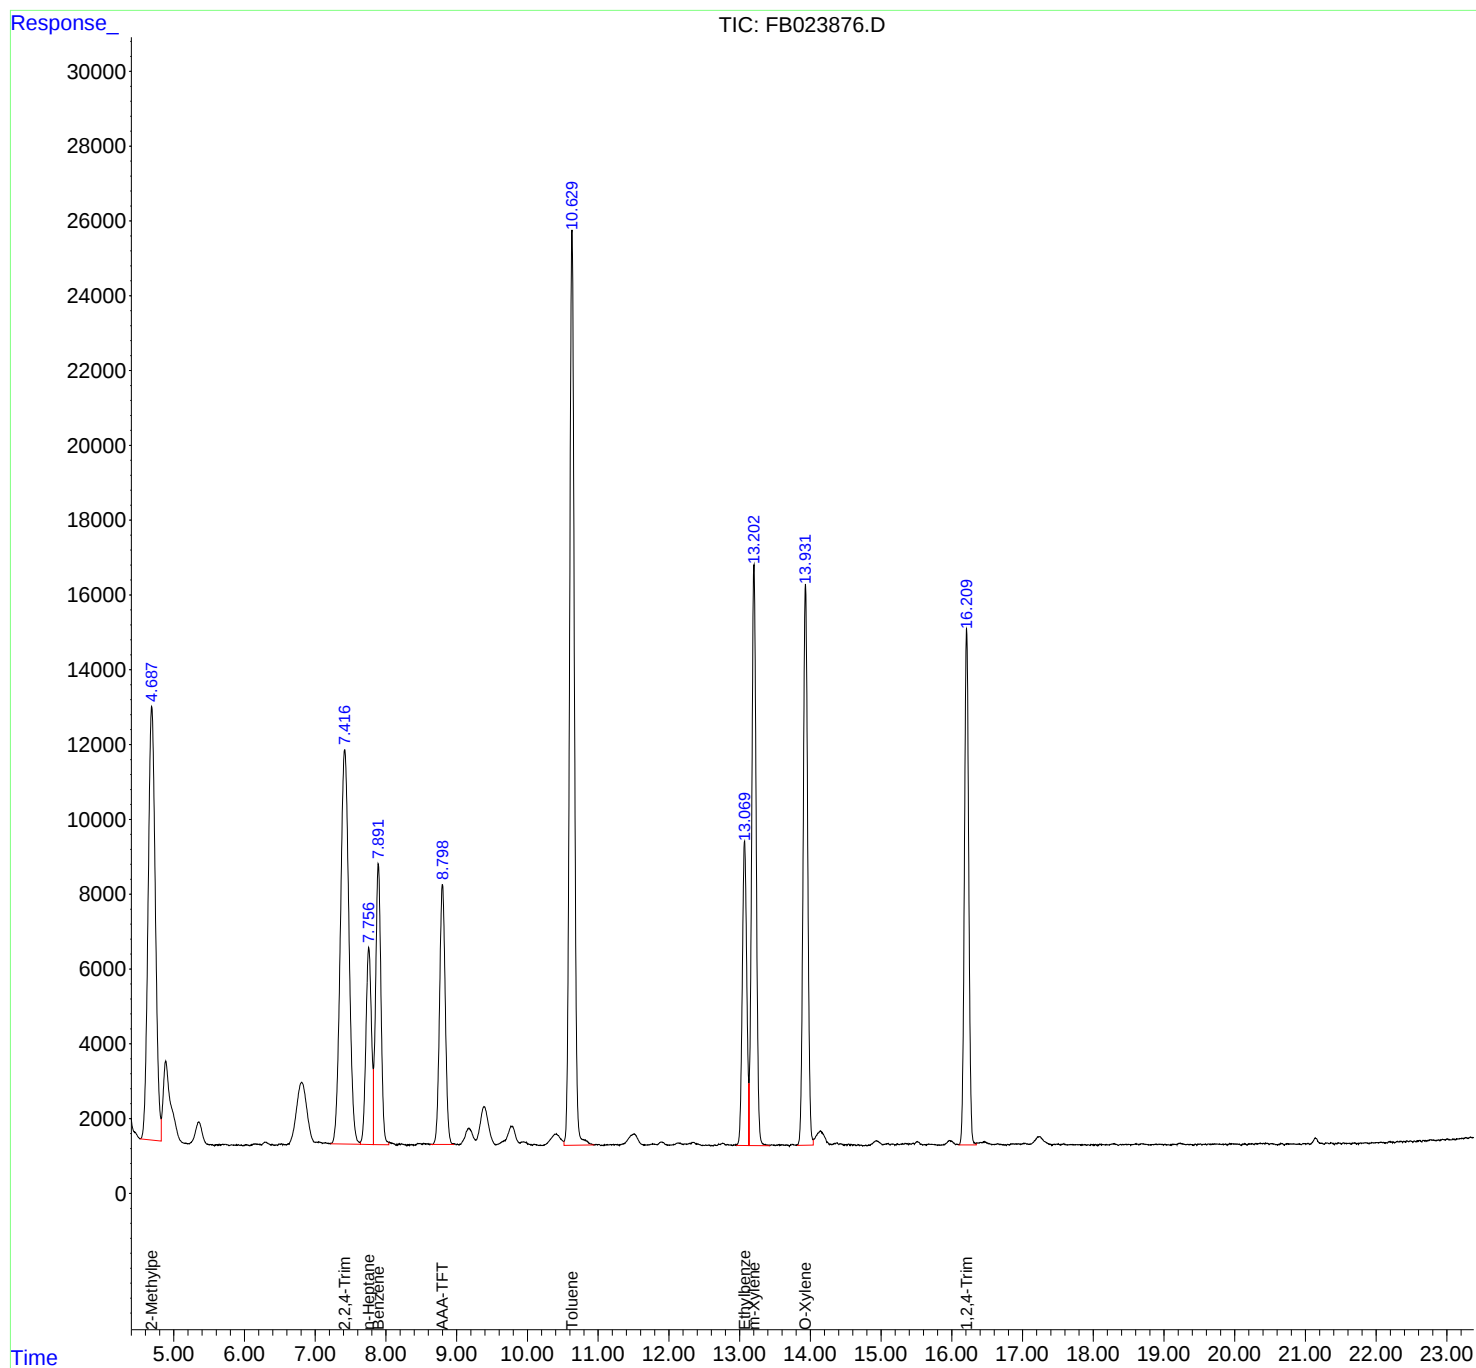

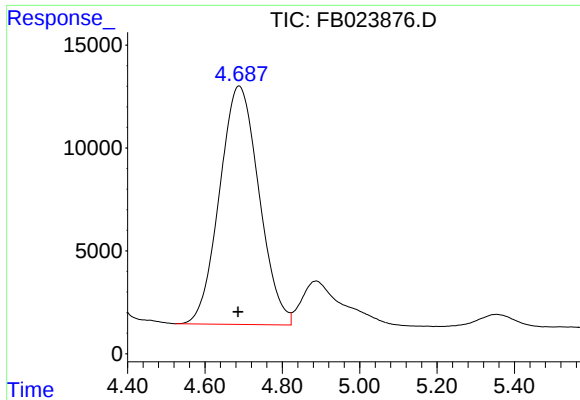


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.003 min
Response: 820339
Conc: 26.54 ng/ml

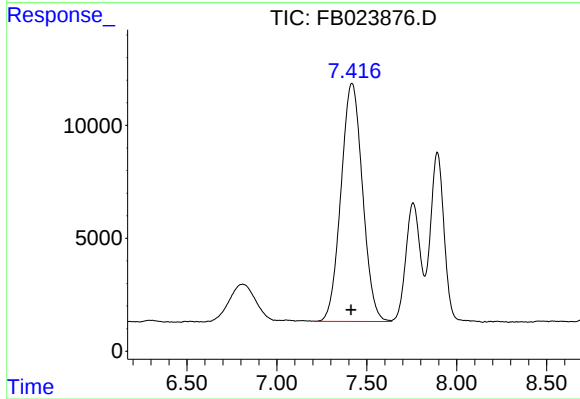


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.005 min
Response: 878284
Conc: 26.05 ng/ml

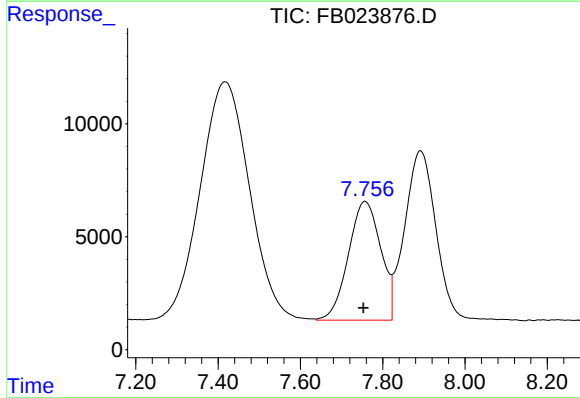


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.004 min
Response: 287500
Conc: 8.68 ng/ml

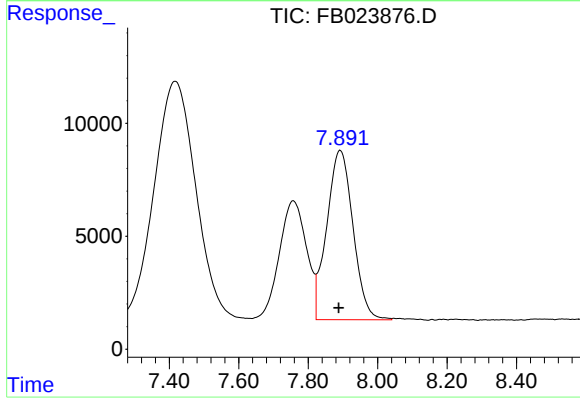


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.004 min
Response: 394272
Conc: 9.42 ng/ml

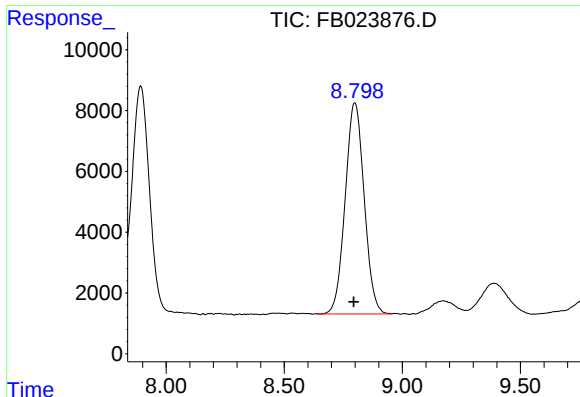


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.005 min
Response: 388454
Conc: 18.45 ng/ml

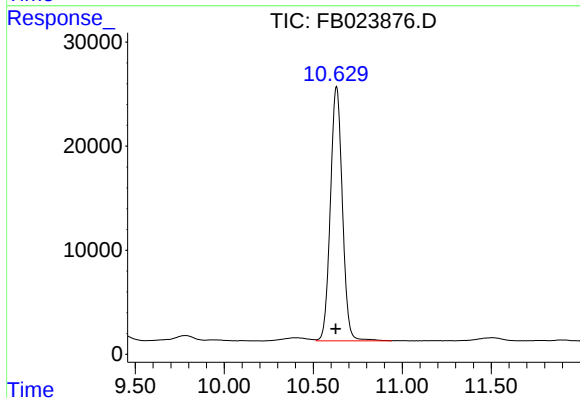


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.005 min
Response: 1143701
Conc: 28.05 ng/ml

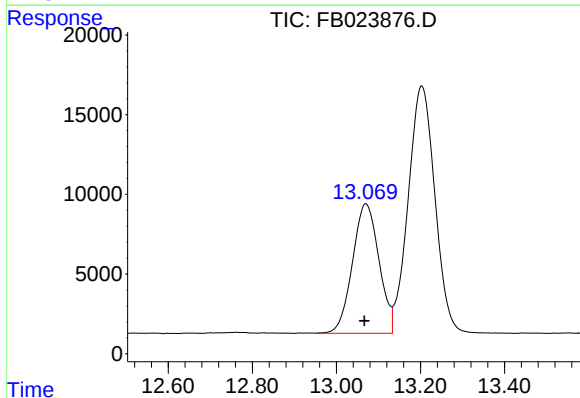


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.004 min
Response: 354654
Conc: 9.28 ng/ml

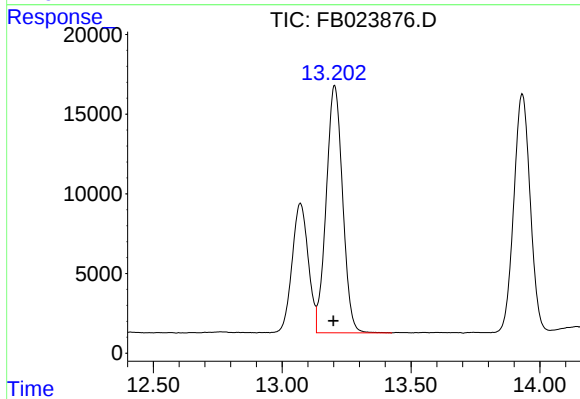

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.004 min
Response: 686243
Conc: 18.64 ng/ml

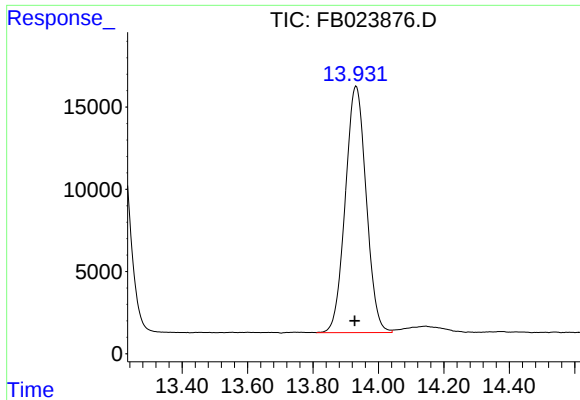


#9 O-Xylene

R.T.: 13.932 min

Delta R.T.: 0.004 min

Response: 664293

Conc: 18.68 ng/ml

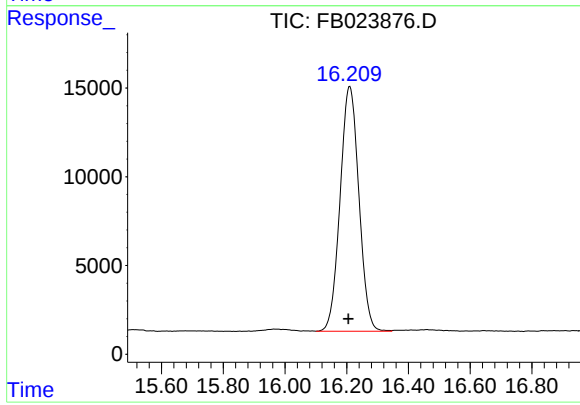

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min

Delta R.T.: 0.004 min

Response: 583684

Conc: 19.27 ng/ml