

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031124\
 Data File : FB030612.D
 Signal(s) : FID2B.CH
 Acq On : 11 Mar 2024 8:04
 Operator : YP/AJ
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 10 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 11 10:03:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
 Quant Title :
 QLast Update : Mon Mar 11 09:44:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	124078	9.730 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	269342	13.608 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	260630	13.152 ng/ml
3) t n-Heptane	7.746	98165	4.271 ng/ml
4) t Benzene	7.881	109346	4.450 ng/ml
6) t Toluene	10.615	314786	13.244 ng/ml
7) t Ethylbenzene	13.052	96932	4.454 ng/ml
8) t m-Xylene	13.184	196466	8.987 ng/ml
9) t O-Xylene	13.911	187290	8.362 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	188250	8.028 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031124\
Data File : FB030612.D
Signal(s) : FID2B.CH
Acq On : 11 Mar 2024 8:04
Operator : YP/AJ
Sample : 10 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
10 GRO STD

Integration File: Calibration.e
Quant Time: Mar 11 10:03:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
Quant Title :
QLast Update : Mon Mar 11 09:44:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

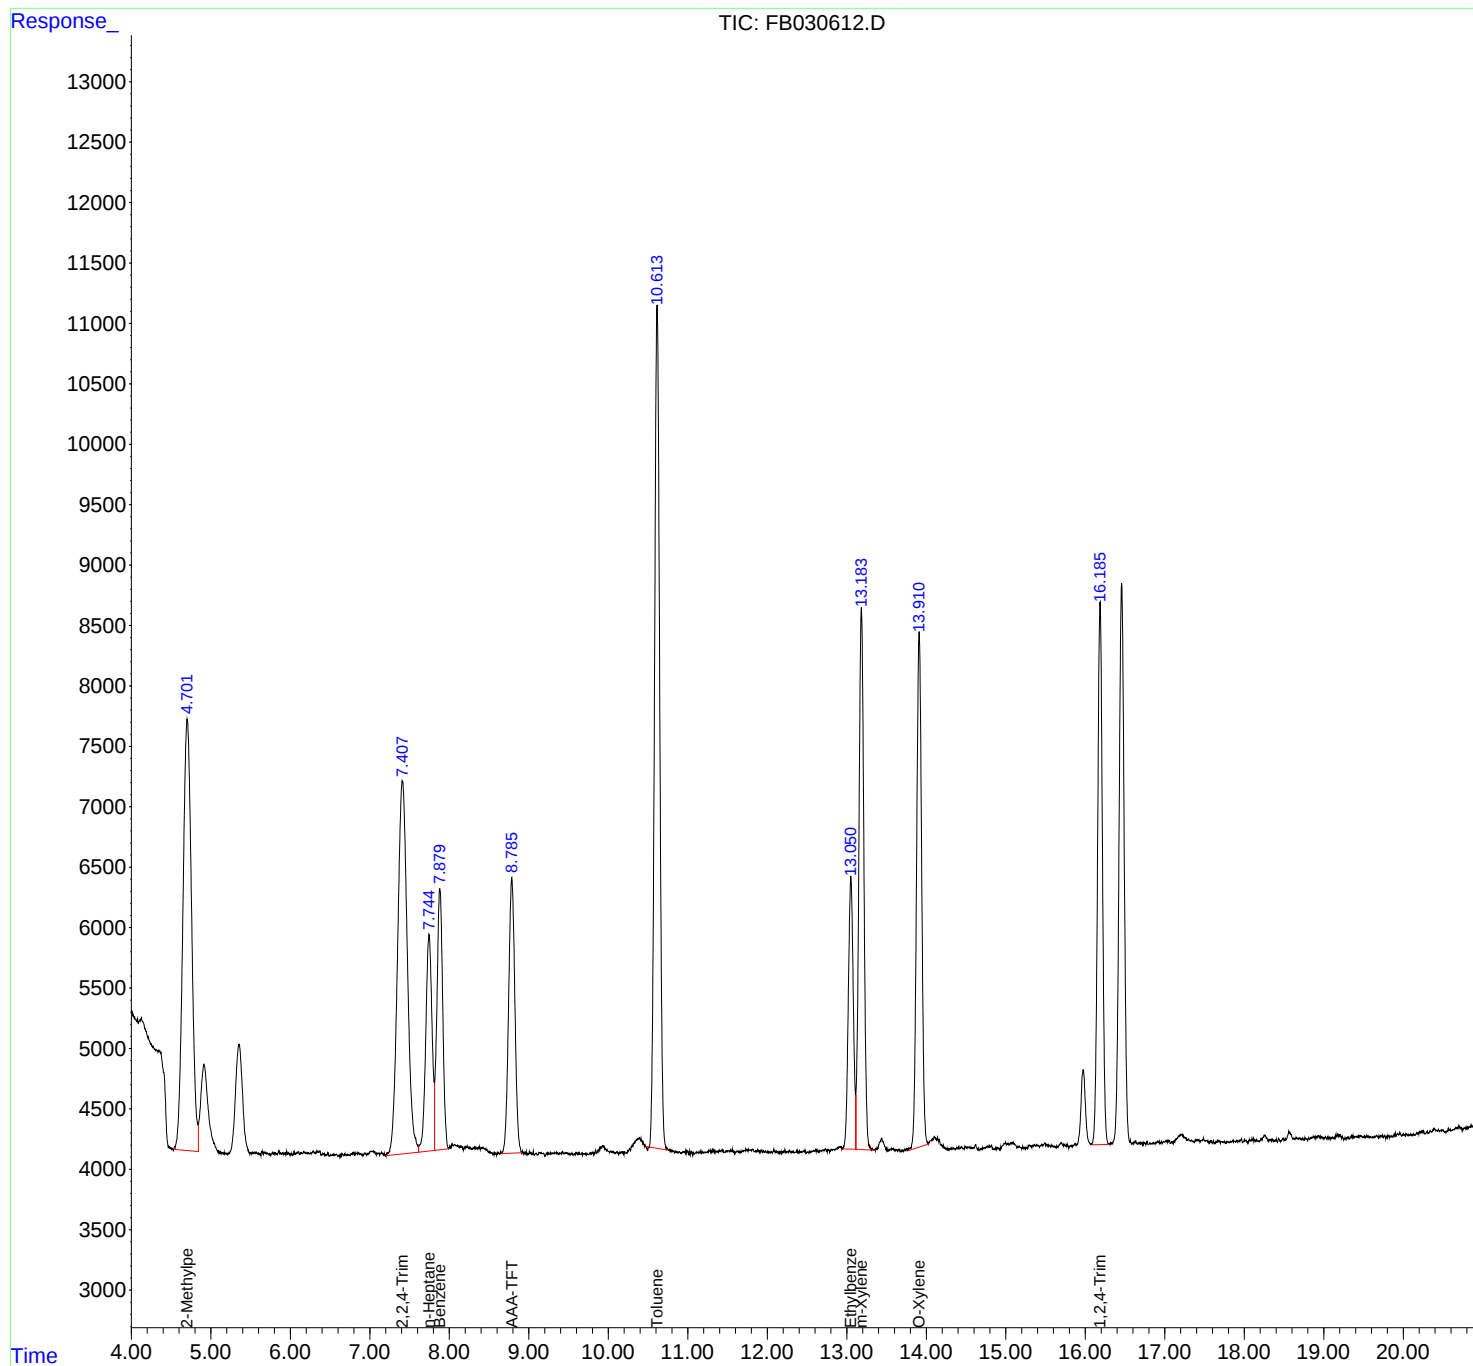


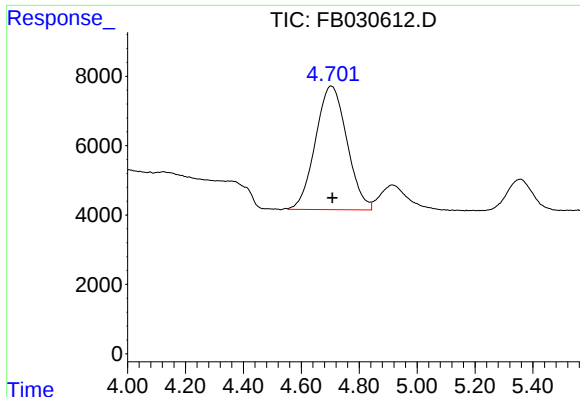

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.005 min
Response: 269342
Conc: 13.61 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

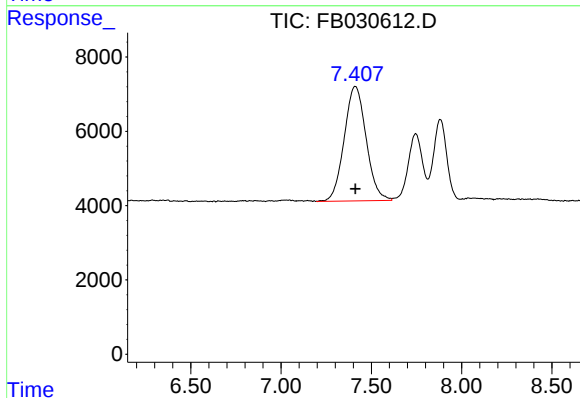


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.003 min
Response: 260630
Conc: 13.15 ng/ml

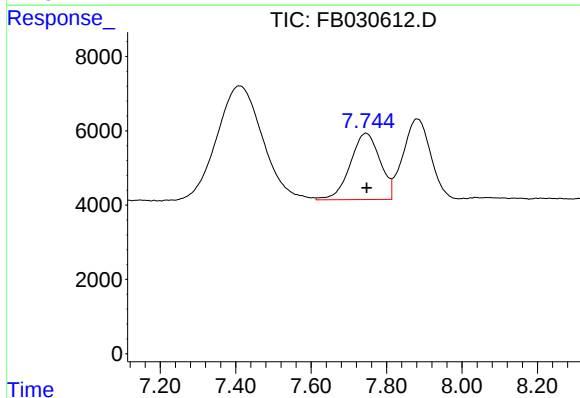


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.001 min
Response: 98165
Conc: 4.27 ng/ml

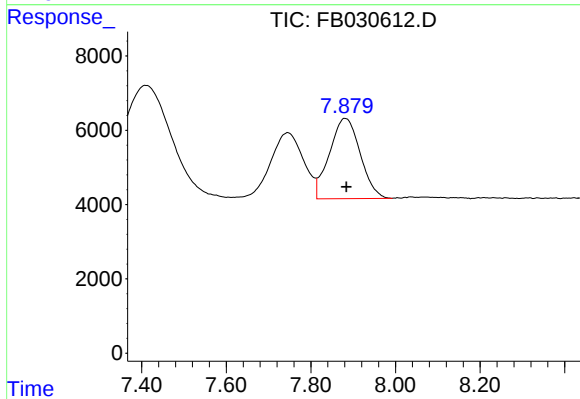

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.003 min
Response: 109346
Conc: 4.45 ng/ml

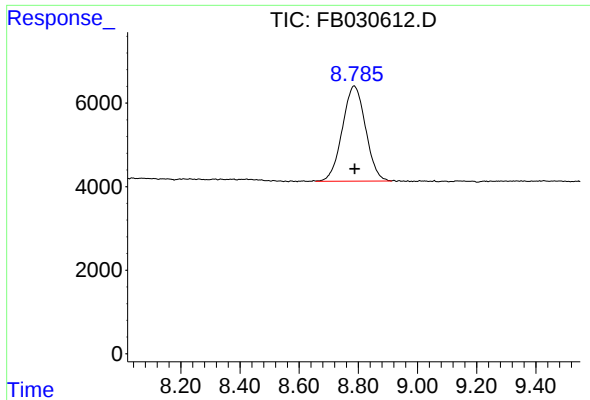

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.002 min
Response: 124078
Conc: 9.73 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

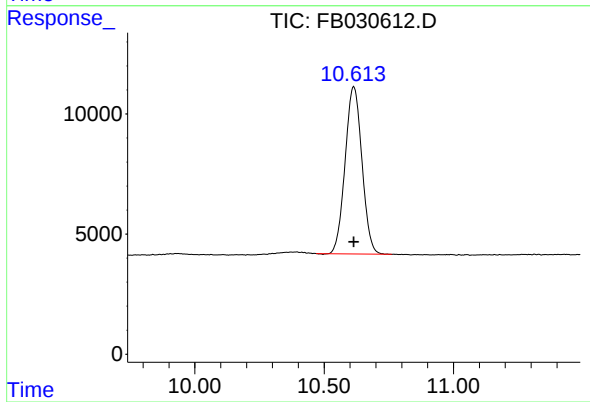


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.000 min
Response: 314786
Conc: 13.24 ng/ml

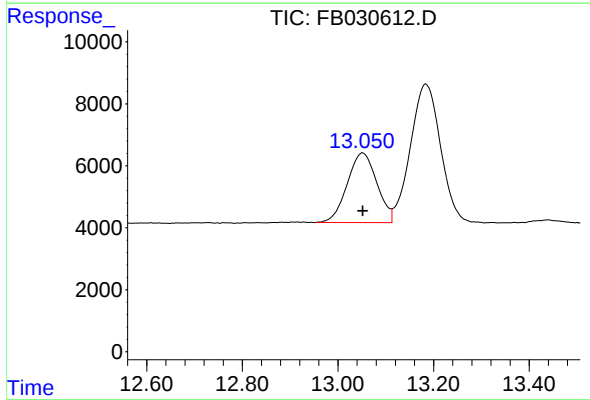


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.000 min
Response: 96932
Conc: 4.45 ng/ml

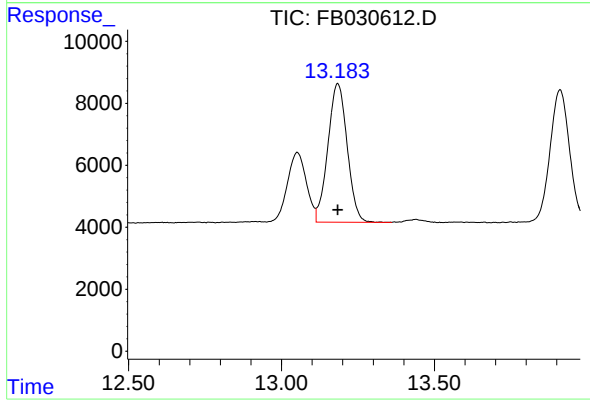

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.000 min
Response: 196466
Conc: 8.99 ng/ml

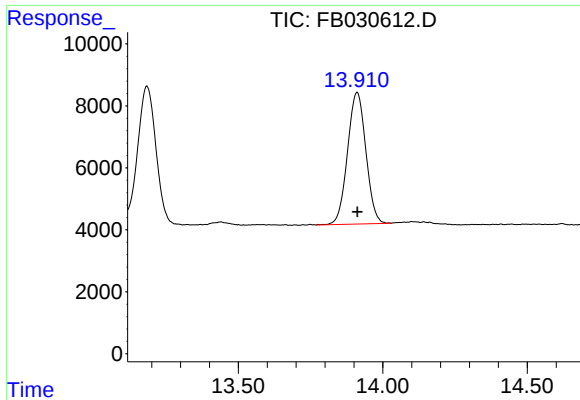

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.000 min
Response: 187290
Conc: 8.36 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

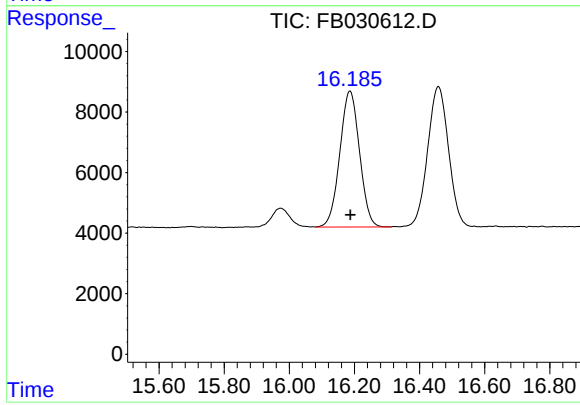

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 188250
Conc: 8.03 ng/ml