

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031124\
 Data File : FB030613.D
 Signal(s) : FID2B.CH
 Acq On : 11 Mar 2024 8:42
 Operator : YP/AJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 11 09:45:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
 Quant Title :
 QLast Update : Mon Mar 11 09:44:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	237284	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	612359	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	580268	30.000 ng/ml
3) t n-Heptane	7.747	225585	10.000 ng/ml
4) t Benzene	7.884	252568	10.000 ng/ml
6) t Toluene	10.615	734871	30.000 ng/ml
7) t Ethylbenzene	13.052	223037	10.000 ng/ml
8) t m-Xylene	13.184	444167	20.000 ng/ml
9) t O-Xylene	13.912	422655	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	418756	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031124\
Data File : FB030613.D
Signal(s) : FID2B.CH
Acq On : 11 Mar 2024 8:42
Operator : YP/AJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Mar 11 09:45:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031124.M
Quant Title :
QLast Update : Mon Mar 11 09:44:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

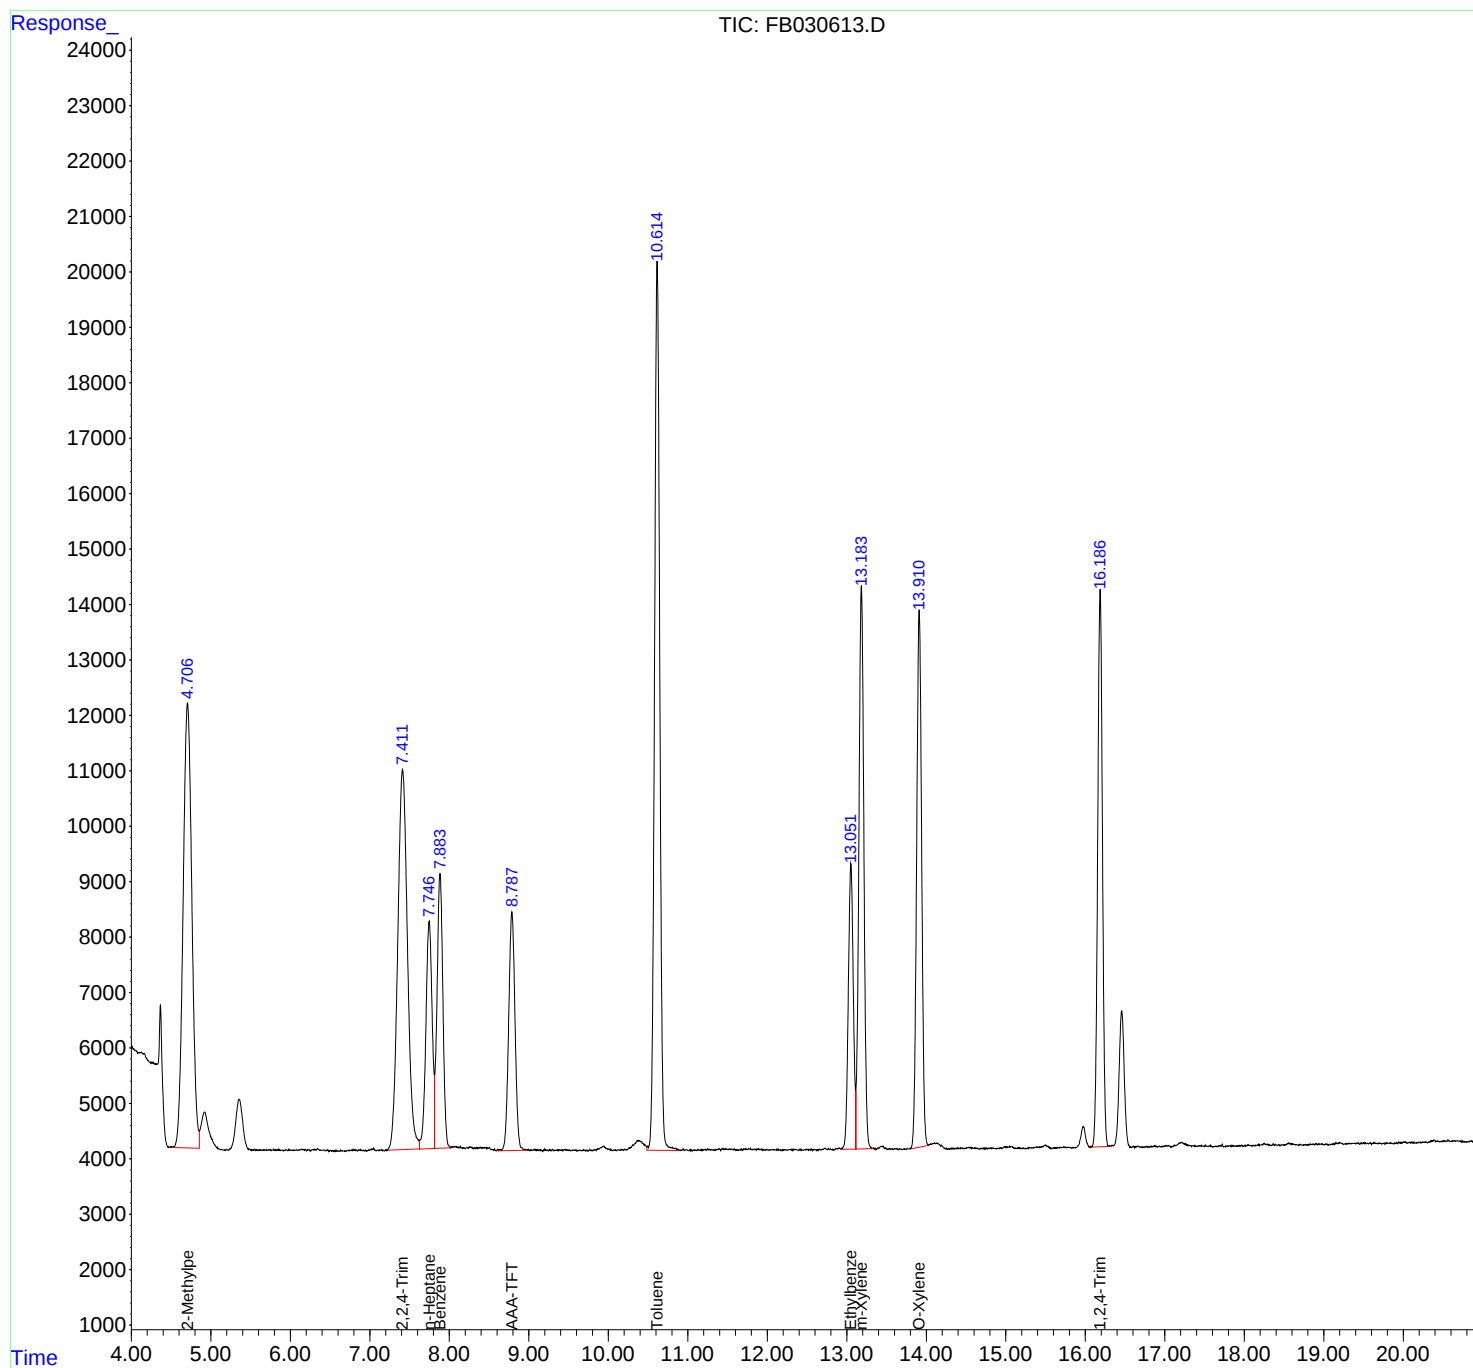


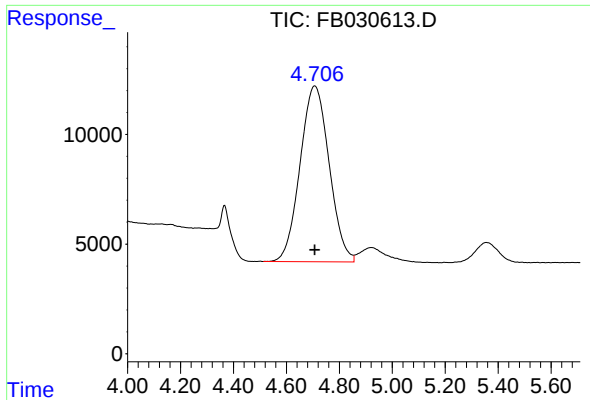

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 612359
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

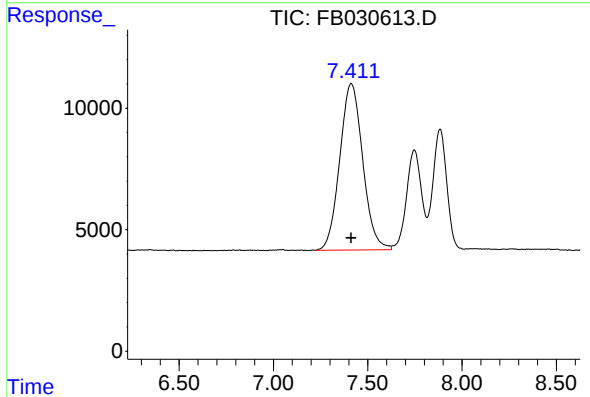


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 580268
Conc: 30.00 ng/ml

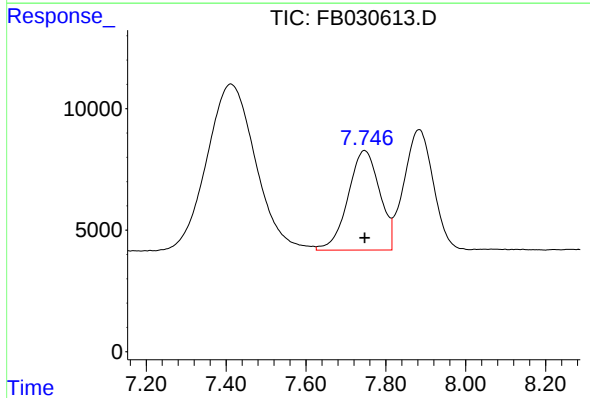


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 225585
Conc: 10.00 ng/ml

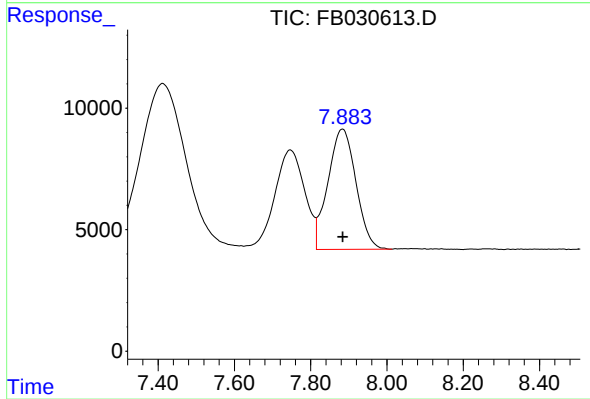

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 252568
Conc: 10.00 ng/ml

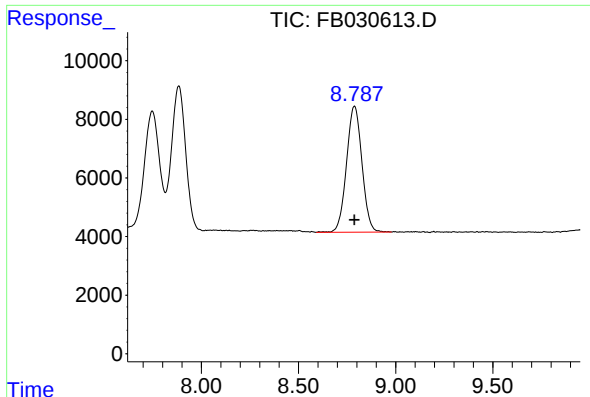

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 237284
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

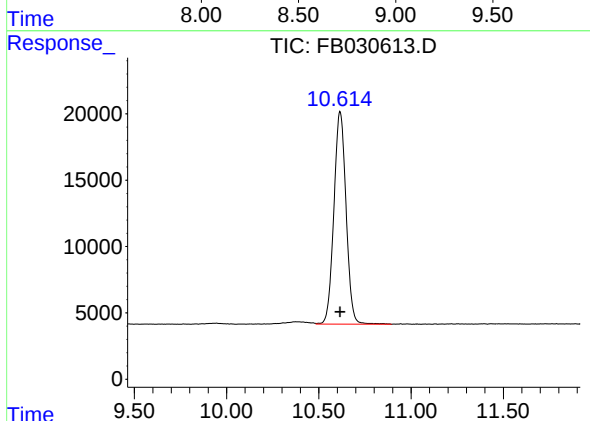


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.000 min
Response: 734871
Conc: 30.00 ng/ml

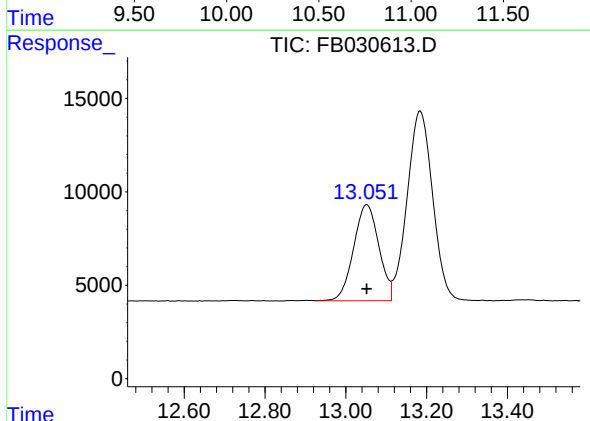


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.000 min
Response: 223037
Conc: 10.00 ng/ml

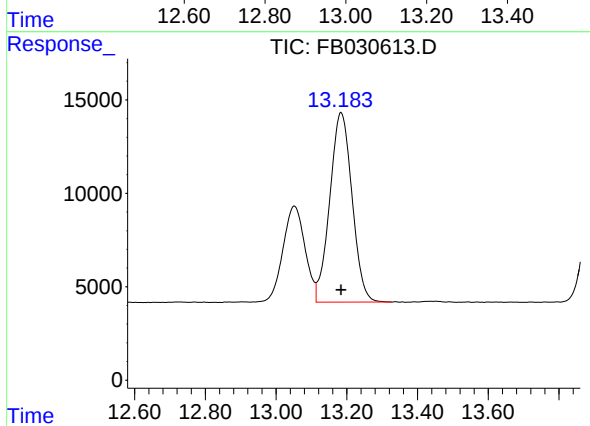

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.000 min
Response: 444167
Conc: 20.00 ng/ml

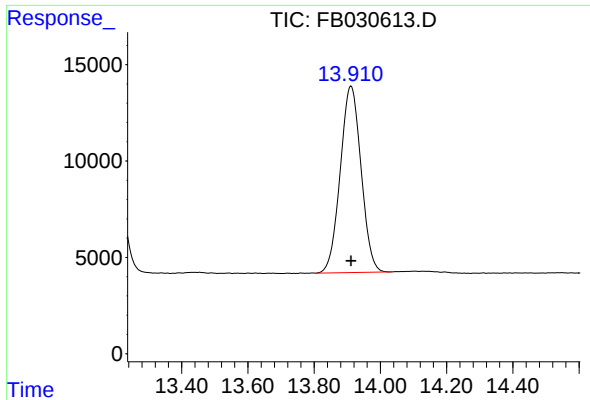

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.000 min
Response: 422655
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

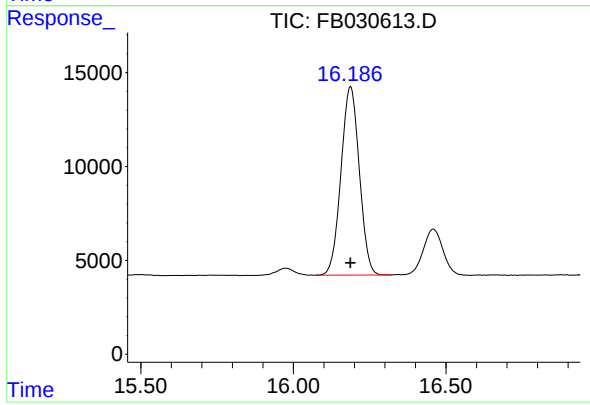

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 418756
Conc: 20.00 ng/ml