

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
 Data File : FB020150.D
 Signal(s) : FID2B.CH
 Acq On : 12 Mar 2019 10:03
 Operator : MJ/SJ
 Sample : BSF0312S1
 Misc : 5.02gm/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0312S1

Integration File: Calibration.e
 Quant Time: Mar 13 02:27:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
 Quant Title :
 QLast Update : Mon Mar 11 13:44:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	508906	19.385 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	1020443	30.250 ng/ml
2) t 2,2,4-Trimethylpentane	7.659	926741	28.259 ng/ml
3) t n-Heptane	7.993	417467	10.031 ng/ml
4) t Benzene	8.130	450568	9.678 ng/ml
6) t Toluene	10.885	1043968	28.251 ng/ml
7) t Ethylbenzene	13.338	221251	9.404 ng/ml
8) t m-Xylene	13.471	417011	19.549 ng/ml
9) t O-Xylene	14.203	392955	20.744 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	417562	21.055 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031219\
Data File : FB020150.D
Signal(s) : FID2B.CH
Acq On : 12 Mar 2019 10:03
Operator : MJ/SJ
Sample : BSF0312S1
Misc : 5.02gm/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0312S1

Integration File: Calibration.e
Quant Time: Mar 13 02:27:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031119.M
Quant Title :
QLast Update : Mon Mar 11 13:44:46 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

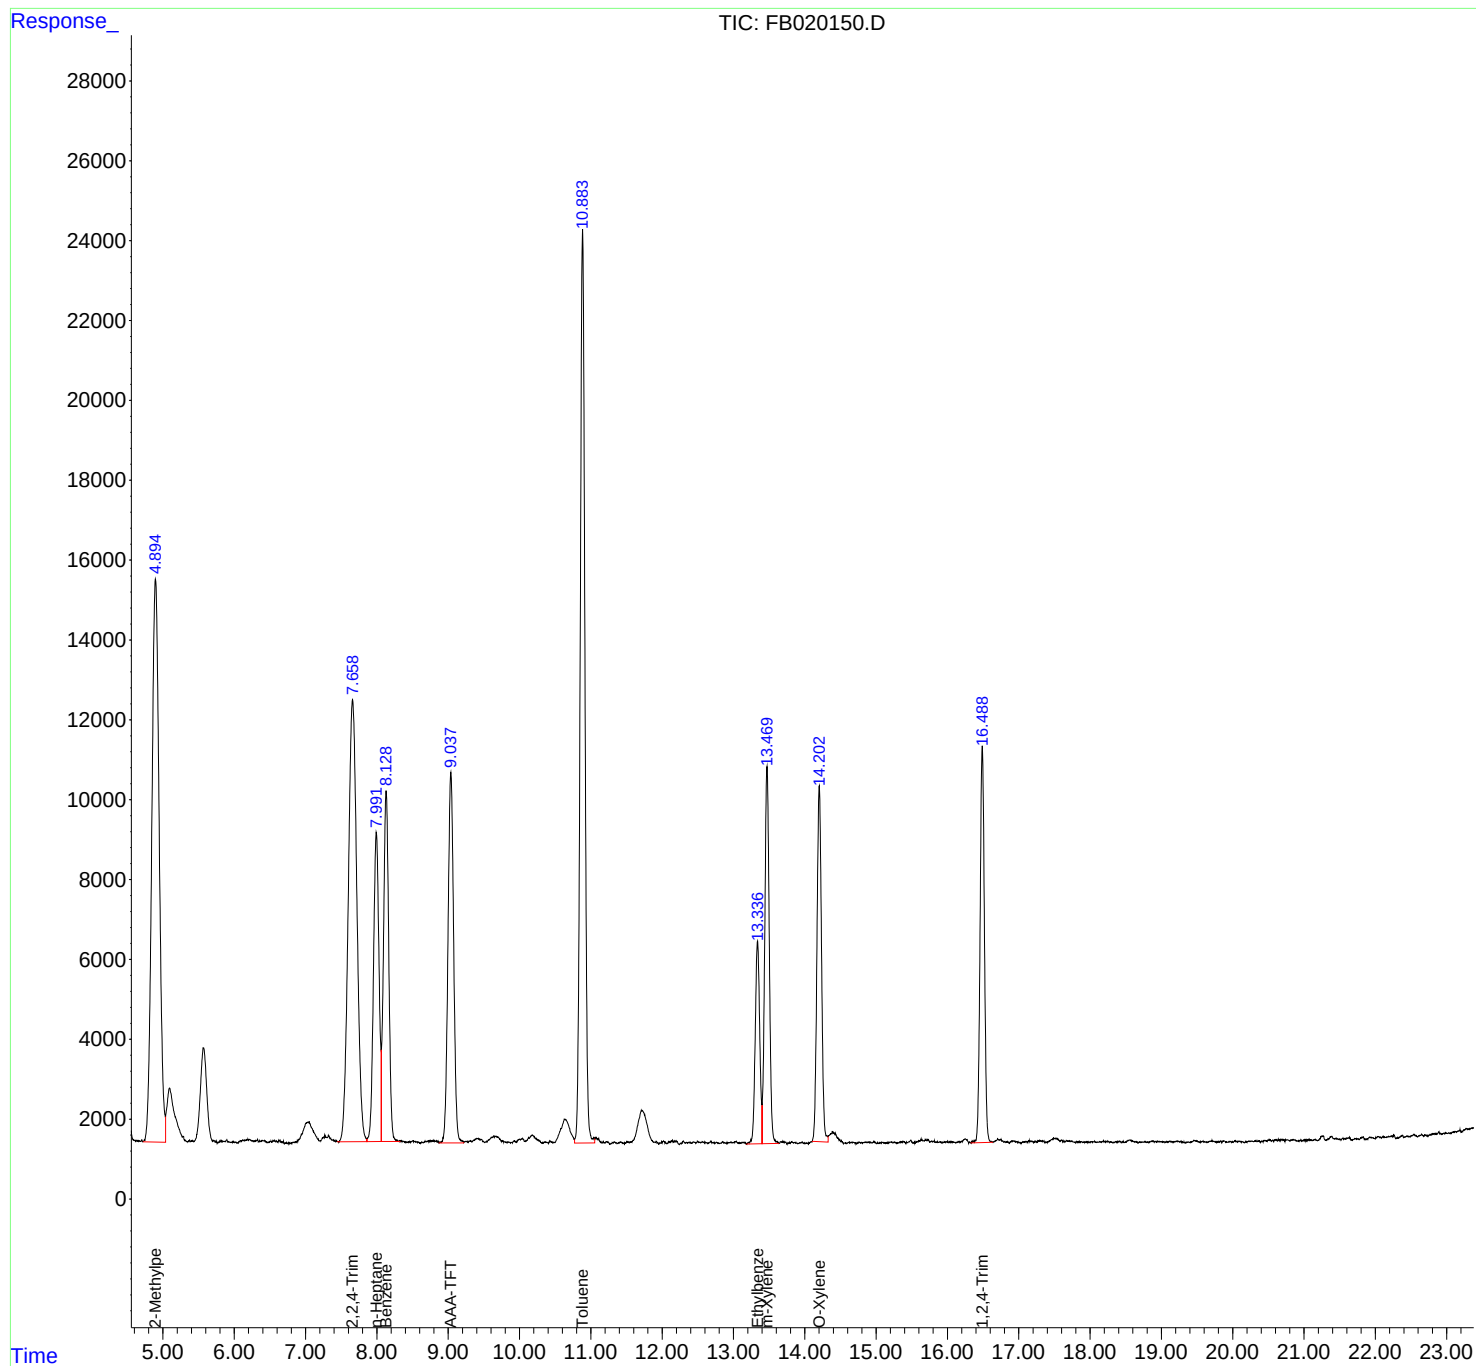


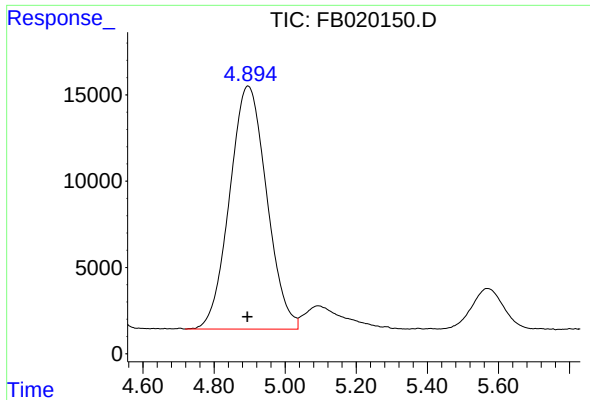

#1 2-Methylpentane


R.T.: 4.896 min
Delta R.T.: 0.002 min
Response: 1020443
Conc: 30.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0312S1

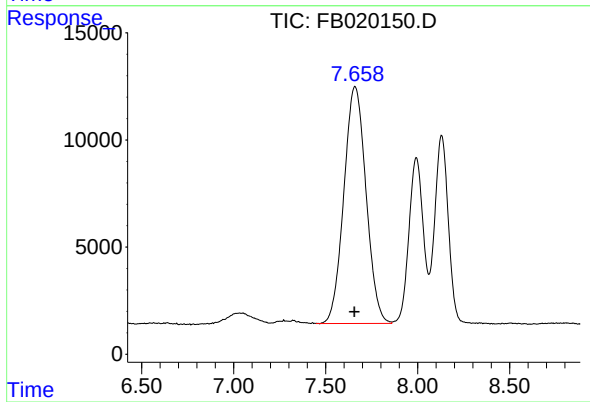


#2 2,2,4-Trimethylpentane

R.T.: 7.659 min
Delta R.T.: 0.002 min
Response: 926741
Conc: 28.26 ng/ml

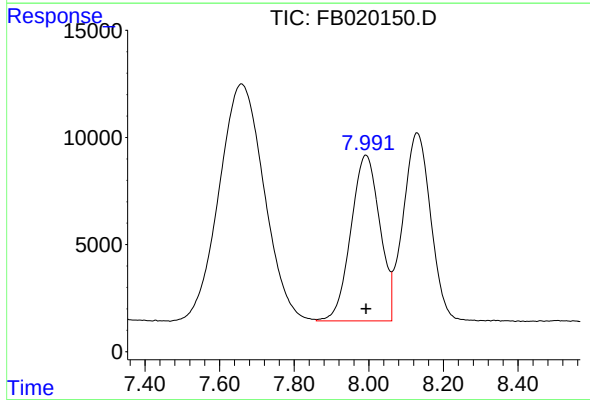


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 417467
Conc: 10.03 ng/ml

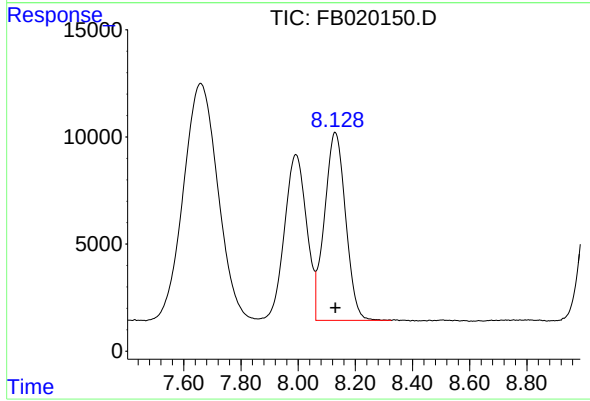

#4 Benzene


R.T.: 8.130 min
Delta R.T.: 0.000 min
Response: 450568
Conc: 9.68 ng/ml

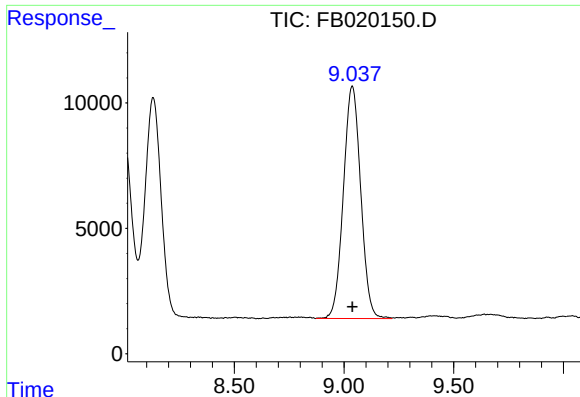

#5 AAA-TFT


R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 508906
Conc: 19.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0312S1

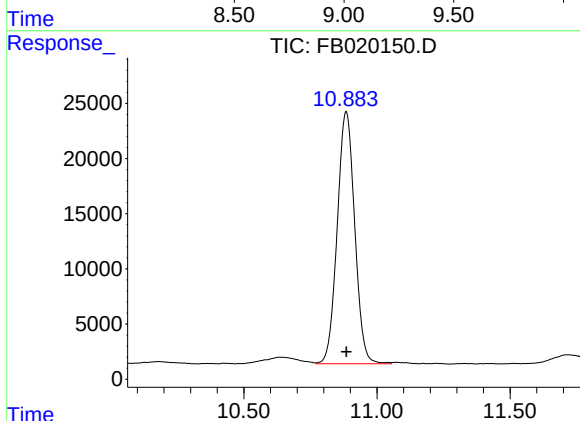


#6 Toluene

R.T.: 10.885 min
Delta R.T.: 0.000 min
Response: 1043968
Conc: 28.25 ng/ml

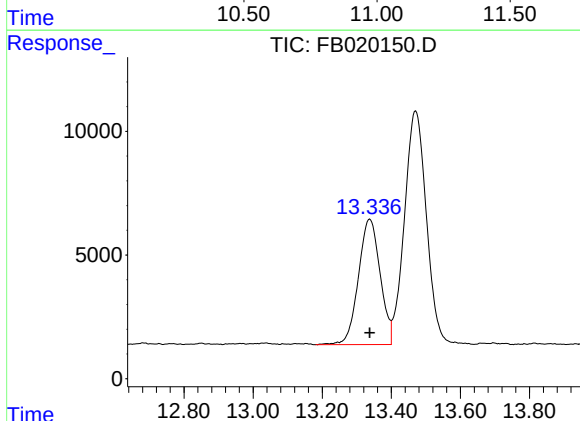


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: 0.000 min
Response: 221251
Conc: 9.40 ng/ml

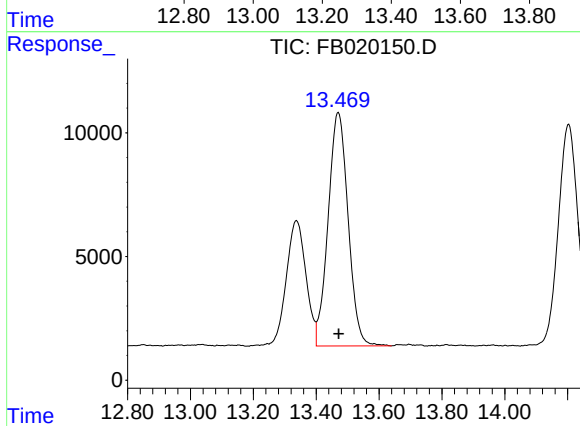

#8 m-Xylene


R.T.: 13.471 min
Delta R.T.: 0.000 min
Response: 417011
Conc: 19.55 ng/ml

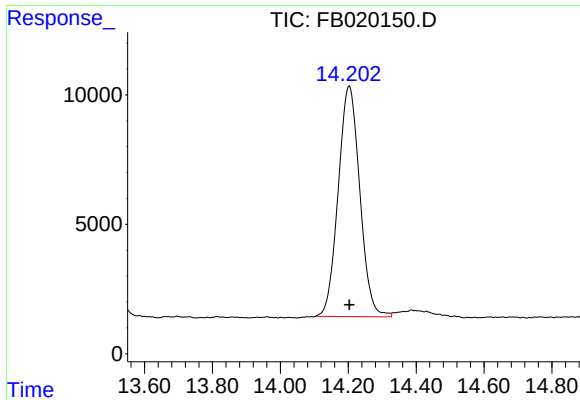

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: 0.000 min
Response: 392955
Conc: 20.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0312S1

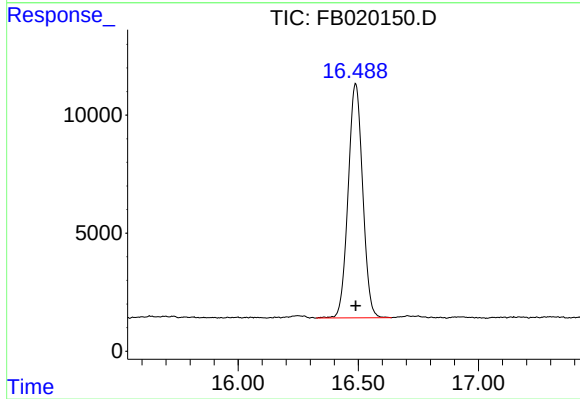

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: 0.000 min
Response: 417562
Conc: 21.06 ng/ml